

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091924\
 Data File : FB030948.D
 Signal(s) : FID2B.CH
 Acq On : 20 Sep 2024 3:13
 Operator : YP/AJ
 Sample : P4103-13 50X
 Misc : 5.03G/5.00 ML MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-14-7.5-10B

Integration File: Calibration.e
 Quant Time: Sep 20 04:12:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
 Quant Title :
 QLast Update : Tue Aug 27 11:54:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	249789	20.645 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	26702	1.494 ng/ml
2) t 2,2,4-Trimethylpentane	7.406	52719	2.875 ng/ml
3) t n-Heptane	7.746	8012	0.433 ng/ml
6) t Toluene	10.616	12204	0.559 ng/ml
7) t Ethylbenzene	13.032	25539	1.220 ng/ml
8) t m-Xylene	13.184	20827	1.004 ng/ml
9) t O-Xylene	13.927	10164	0.504 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091924\
Data File : FB030948.D
Signal(s) : FID2B.CH
Acq On : 20 Sep 2024 3:13
Operator : YP/AJ
Sample : P4103-13 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-14-7.5-10B

Integration File: Calibration.e
Quant Time: Sep 20 04:12:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
Quant Title :
QLast Update : Tue Aug 27 11:54:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

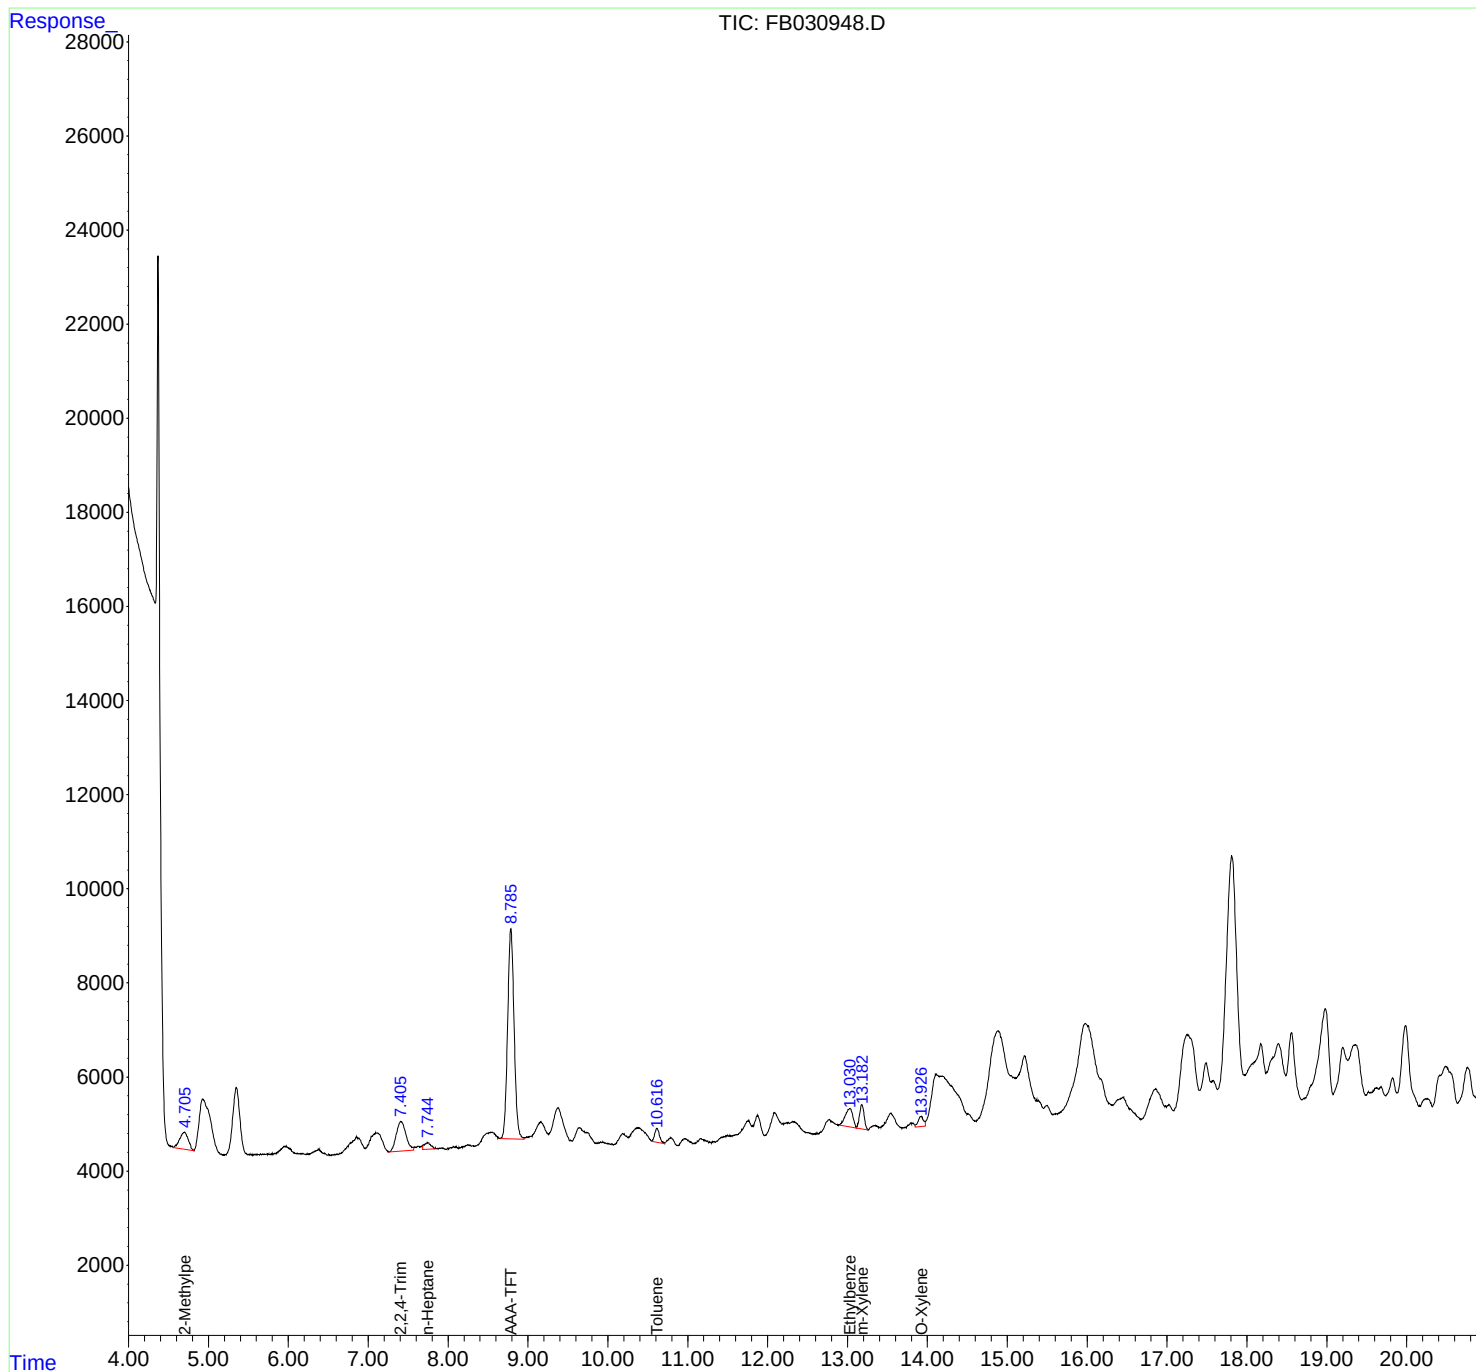


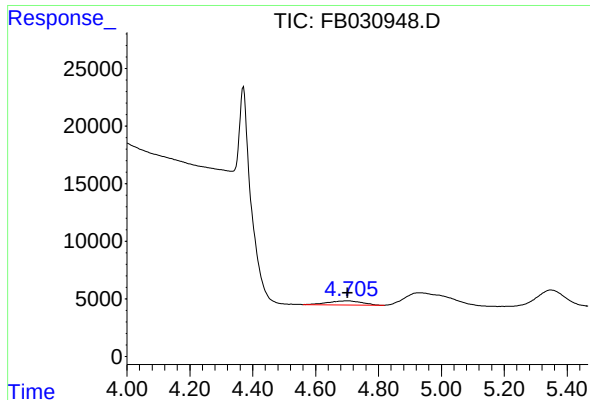

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.004 min
Response: 26702
Conc: 1.49 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14-7.5-10B

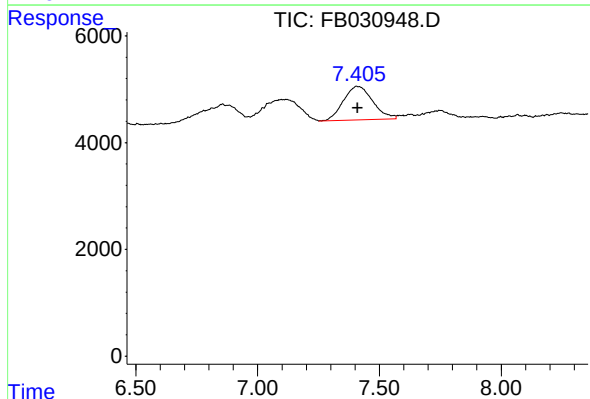


#2 2,2,4-Trimethylpentane

R.T.: 7.406 min
Delta R.T.: -0.005 min
Response: 52719
Conc: 2.88 ng/ml

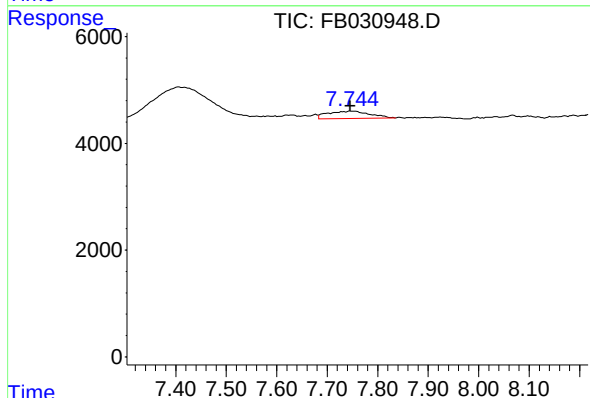


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: 0.000 min
Response: 8012
Conc: 0.43 ng/ml

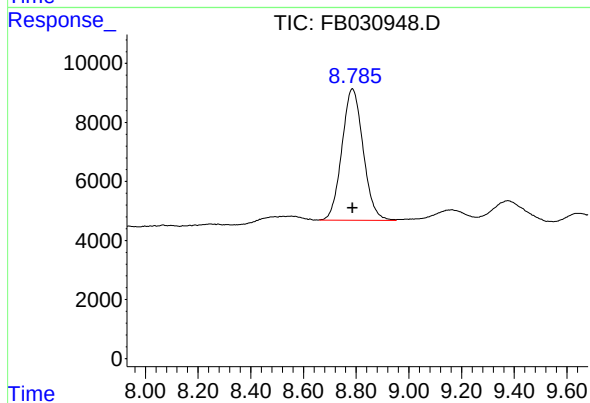

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 249789
Conc: 20.65 ng/ml

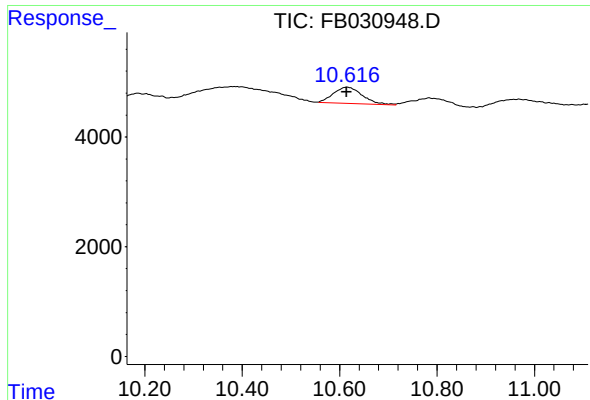

#6 Toluene


R.T.: 10.616 min
Delta R.T.: 0.002 min
Response: 12204
Conc: 0.56 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-14-7.5-10B

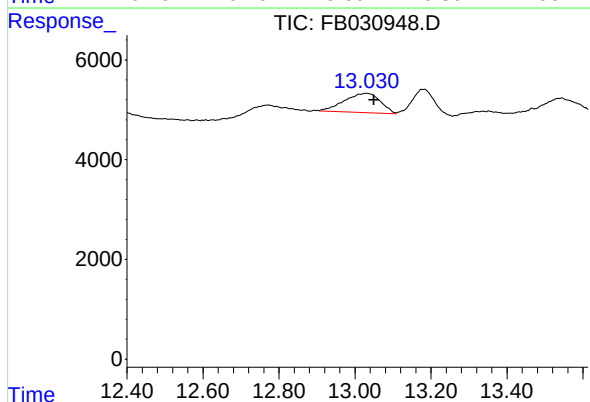


#7 Ethylbenzene

R.T.: 13.032 min
Delta R.T.: -0.018 min
Response: 25539
Conc: 1.22 ng/ml

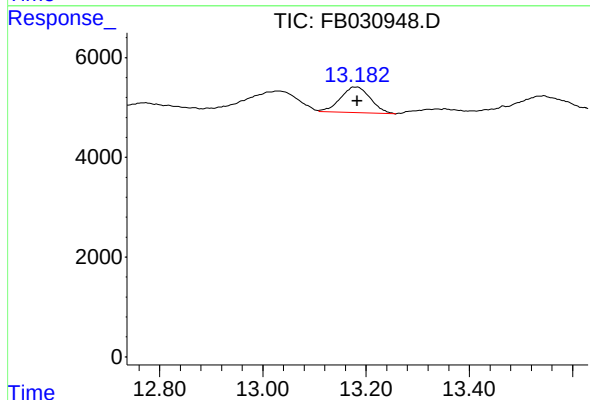

#8 m-Xylene

R.T.: 13.184 min
Delta R.T.: 0.001 min
Response: 20827
Conc: 1.00 ng/ml

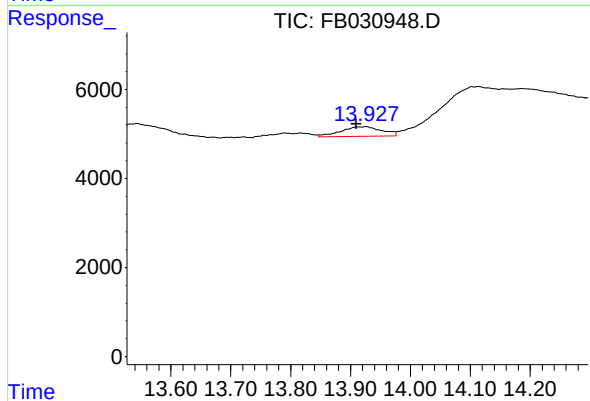

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.018 min
Response: 10164
Conc: 0.50 ng/ml