

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091924\
 Data File : FB030951.D
 Signal(s) : FID2B.CH
 Acq On : 20 Sep 2024 5:09
 Operator : YP/AJ
 Sample : P4103-16MSD 50X
 Misc : 5.02G/5.00 ML MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-23MSD

Integration File: Calibration.e
 Quant Time: Sep 20 05:59:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
 Quant Title :
 QLast Update : Tue Aug 27 11:54:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	346917	28.673 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	563367	31.527 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	1229581	67.062 ng/ml
3) t n-Heptane	7.743	374097	20.228 ng/ml
4) t Benzene	7.879	214219	9.482 ng/ml
6) t Toluene	10.614	632714	28.969 ng/ml
7) t Ethylbenzene	13.049	544873	26.028 ng/ml
8) t m-Xylene	13.180	1164485	56.123 ng/ml
9) t O-Xylene	13.910	487508	24.189 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	1376917	69.005 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB091924\
Data File : FB030951.D
Signal(s) : FID2B.CH
Acq On : 20 Sep 2024 5:09
Operator : YP/AJ
Sample : P4103-16MSD 50X
Misc : 5.02G/5.00 ML MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-23MSD

Integration File: Calibration.e
Quant Time: Sep 20 05:59:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
Quant Title :
QLast Update : Tue Aug 27 11:54:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

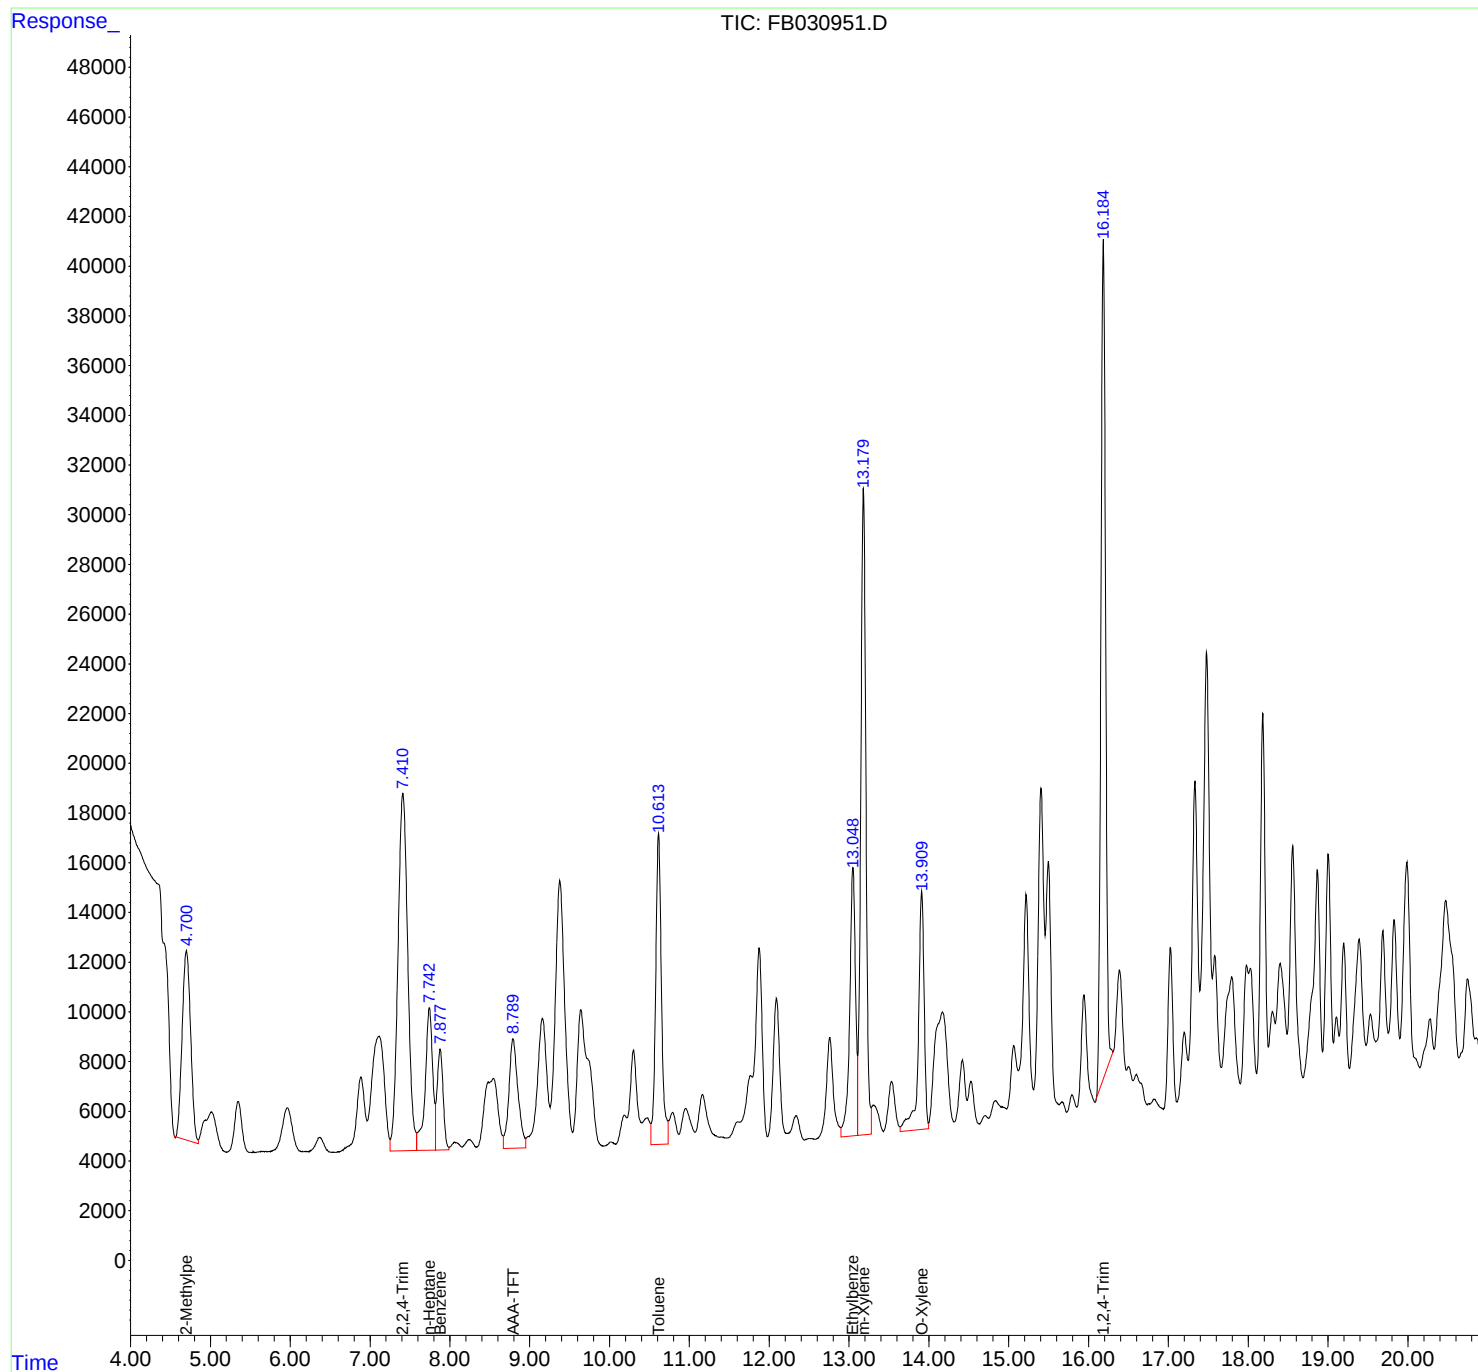


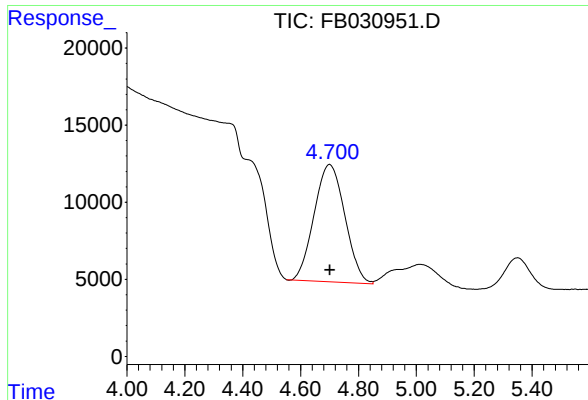

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 563367
Conc: 31.53 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-23MSD

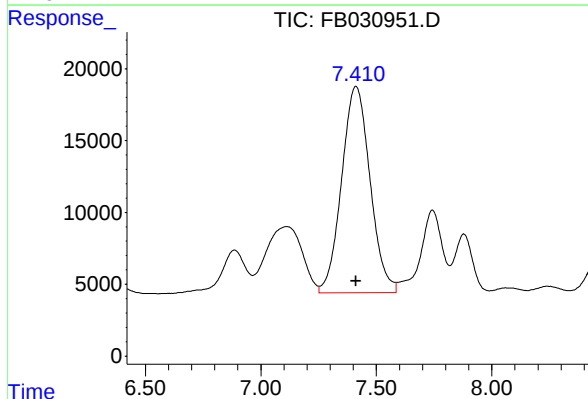


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.000 min
Response: 1229581
Conc: 67.06 ng/ml

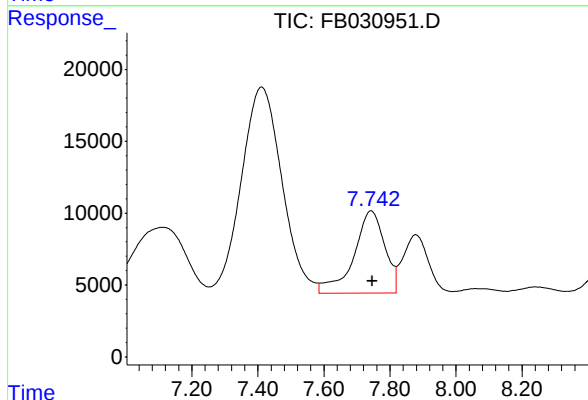


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.003 min
Response: 374097
Conc: 20.23 ng/ml

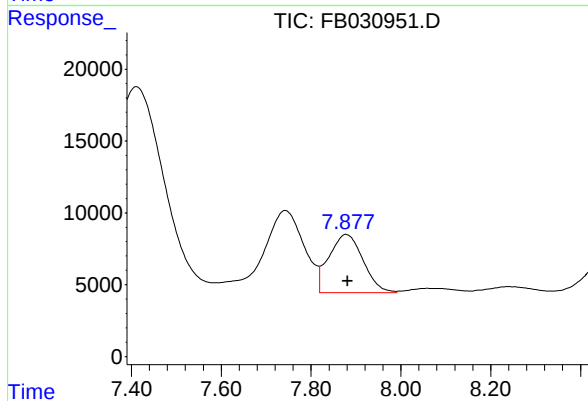

#4 Benzene


R.T.: 7.879 min
Delta R.T.: -0.003 min
Response: 214219
Conc: 9.48 ng/ml

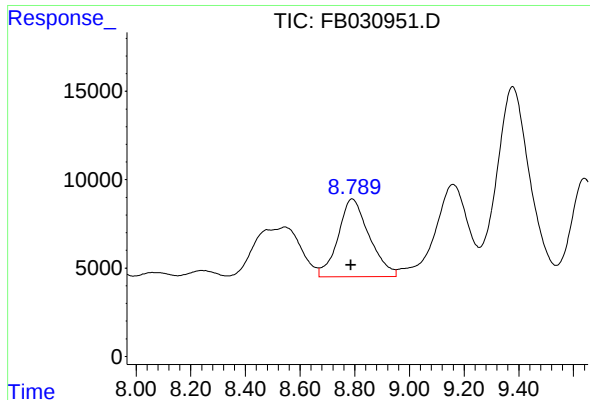

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.004 min
Response: 346917
Conc: 28.67 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-23MSD

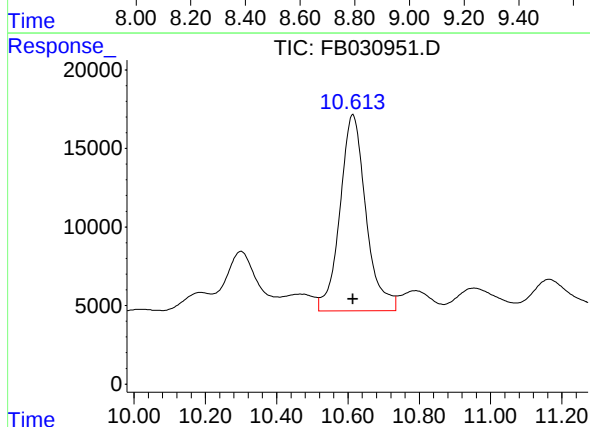


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.000 min
Response: 632714
Conc: 28.97 ng/ml

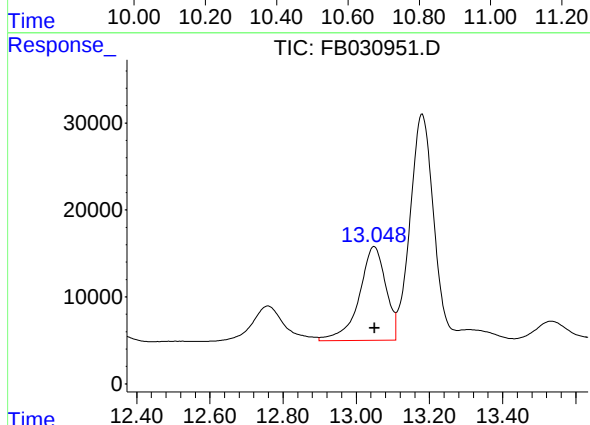


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.001 min
Response: 544873
Conc: 26.03 ng/ml

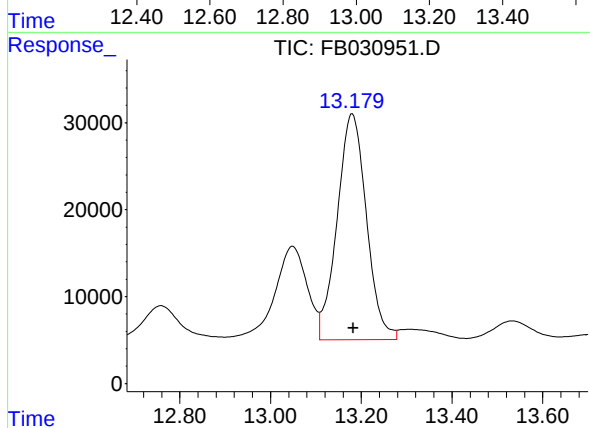

#8 m-Xylene


R.T.: 13.180 min
Delta R.T.: -0.002 min
Response: 1164485
Conc: 56.12 ng/ml

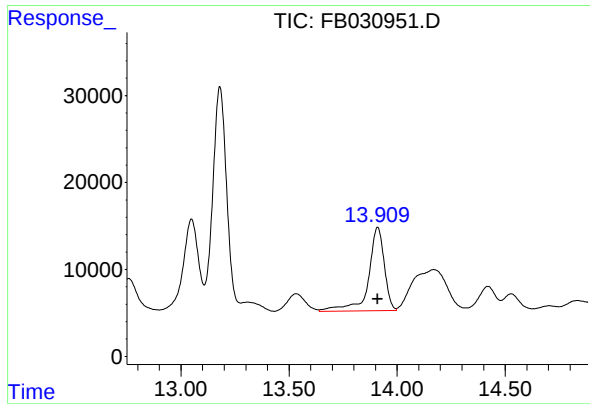

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: 0.000 min
Response: 487508
Conc: 24.19 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-23MSD

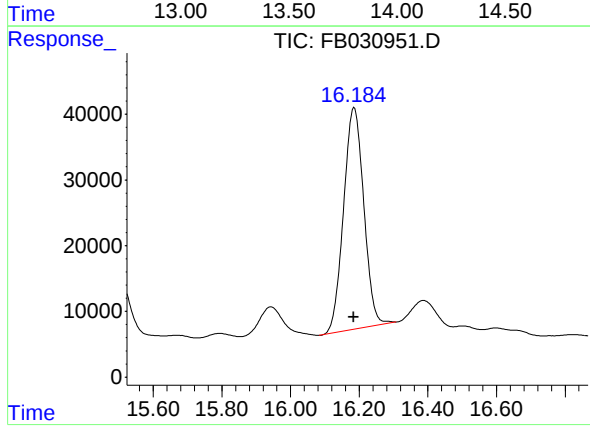

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: 0.001 min
Response: 1376917
Conc: 69.01 ng/ml