

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092018\
 Data File : FB017817.D
 Signal(s) : FID2B.CH
 Acq On : 20 Sep 2018 9:22
 Operator : MJ/SJ
 Sample : BSF0920S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 20 14:01:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.106	180157	21.298 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.958	463282	29.091 ng/ml
2) t 2,2,4-Trimethylpentane	7.723	468586	29.446 ng/ml
3) t n-Heptane	8.062	151916	9.858 ng/ml
4) t Benzene	8.201	189093	9.933 ng/ml
6) t Toluene	10.955	464554	29.354 ng/ml
7) t Ethylbenzene	13.405	163257	9.991 ng/ml
8) t m-Xylene	13.537	344542	19.916 ng/ml
9) t O-Xylene	14.269	379782	20.899 ng/ml
10) t 1,2,4-Trimethylbenzene	16.551	412287	19.382 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092018\
Data File : FB017817.D
Signal(s) : FID2B.CH
Acq On : 20 Sep 2018 9:22
Operator : MJ/SJ
Sample : BSF0920S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 20 14:01:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

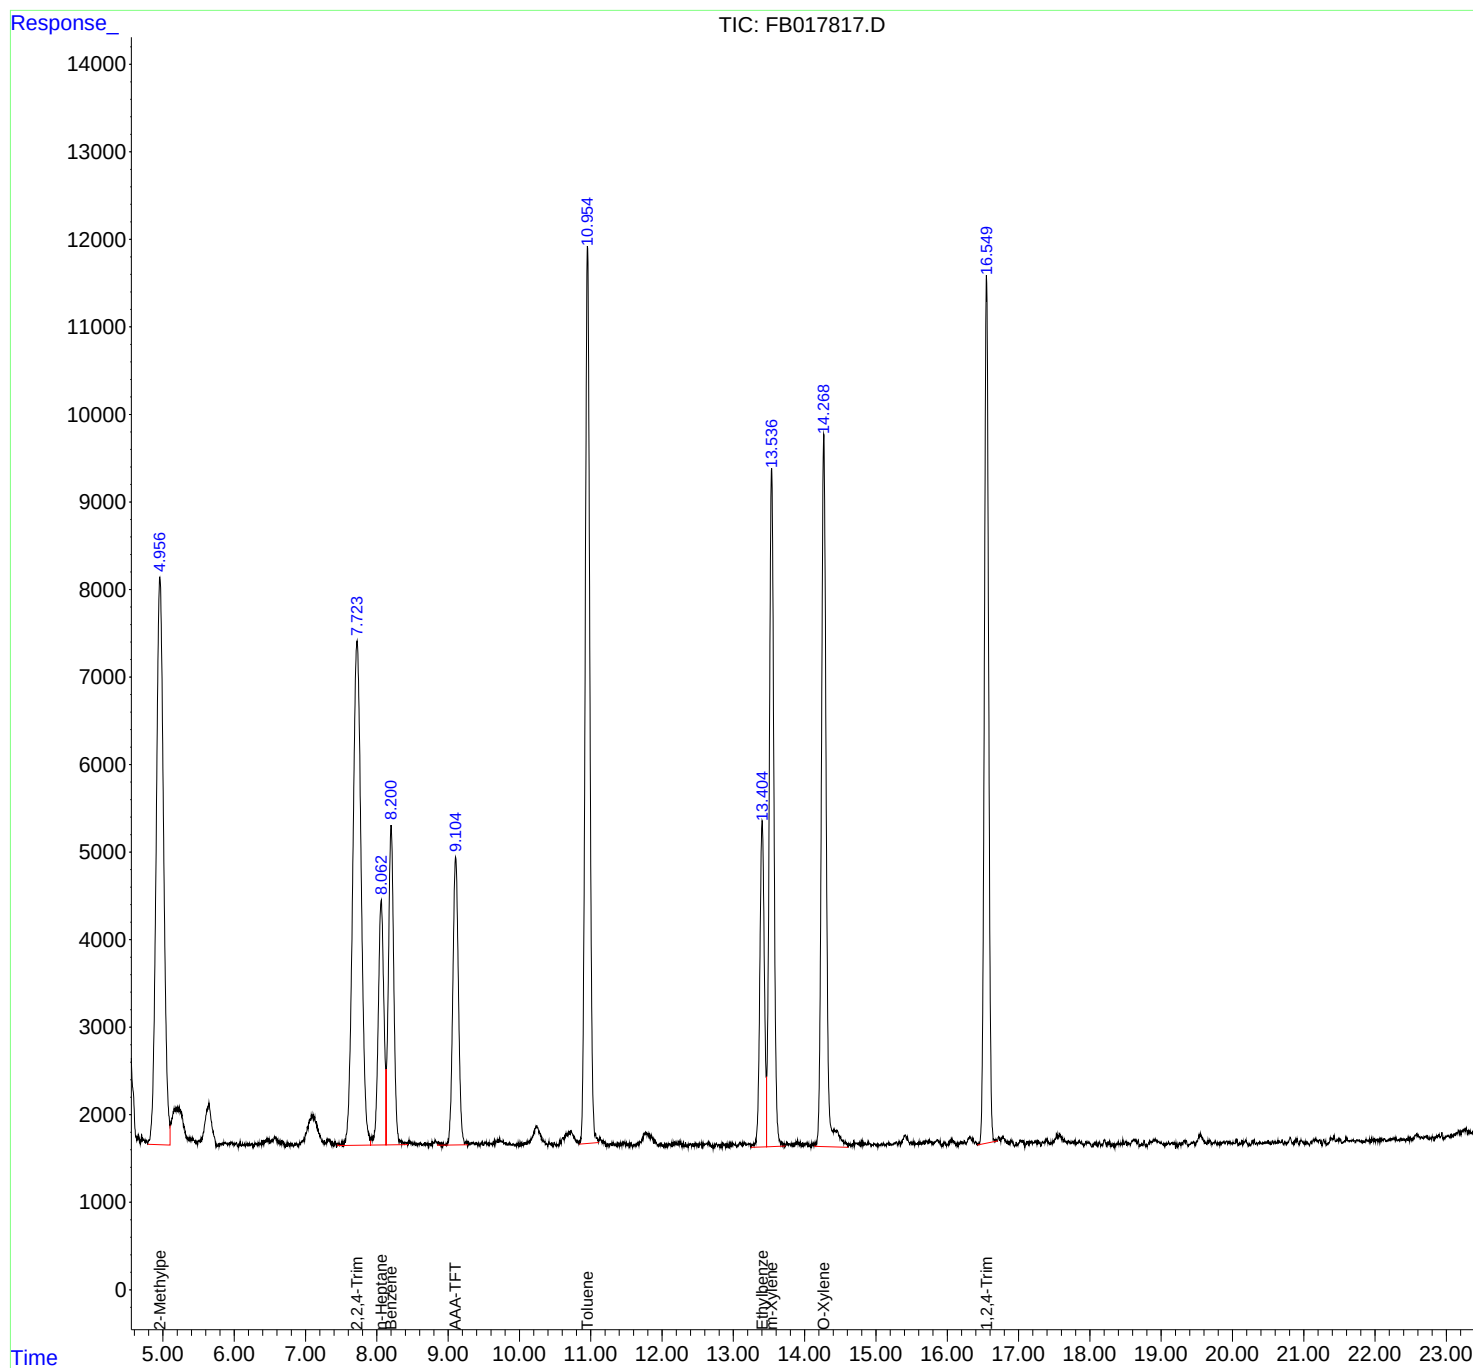

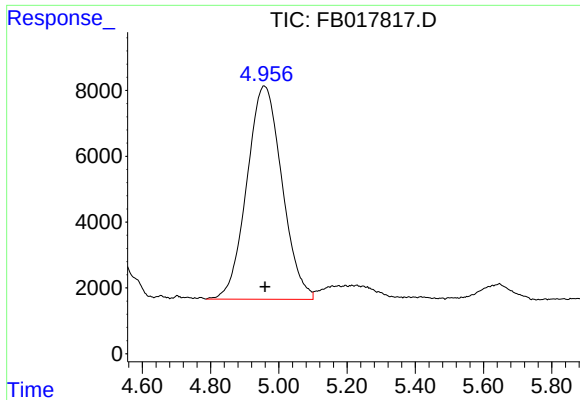


#1 2-Methylpentane

R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 463282
Conc: 29.09 ng/ml

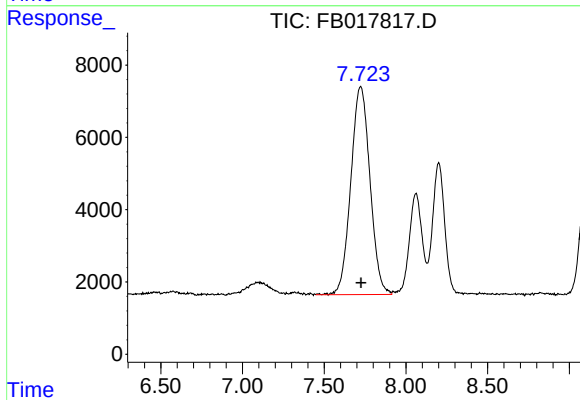


#2 2,2,4-Trimethylpentane

R.T.: 7.723 min
Delta R.T.: -0.004 min
Response: 468586
Conc: 29.45 ng/ml

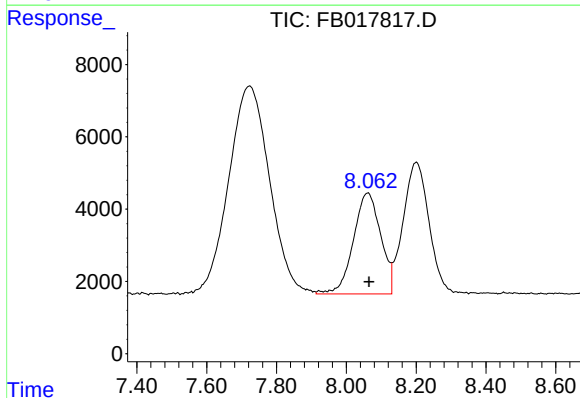


#3 n-Heptane

R.T.: 8.062 min
Delta R.T.: -0.004 min
Response: 151916
Conc: 9.86 ng/ml

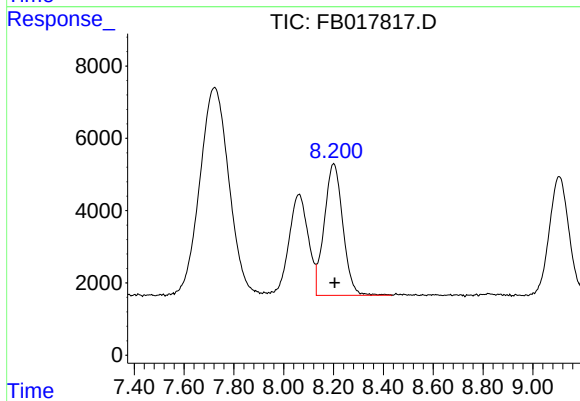


#4 Benzene

R.T.: 8.201 min
Delta R.T.: -0.004 min
Response: 189093
Conc: 9.93 ng/ml

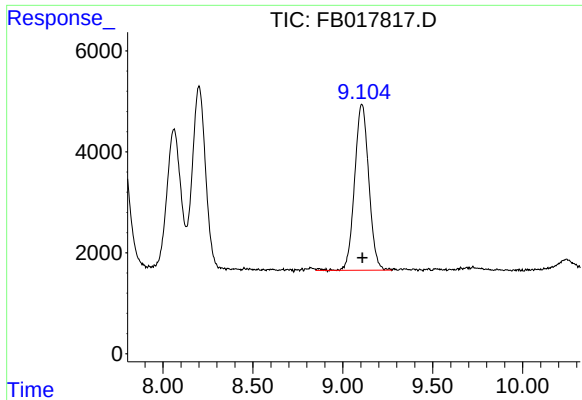


#5 AAA-TFT

R.T.: 9.106 min
Delta R.T.: -0.004 min
Response: 180157
Conc: 21.30 ng/ml

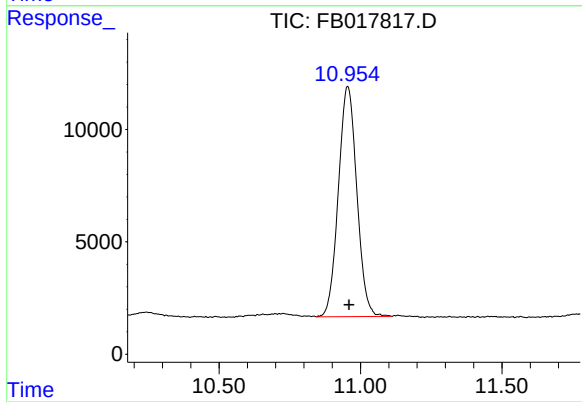


#6 Toluene

R.T.: 10.955 min
Delta R.T.: -0.004 min
Response: 464554
Conc: 29.35 ng/ml

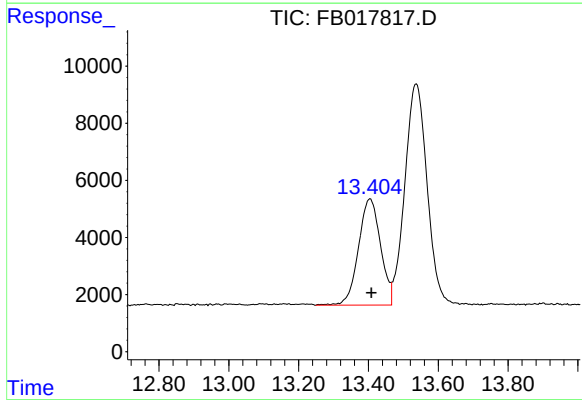


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: -0.004 min
Response: 163257
Conc: 9.99 ng/ml

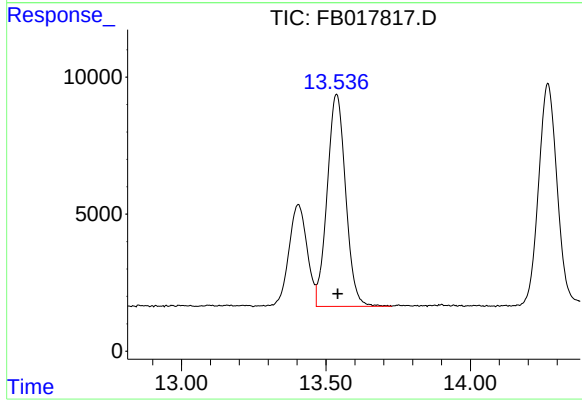


#8 m-Xylene

R.T.: 13.537 min
Delta R.T.: -0.004 min
Response: 344542
Conc: 19.92 ng/ml

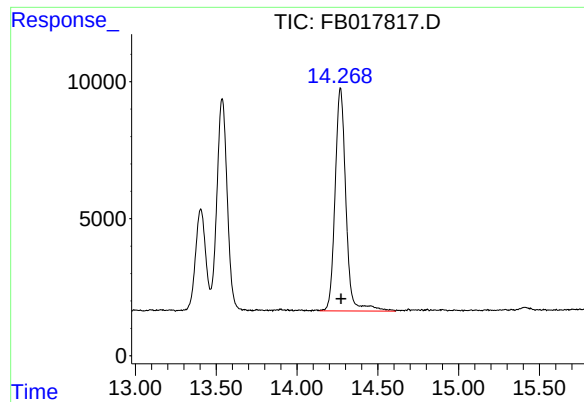

#9 O-Xylene

R.T.: 14.269 min
Delta R.T.: -0.004 min
Response: 379782
Conc: 20.90 ng/ml

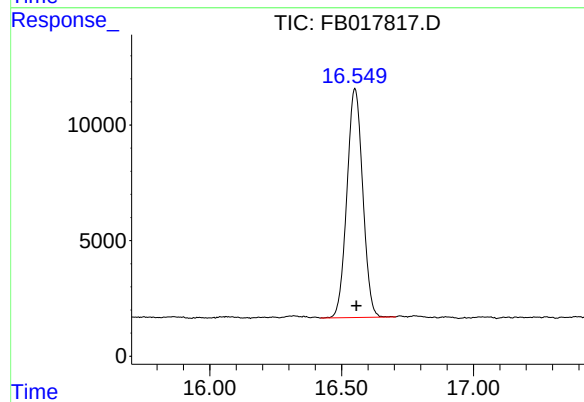

#10 1,2,4-Trimethylbenzene

R.T.: 16.551 min
Delta R.T.: -0.004 min
Response: 412287
Conc: 19.38 ng/ml