

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092018\
 Data File : FB017820.D
 Signal(s) : FID2B.CH
 Acq On : 20 Sep 2018 11:20
 Operator : MJ/SJ
 Sample : J5001-03MSD
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 20 14:01:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.107	180310	21.316 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	437201	27.453 ng/ml
2) t 2,2,4-Trimethylpentane	7.723	425099	26.713 ng/ml
3) t n-Heptane	8.062	132392	8.591 ng/ml
4) t Benzene	8.201	180798	9.497 ng/ml
6) t Toluene	10.955	477160	30.150 ng/ml
7) t Ethylbenzene	13.405	167494	10.251 ng/ml
8) t m-Xylene	13.537	357390	20.658 ng/ml
9) t O-Xylene	14.269	379427	20.880 ng/ml
10) t 1,2,4-Trimethylbenzene	16.552	418877	19.692 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092018\
Data File : FB017820.D
Signal(s) : FID2B.CH
Acq On : 20 Sep 2018 11:20
Operator : MJ/SJ
Sample : J5001-03MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 20 14:01:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

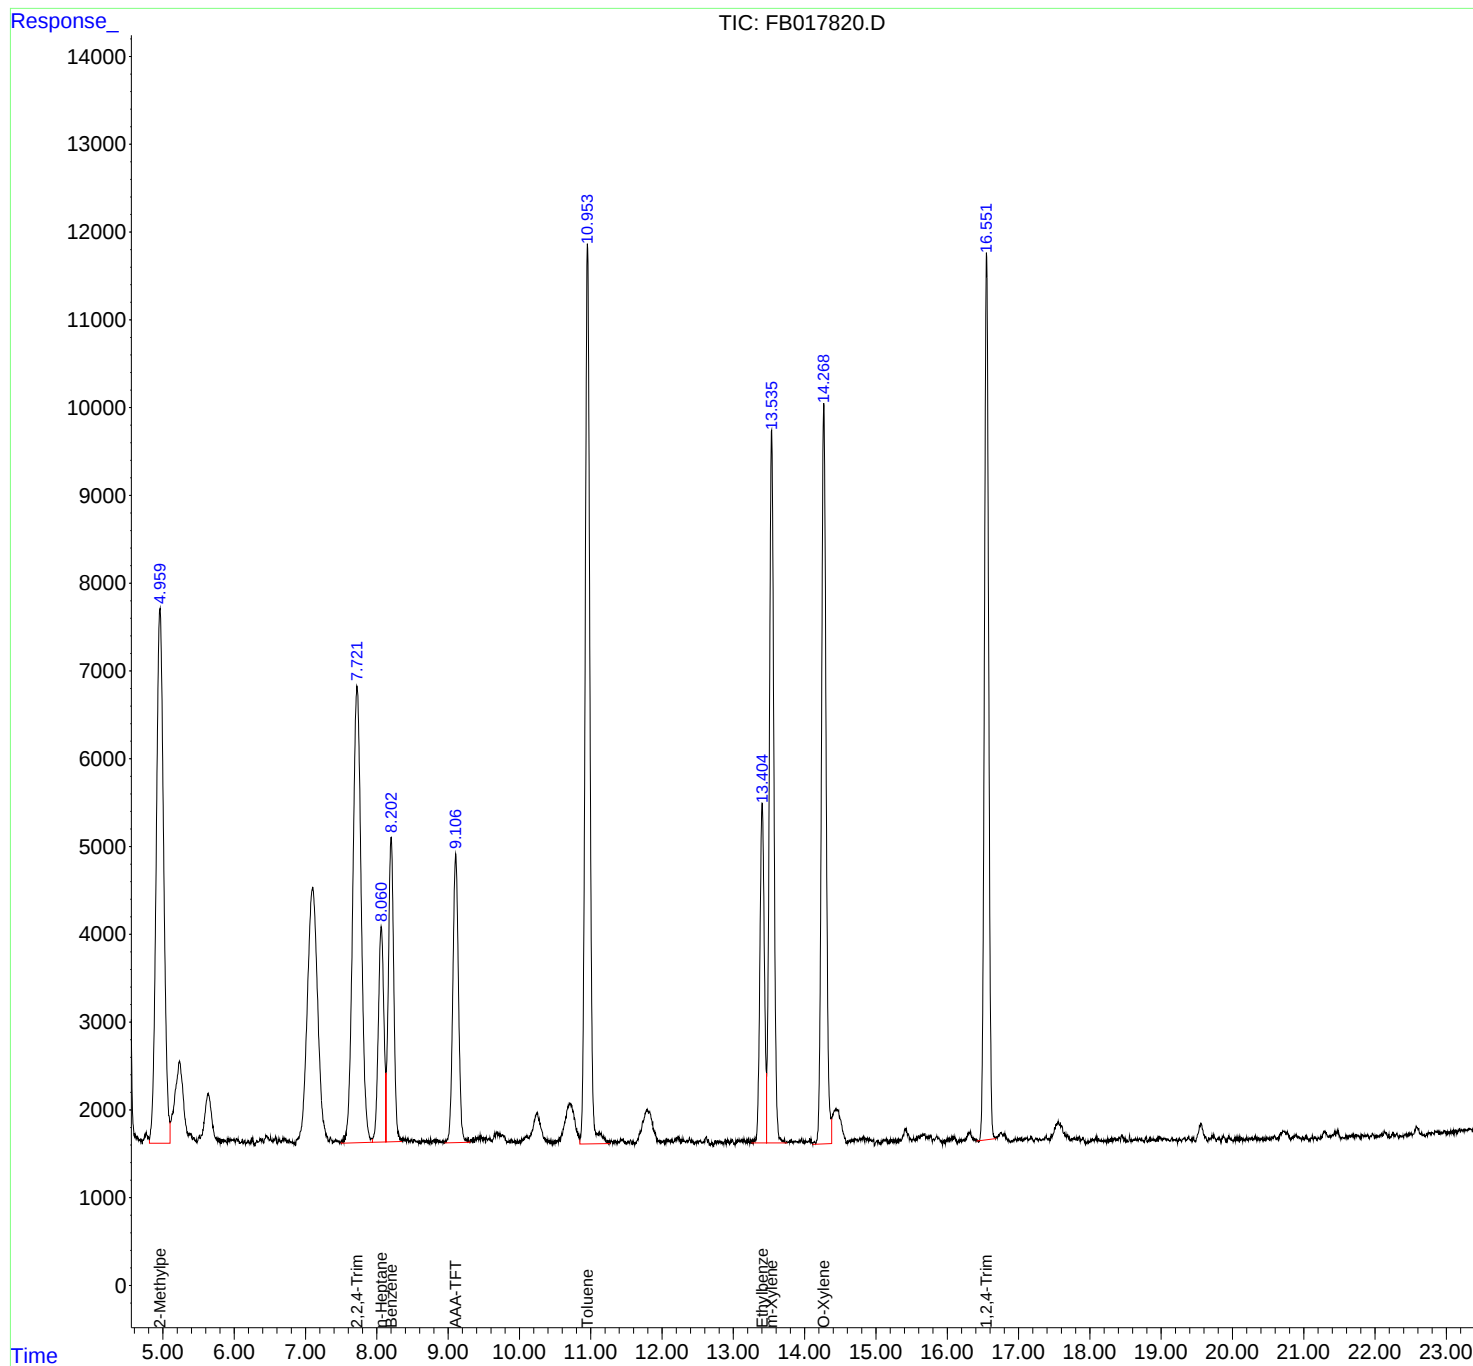

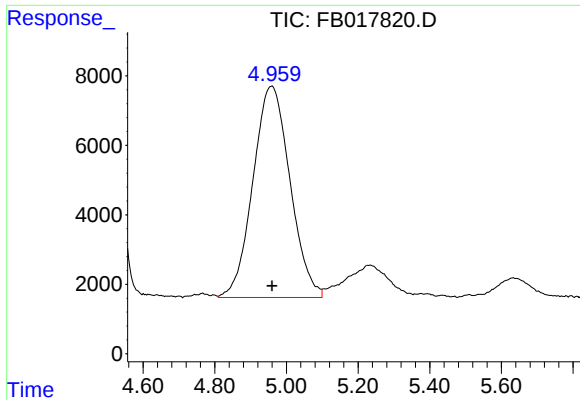


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 437201
Conc: 27.45 ng/ml

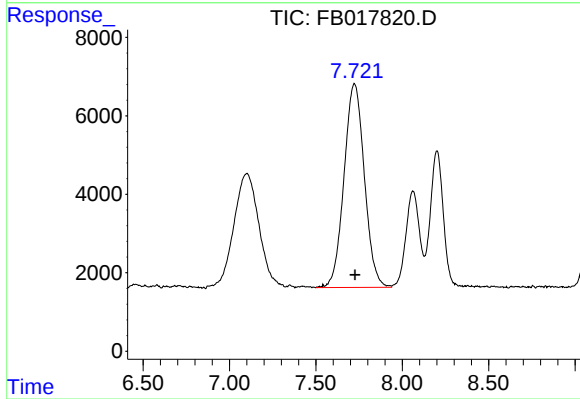


#2 2,2,4-Trimethylpentane

R.T.: 7.723 min
Delta R.T.: -0.004 min
Response: 425099
Conc: 26.71 ng/ml

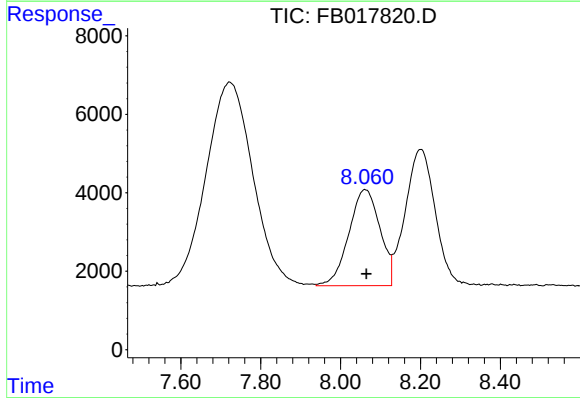


#3 n-Heptane

R.T.: 8.062 min
Delta R.T.: -0.003 min
Response: 132392
Conc: 8.59 ng/ml

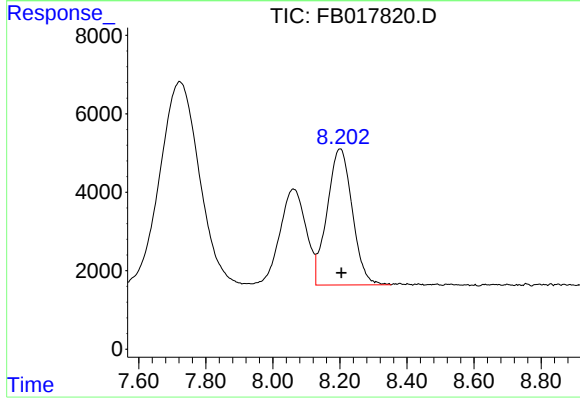


#4 Benzene

R.T.: 8.201 min
Delta R.T.: -0.003 min
Response: 180798
Conc: 9.50 ng/ml

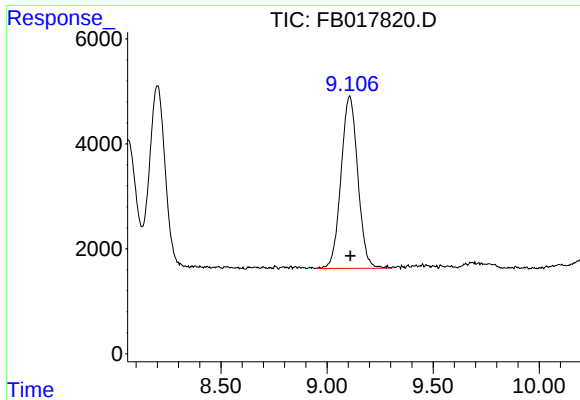


#5 AAA-TFT

R.T.: 9.107 min
Delta R.T.: -0.003 min
Response: 180310
Conc: 21.32 ng/ml

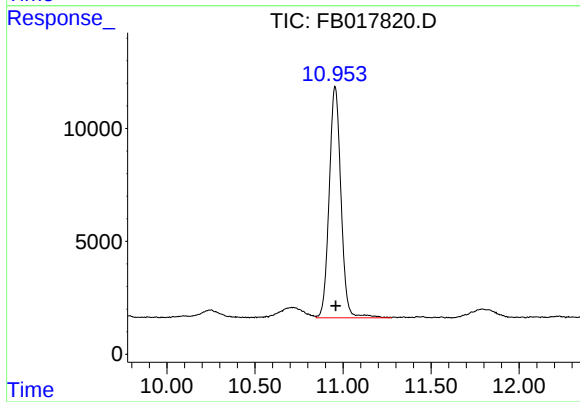


#6 Toluene

R.T.: 10.955 min
Delta R.T.: -0.004 min
Response: 477160
Conc: 30.15 ng/ml

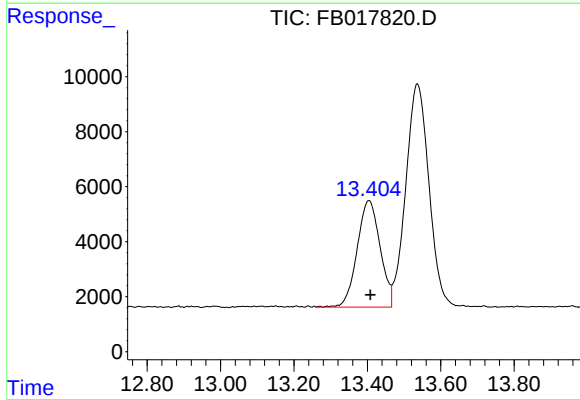


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: -0.004 min
Response: 167494
Conc: 10.25 ng/ml

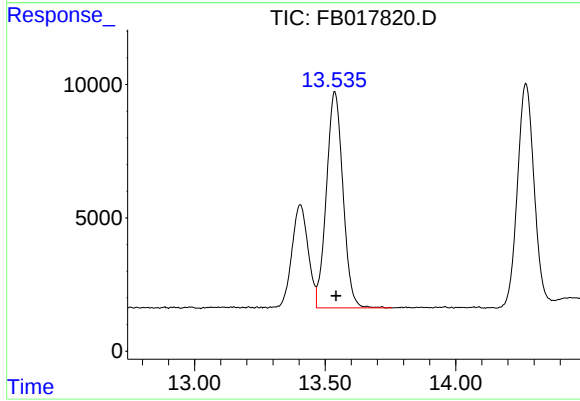


#8 m-Xylene

R.T.: 13.537 min
Delta R.T.: -0.004 min
Response: 357390
Conc: 20.66 ng/ml

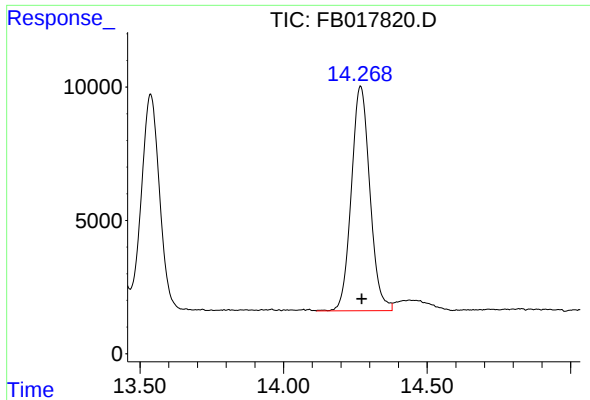

#9 O-Xylene

R.T.: 14.269 min
Delta R.T.: -0.004 min
Response: 379427
Conc: 20.88 ng/ml

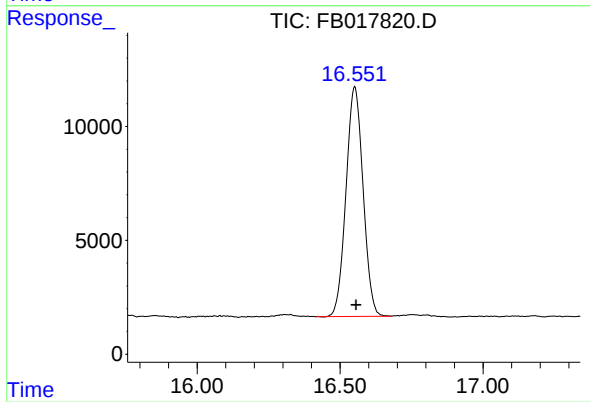

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: -0.004 min
Response: 418877
Conc: 19.69 ng/ml