

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092022\
 Data File : FB028319.D
 Signal(s) : FID2B.CH
 Acq On : 20 Sep 2022 11:28
 Operator : AJ/MA
 Sample : BSF0920S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0920S1

Integration File: Calibration.e
 Quant Time: Sep 21 05:50:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	270533	22.603 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.724	515538	25.462 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	582756	27.703 ng/ml
3) t n-Heptane	7.760	176335	8.203 ng/ml
4) t Benzene	7.897	223962	9.104 ng/ml
6) t Toluene	10.630	636412	27.336 ng/ml
7) t Ethylbenzene	13.066	205604	9.245 ng/ml
8) t m-Xylene	13.199	405601	18.586 ng/ml
9) t O-Xylene	13.926	392234	18.721 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	385360	19.165 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092022\
Data File : FB028319.D
Signal(s) : FID2B.CH
Acq On : 20 Sep 2022 11:28
Operator : AJ/MA
Sample : BSF0920S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0920S1

Integration File: Calibration.e
Quant Time: Sep 21 05:50:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

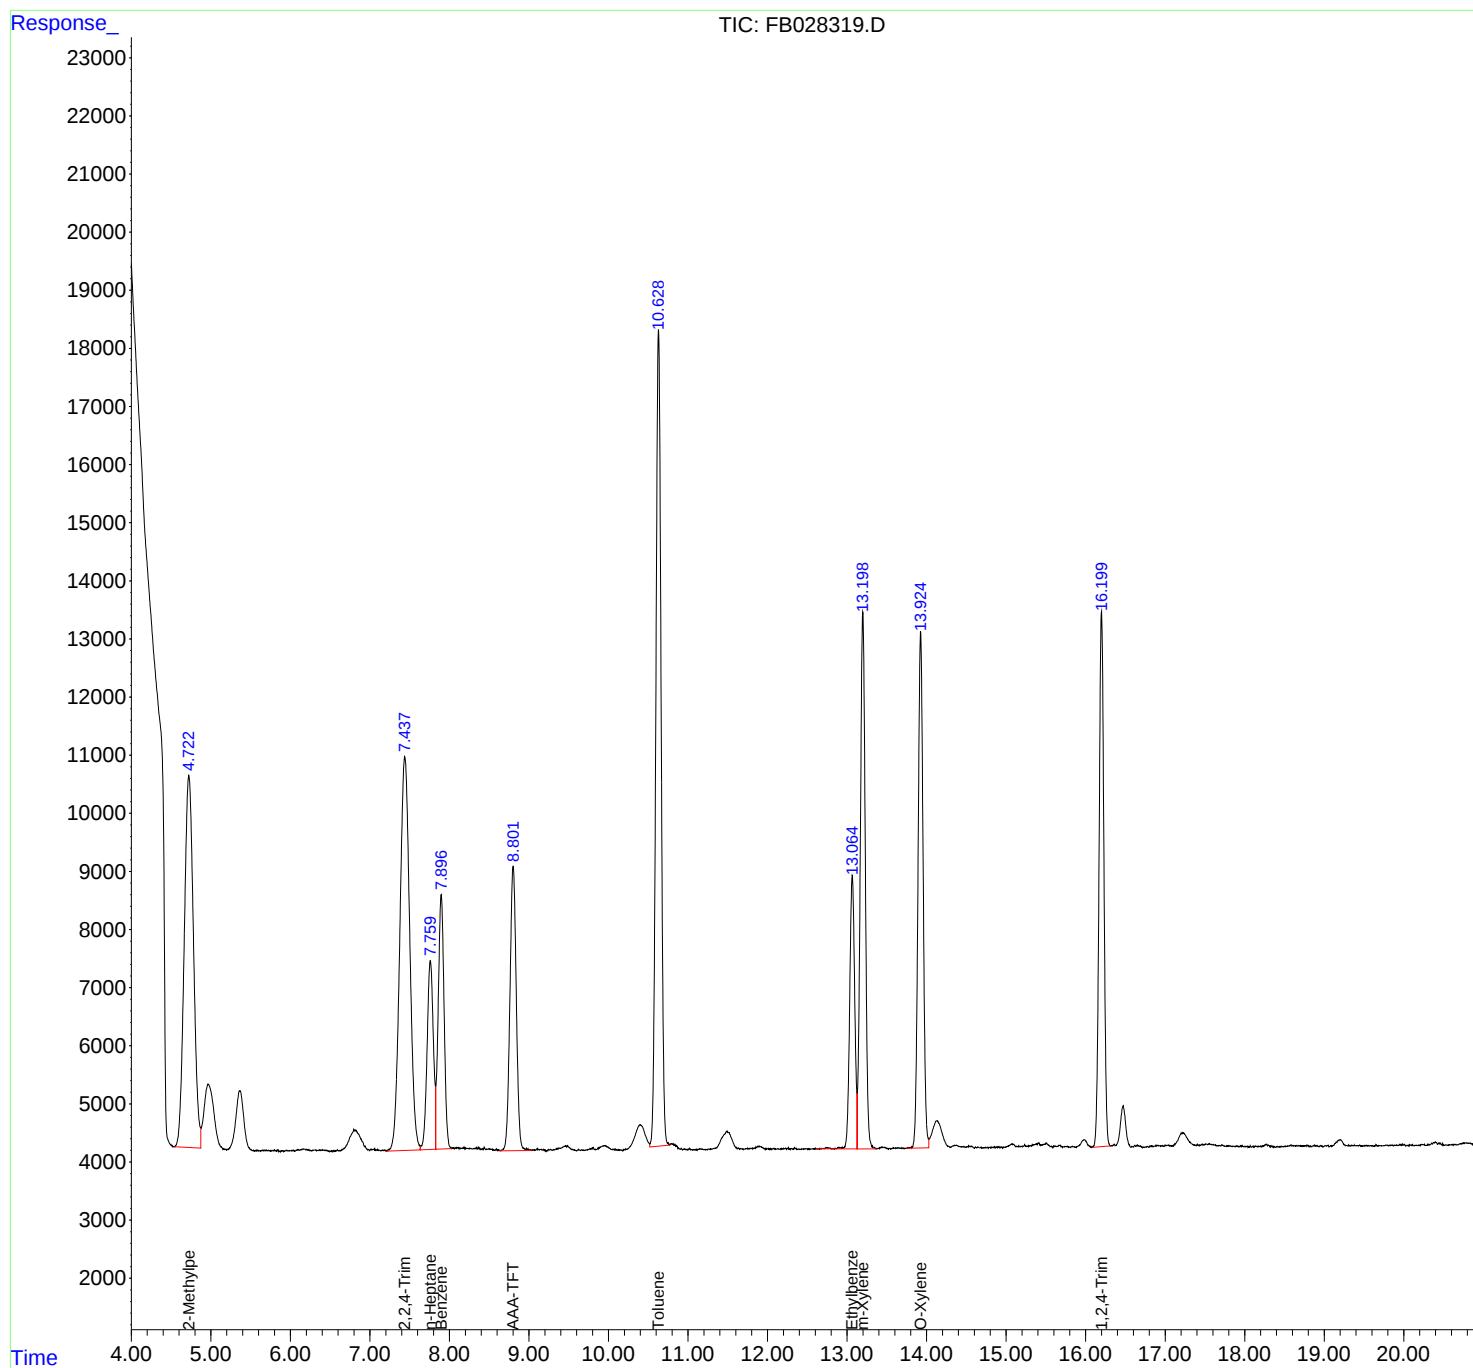


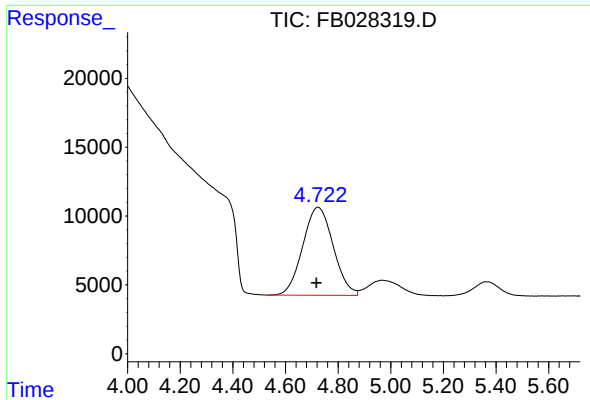

#1 2-Methylpentane


R.T.: 4.724 min
Delta R.T.: 0.006 min
Response: 515538
Conc: 25.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0920S1

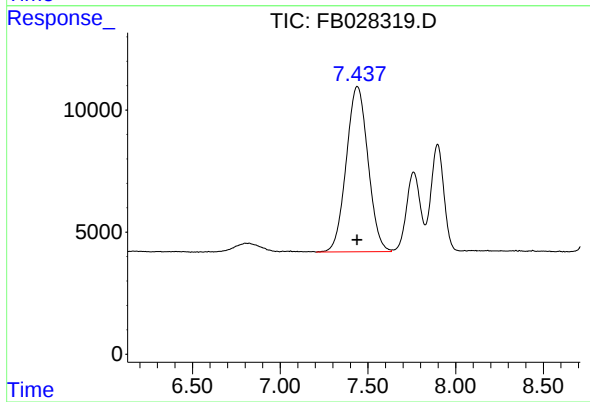


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: 0.002 min
Response: 582756
Conc: 27.70 ng/ml

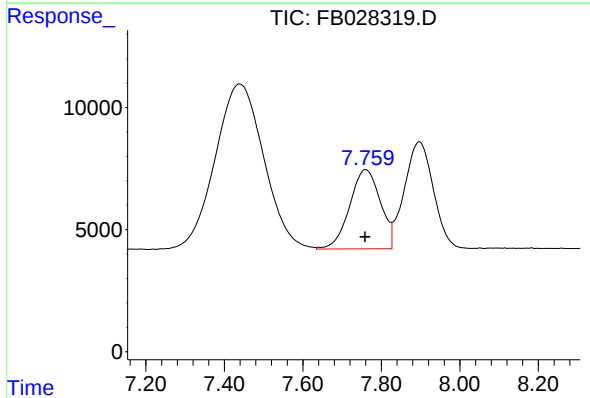


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.002 min
Response: 176335
Conc: 8.20 ng/ml

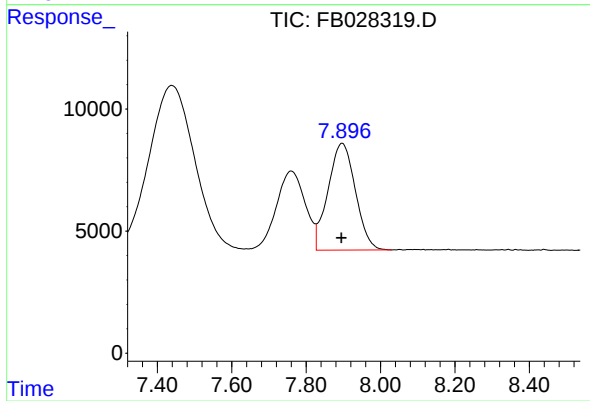

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.003 min
Response: 223962
Conc: 9.10 ng/ml

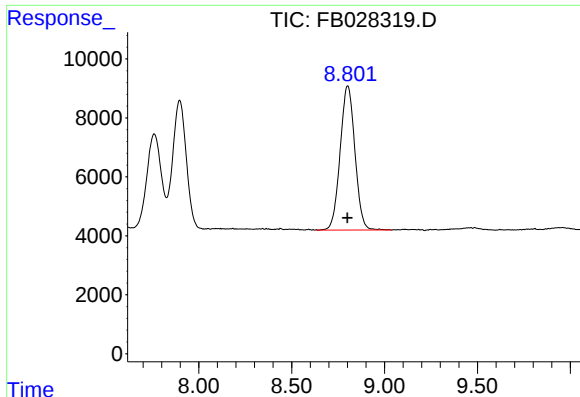

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 270533
Conc: 22.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0920S1

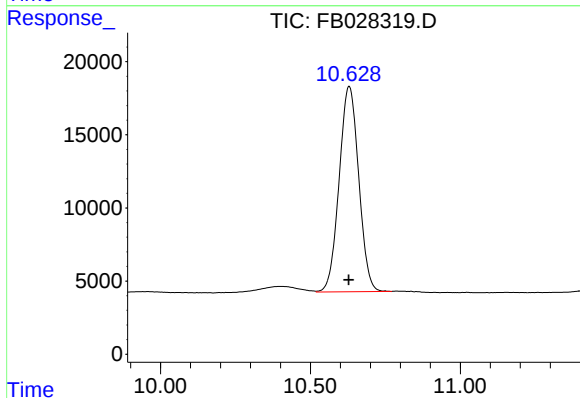


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.002 min
Response: 636412
Conc: 27.34 ng/ml

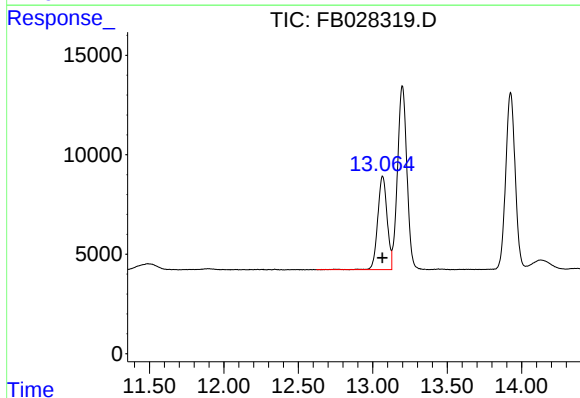


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.002 min
Response: 205604
Conc: 9.25 ng/ml

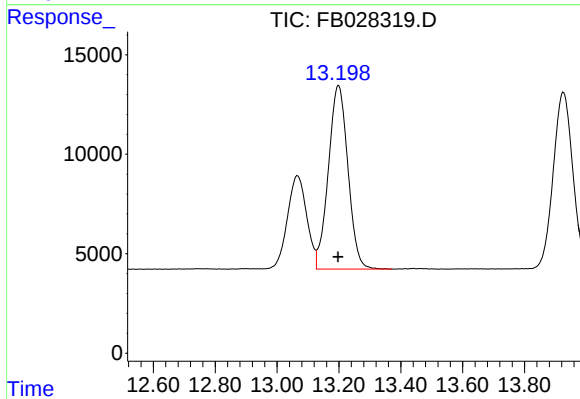

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: 0.001 min
Response: 405601
Conc: 18.59 ng/ml

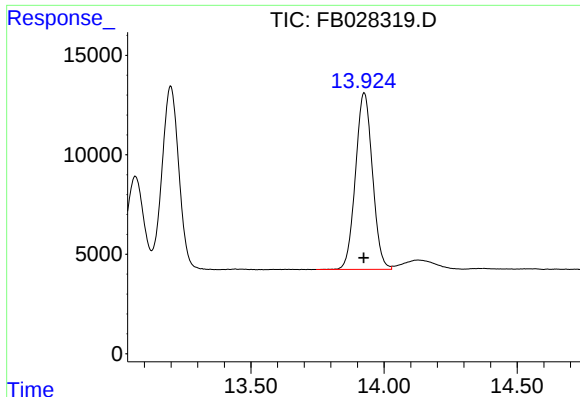

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.002 min
Response: 392234
Conc: 18.72 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0920S1

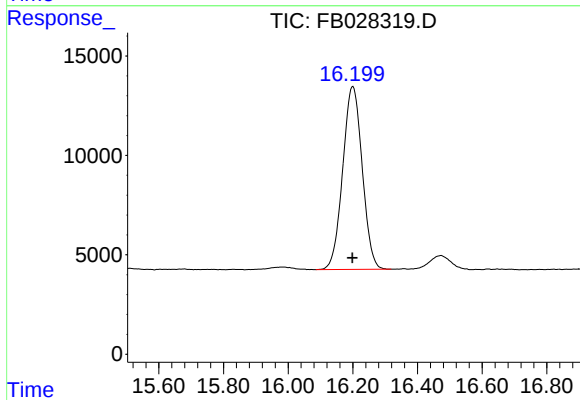

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.001 min
Response: 385360
Conc: 19.17 ng/ml