

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092022\
 Data File : FB028327.D
 Signal(s) : FID2B.CH
 Acq On : 20 Sep 2022 17:06
 Operator : AJ/MA
 Sample : N4702-01MS 50X
 Misc : 5.09G/5.00 ML MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-03-091622MS

Integration File: Calibration.e
 Quant Time: Sep 21 05:51:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	306679	25.623 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	418400	20.665 ng/ml
2) t 2,2,4-Trimethylpentane	7.441	526680	25.037 ng/ml
3) t n-Heptane	7.759	168217	7.825 ng/ml
4) t Benzene	7.896	239740	9.745 ng/ml
6) t Toluene	10.631	664981	28.563 ng/ml
7) t Ethylbenzene	13.067	210474	9.464 ng/ml
8) t m-Xylene	13.200	409270	18.754 ng/ml
9) t O-Xylene	13.927	391078	18.665 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	353722	17.592 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092022\
Data File : FB028327.D
Signal(s) : FID2B.CH
Acq On : 20 Sep 2022 17:06
Operator : AJ/MA
Sample : N4702-01MS 50X
Misc : 5.09G/5.00 ML MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-03-091622MS

Integration File: Calibration.e
Quant Time: Sep 21 05:51:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

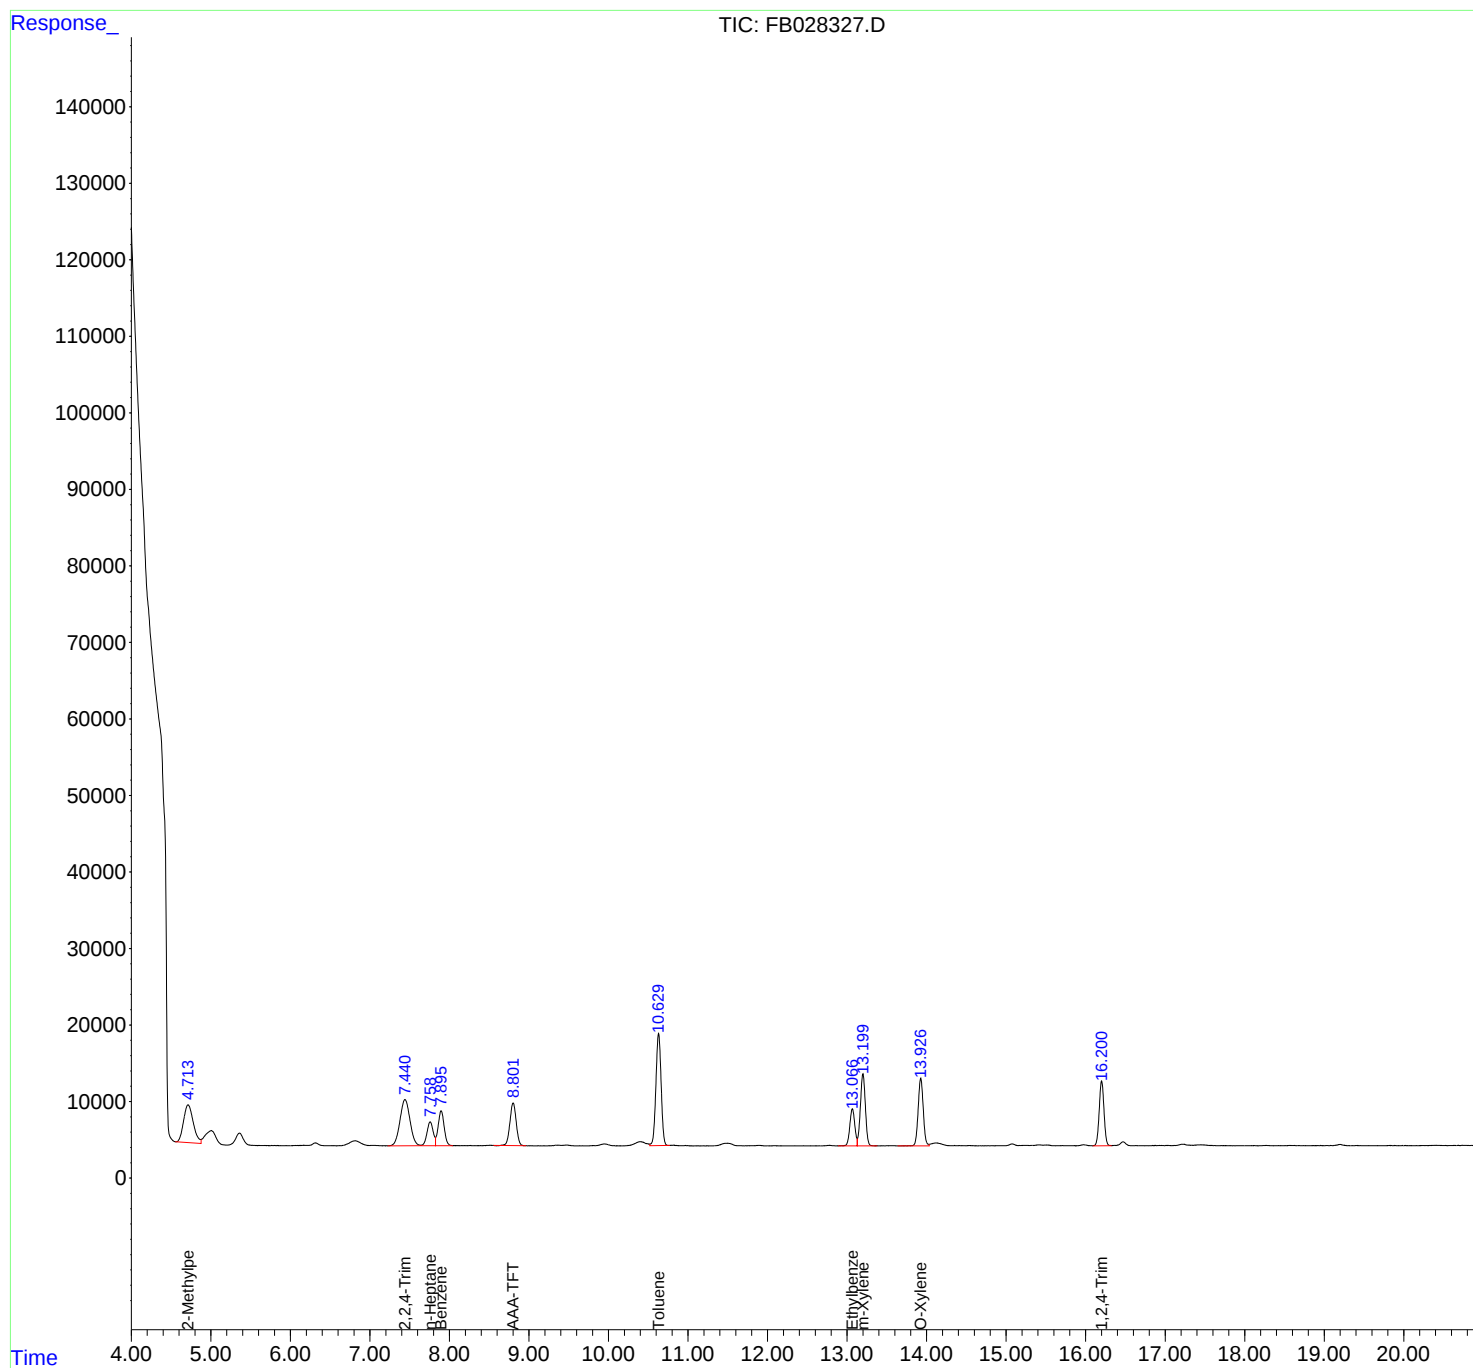


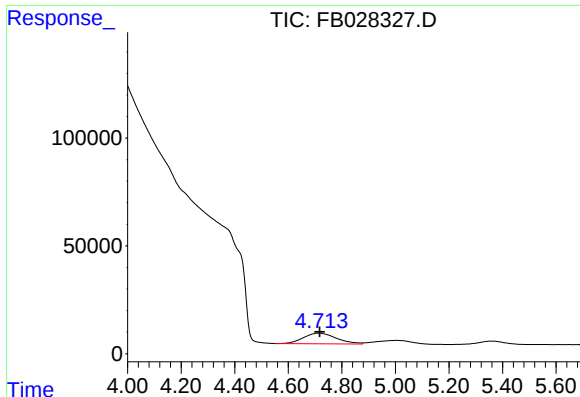

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: -0.003 min
Response: 418400
Conc: 20.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-091622MS

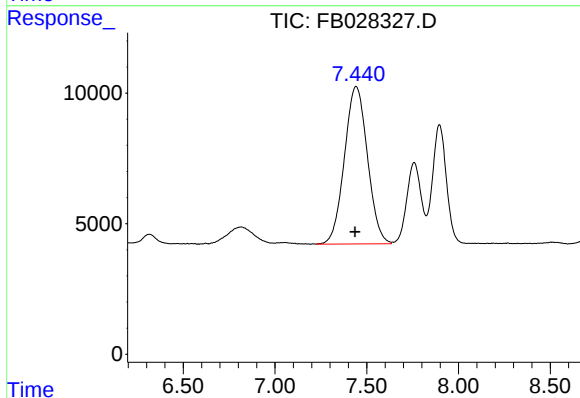


#2 2,2,4-Trimethylpentane

R.T.: 7.441 min
Delta R.T.: 0.004 min
Response: 526680
Conc: 25.04 ng/ml

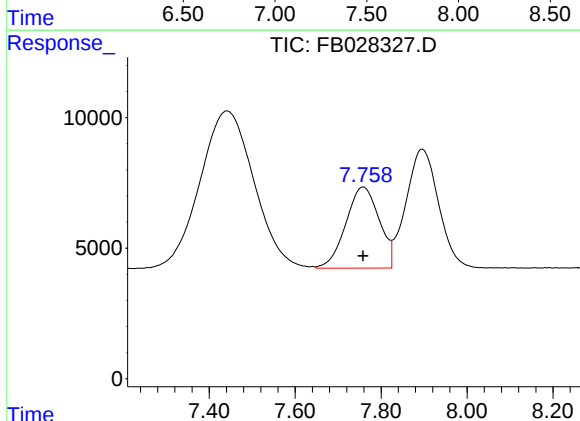


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 168217
Conc: 7.83 ng/ml

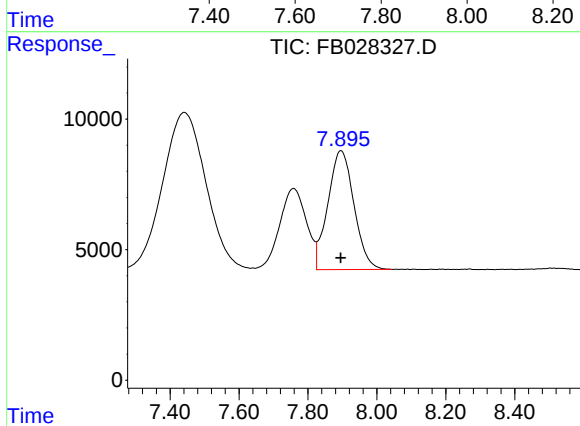

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.001 min
Response: 239740
Conc: 9.75 ng/ml

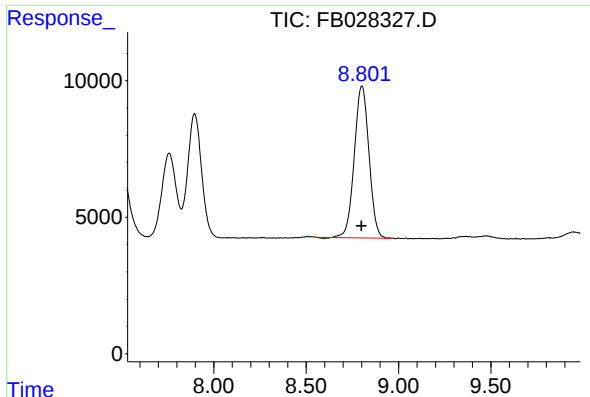

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 306679
Conc: 25.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-091622MS

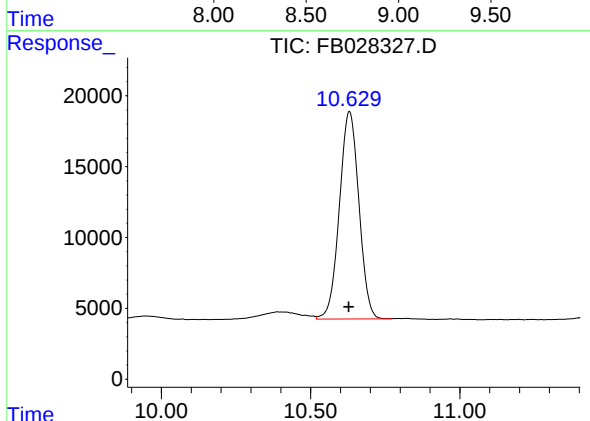


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.003 min
Response: 664981
Conc: 28.56 ng/ml

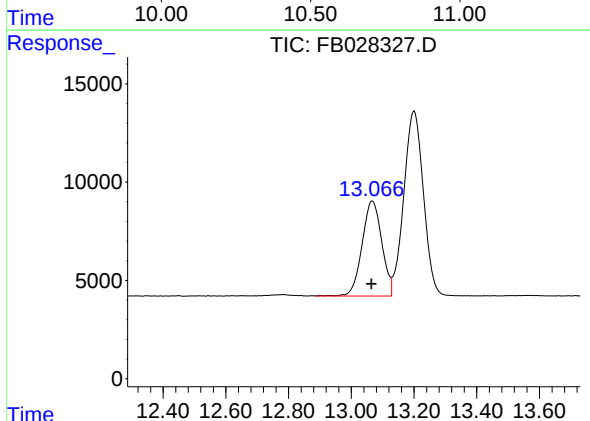


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.003 min
Response: 210474
Conc: 9.46 ng/ml

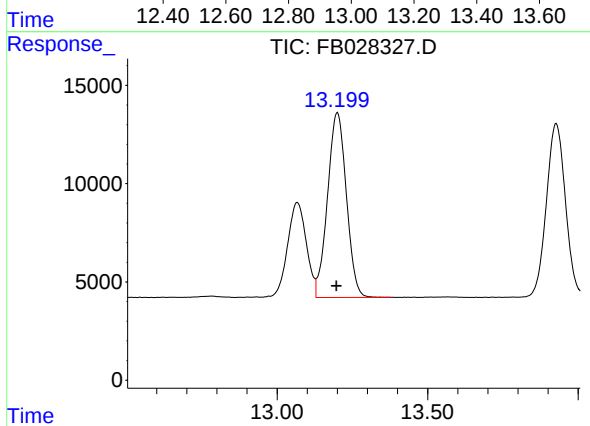

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: 0.003 min
Response: 409270
Conc: 18.75 ng/ml

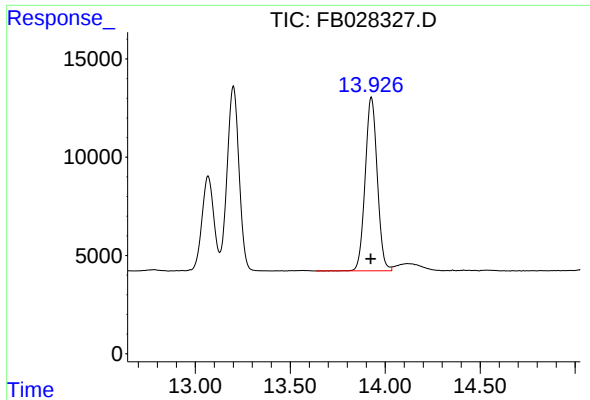

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.003 min
Response: 391078
Conc: 18.67 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-091622MS

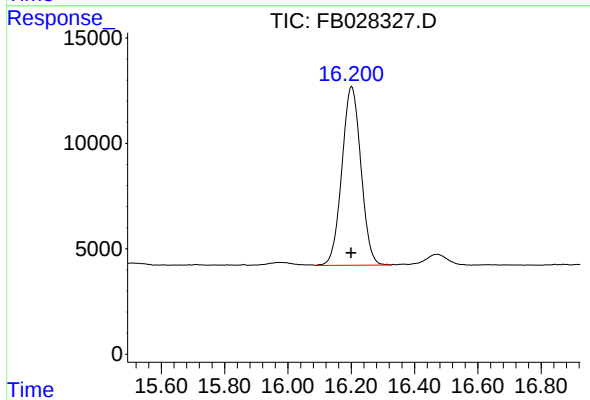

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.003 min
Response: 353722
Conc: 17.59 ng/ml