

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092022\
 Data File : FB028328.D
 Signal(s) : FID2B.CH
 Acq On : 20 Sep 2022 17:44
 Operator : AJ/MA
 Sample : N4702-01MSD 50X
 Misc : 5.08G/5.00 ML MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-03-091622MSD

Integration File: Calibration.e
 Quant Time: Sep 21 05:51:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	300415	25.100 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	419794	20.734 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	548346	26.067 ng/ml
3) t n-Heptane	7.759	181548	8.445 ng/ml
4) t Benzene	7.896	261292	10.621 ng/ml
6) t Toluene	10.631	718595	30.866 ng/ml
7) t Ethylbenzene	13.067	227158	10.215 ng/ml
8) t m-Xylene	13.200	440112	20.168 ng/ml
9) t O-Xylene	13.927	419073	20.002 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	365257	18.166 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092022\
Data File : FB028328.D
Signal(s) : FID2B.CH
Acq On : 20 Sep 2022 17:44
Operator : AJ/MA
Sample : N4702-01MSD 50X
Misc : 5.08G/5.00 ML MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-03-091622MSD

Integration File: Calibration.e
Quant Time: Sep 21 05:51:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

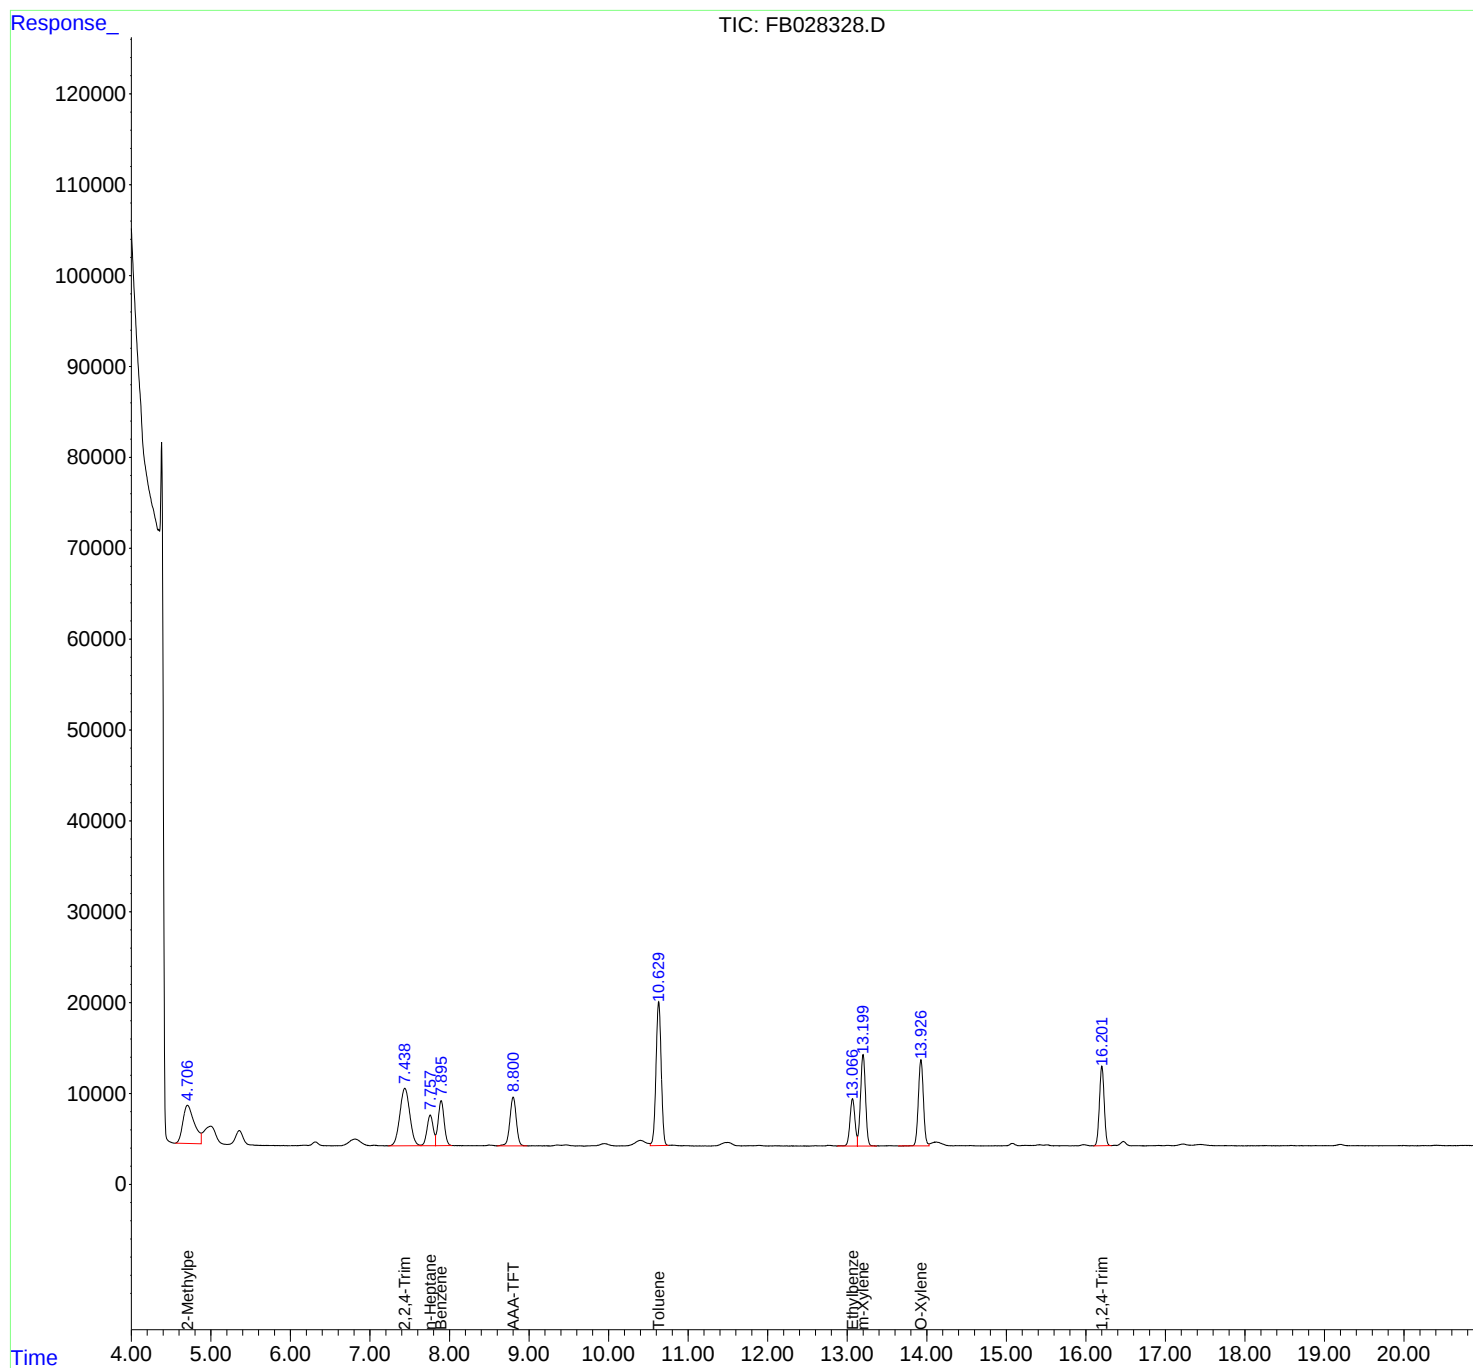


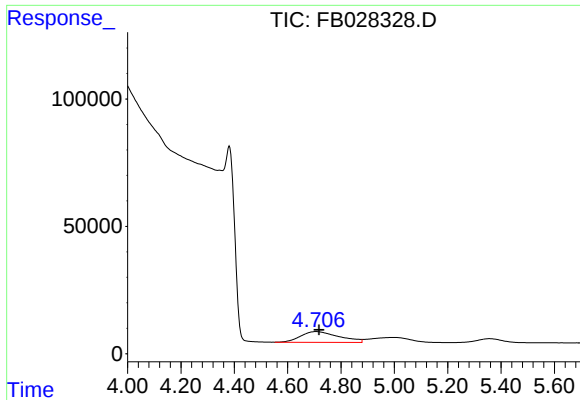

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.011 min
Response: 419794
Conc: 20.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-091622MSD

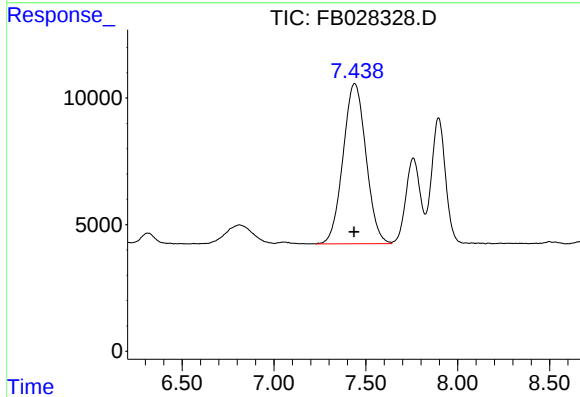


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: 0.002 min
Response: 548346
Conc: 26.07 ng/ml

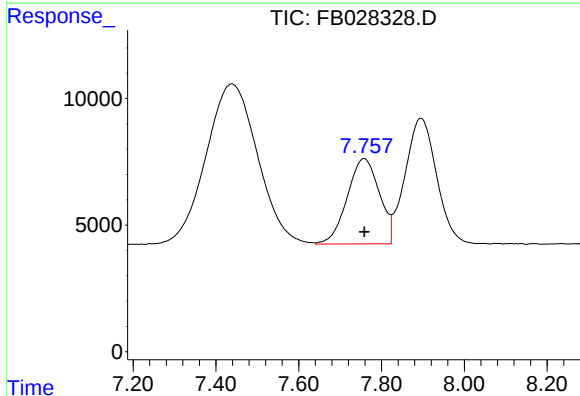


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 181548
Conc: 8.45 ng/ml

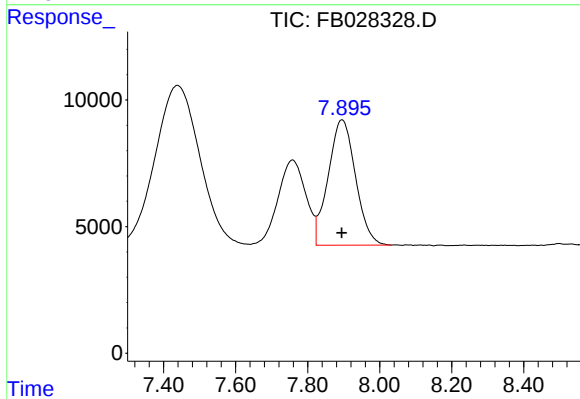

#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 261292
Conc: 10.62 ng/ml

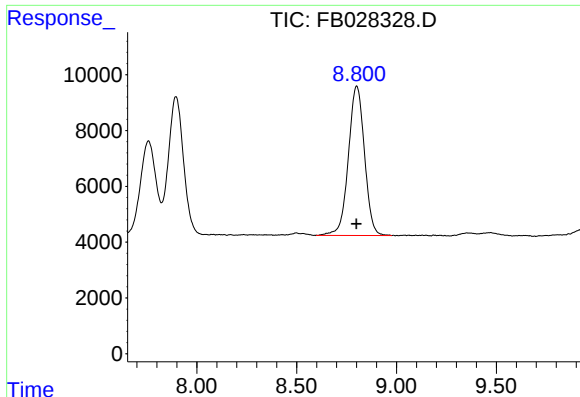

#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.001 min
Response: 300415
Conc: 25.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-091622MSD

#6 Toluene


R.T.: 10.631 min
Delta R.T.: 0.002 min
Response: 718595
Conc: 30.87 ng/ml

#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.003 min
Response: 227158
Conc: 10.21 ng/ml

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: 0.003 min
Response: 440112
Conc: 20.17 ng/ml

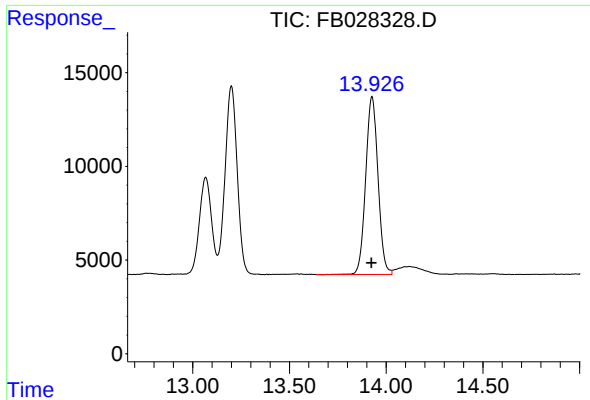

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.004 min
Response: 419073
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-091622MSD

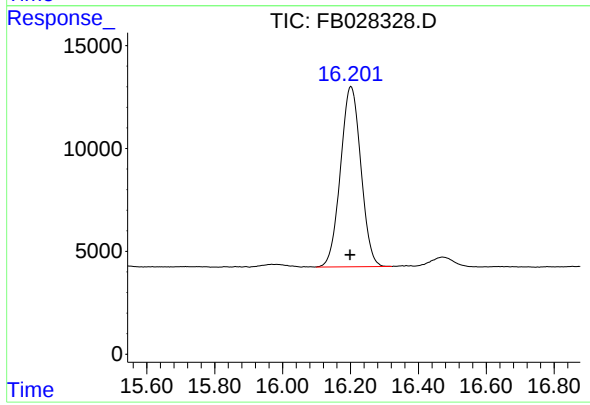

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.003 min
Response: 365257
Conc: 18.17 ng/ml