

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB092022\  
Data File : FB028362.D  
Signal(s) : FID2B.CH  
Acq On : 21 Sep 2022 17:55  
Operator : AJ/MA  
Sample : N4697-12 50X  
Misc : 5.09G/5.00 ML MEOH  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-20-COMP

Integration File: Calibration.e  
Quant Time: Sep 21 18:42:32 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090822.M  
Quant Title :  
QLast Update : Thu Sep 08 15:28:37 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 5) s AAA-TFT                | 8.801 | 247156   | 20.650 ng/ml |
|                             |       |          |              |
| Target Compounds            |       |          |              |
| 4) t Benzene                | 7.952 | 8674     | 0.353 ng/ml  |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB092022\  
Data File : FB028362.D  
Signal(s) : FID2B.CH  
Acq On : 21 Sep 2022 17:55  
Operator : AJ/MA  
Sample : N4697-12 50X  
Misc : 5.09G/5.00 ML MEOH  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-20-COMP

Integration File: Calibration.e  
Quant Time: Sep 21 18:42:32 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090822.M  
Quant Title :  
QLast Update : Thu Sep 08 15:28:37 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

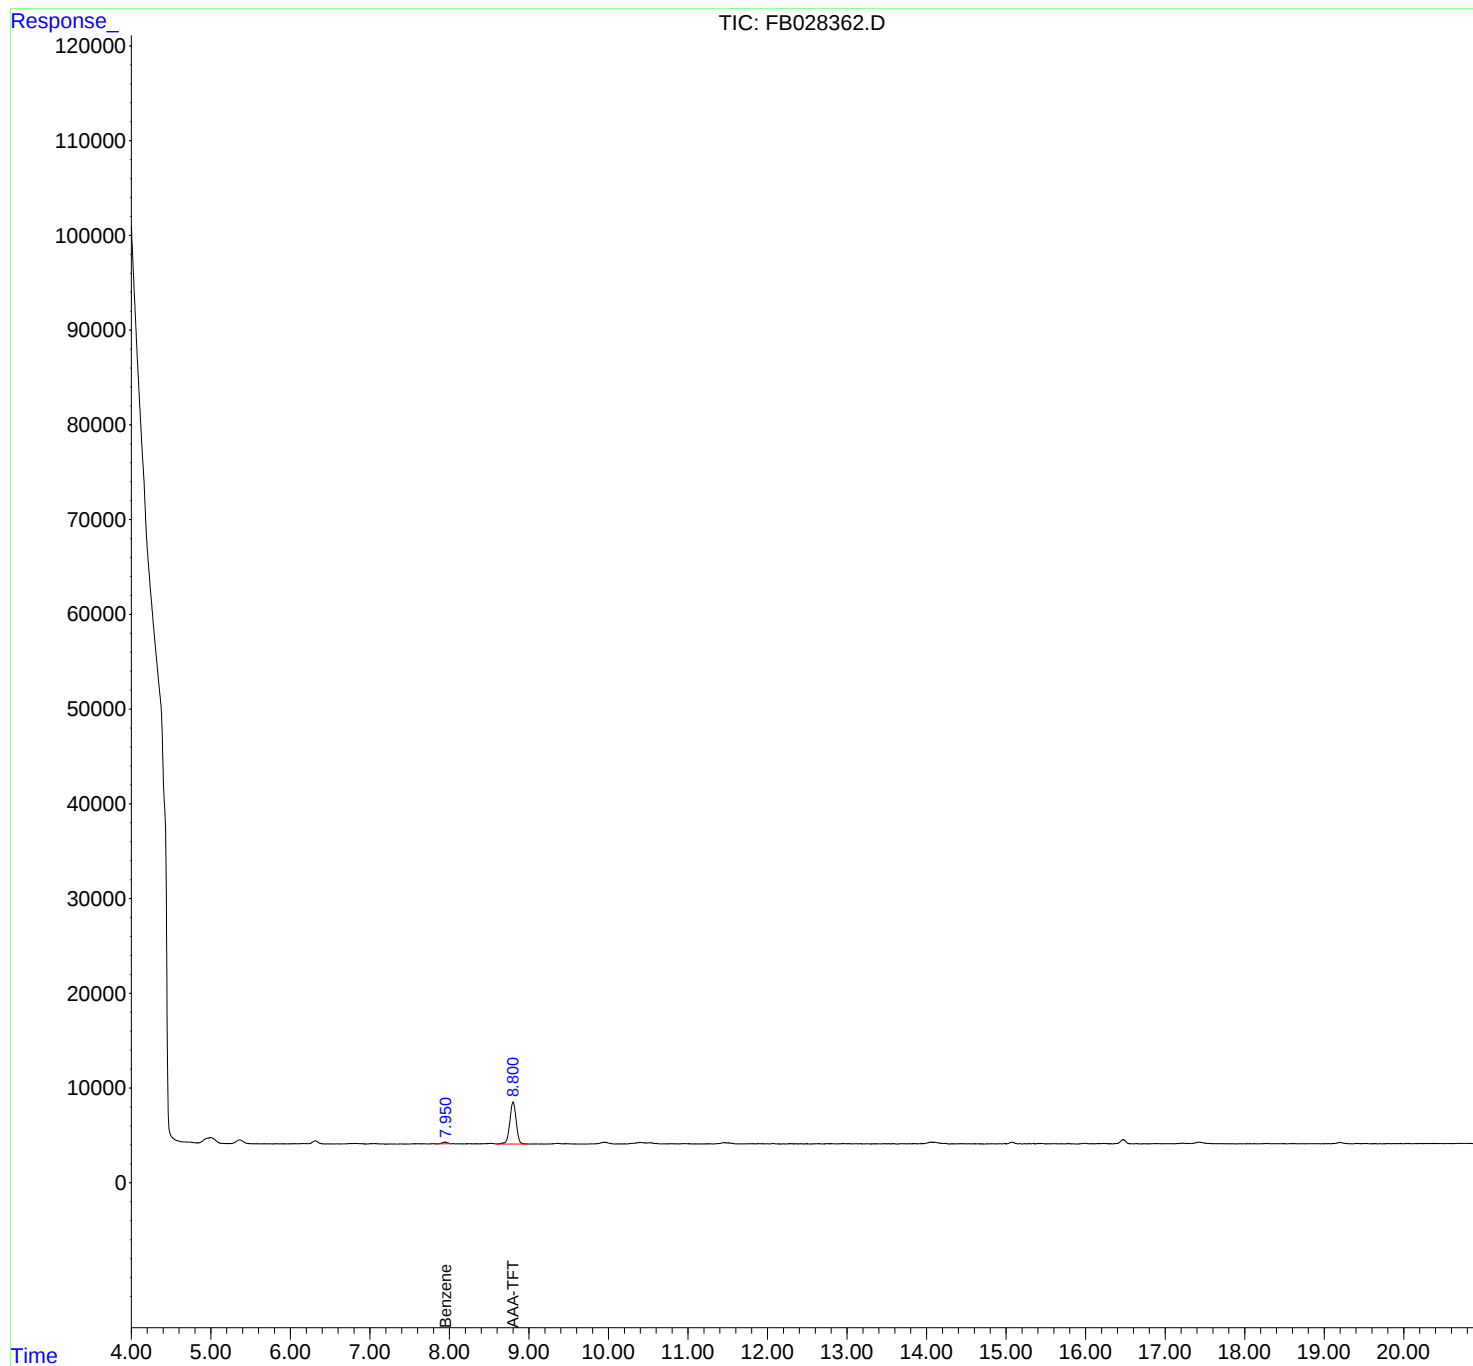


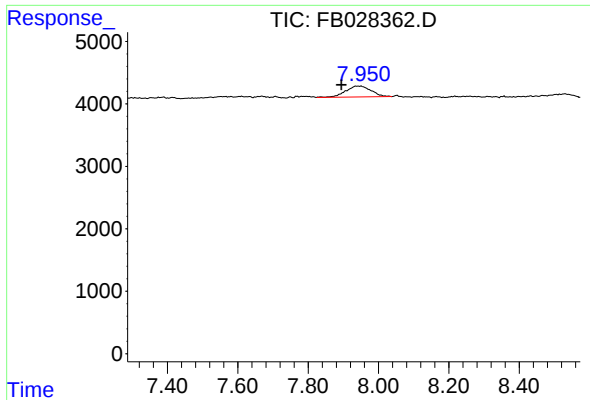

#4 Benzene

R.T.: 7.952 min  
Delta R.T.: 0.057 min  
Response: 8674  
Conc: 0.35 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
SB-20-COMP

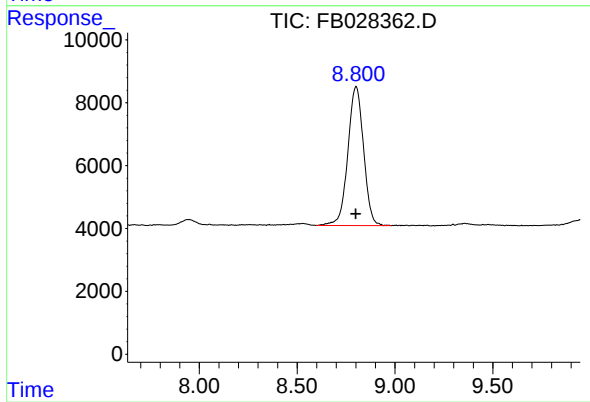

#5 AAA-TFT

R.T.: 8.801 min  
Delta R.T.: 0.001 min  
Response: 247156  
Conc: 20.65 ng/ml