

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB092022\  
Data File : FB028329.D  
Signal(s) : FID2B.CH  
Acq On : 20 Sep 2022 18:21  
Operator : AJ/MA  
Sample : N4697-02  
Misc : 5.09G/5.00 ML DI WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-22-COMP

Integration File: Calibration.e  
Quant Time: Sep 21 05:51:24 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090822.M  
Quant Title :  
QLast Update : Thu Sep 08 15:28:37 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T. | Response | Conc Units |
|-----------------------------|------|----------|------------|
| -----                       |      |          |            |
| System Monitoring Compounds |      |          |            |
| Target Compounds            |      |          |            |
| -----                       |      |          |            |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB092022\  
Data File : FB028329.D  
Signal(s) : FID2B.CH  
Acq On : 20 Sep 2022 18:21  
Operator : AJ/MA  
Sample : N4697-02  
Misc : 5.09G/5.00 ML DI WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-22-COMP

Integration File: Calibration.e  
Quant Time: Sep 21 05:51:24 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090822.M  
Quant Title :  
QLast Update : Thu Sep 08 15:28:37 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

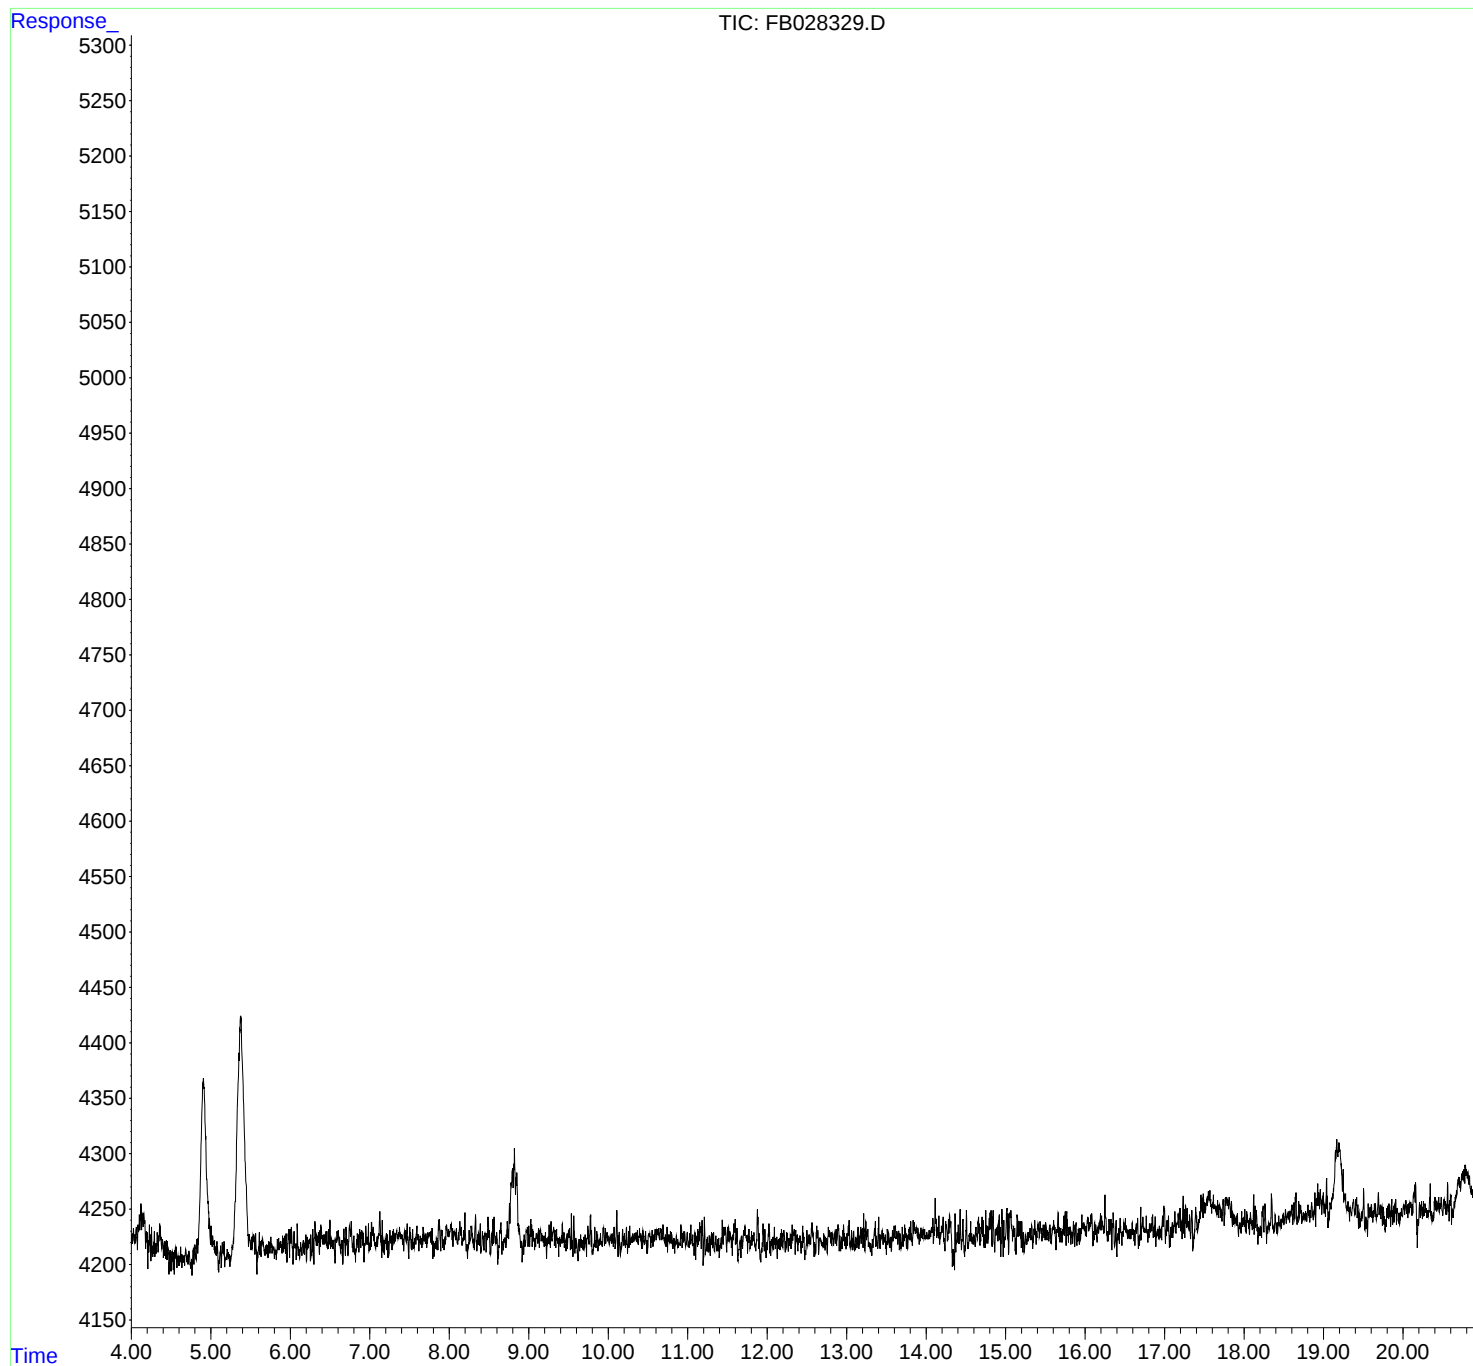

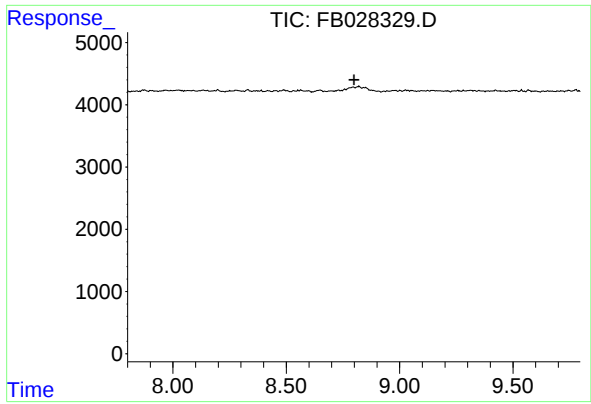

#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T.: 8.800 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_B  
ClientSampleId :  
SB-22-COMP