

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092118\
 Data File : FB017861.D
 Signal(s) : FID2B.CH
 Acq On : 21 Sep 2018 15:08
 Operator : MJ/SJ
 Sample : BSF0921S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0921S1

Integration File: Calibration.e
 Quant Time: Sep 24 07:04:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	165066	19.514 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	448236	28.146 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	456136	28.663 ng/ml
3) t n-Heptane	8.064	146951	9.536 ng/ml
4) t Benzene	8.203	178819	9.393 ng/ml
6) t Toluene	10.957	457052	28.880 ng/ml
7) t Ethylbenzene	13.406	162453	9.942 ng/ml
8) t m-Xylene	13.539	342293	19.786 ng/ml
9) t O-Xylene	14.271	356958	19.643 ng/ml
10) t 1,2,4-Trimethylbenzene	16.553	409446	19.248 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092118\
Data File : FB017861.D
Signal(s) : FID2B.CH
Acq On : 21 Sep 2018 15:08
Operator : MJ/SJ
Sample : BSF0921S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0921S1

Integration File: Calibration.e
Quant Time: Sep 24 07:04:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

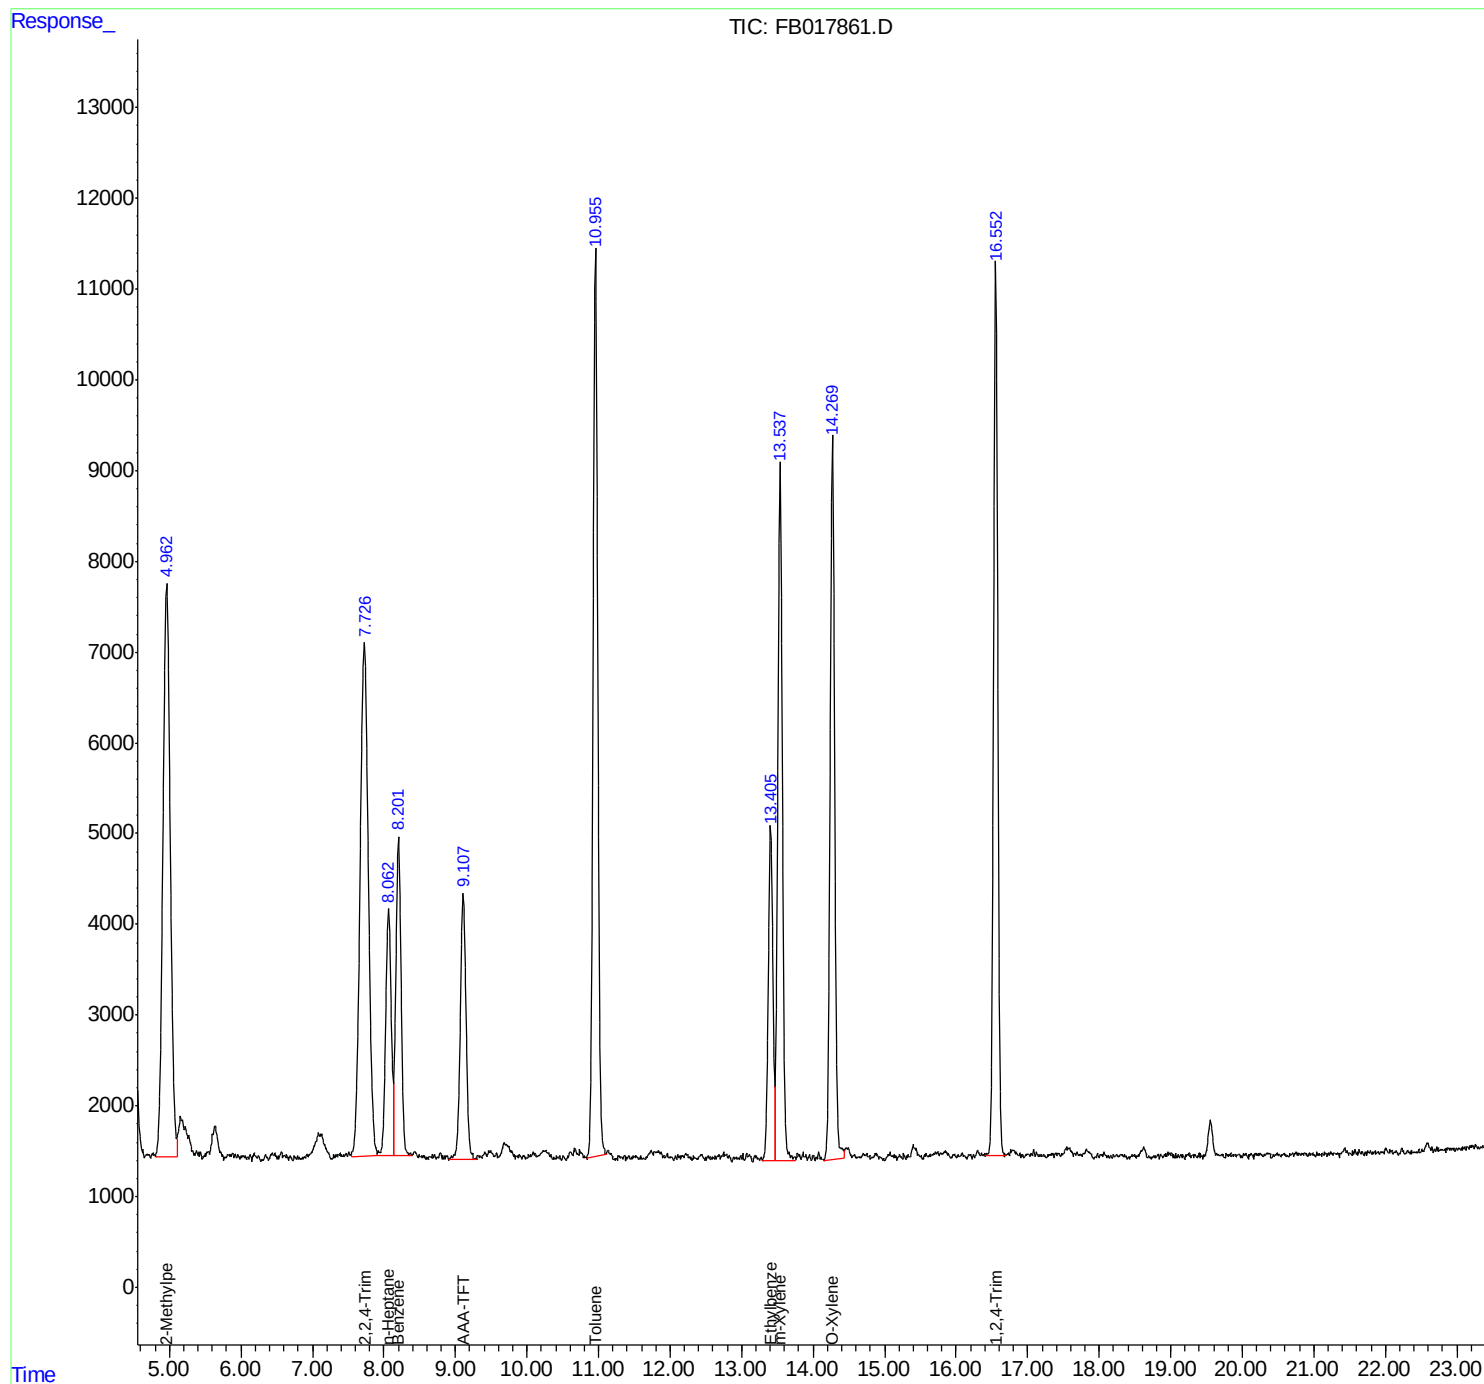


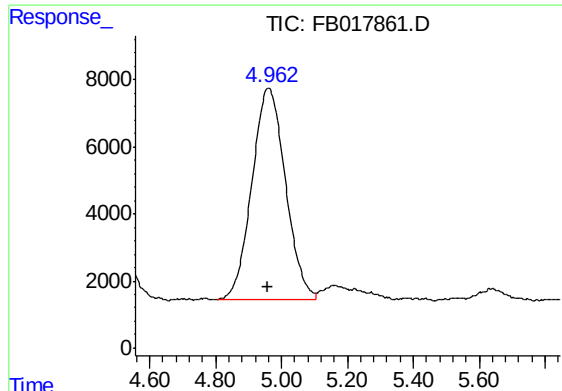

#1 2-Methylpentane


R.T.: 4.961 min
Delta R.T.: 0.001 min
Response: 448236
Conc: 28.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0921S1

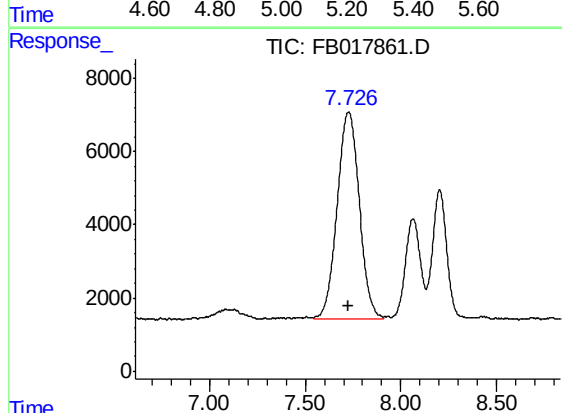


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.001 min
Response: 456136
Conc: 28.66 ng/ml

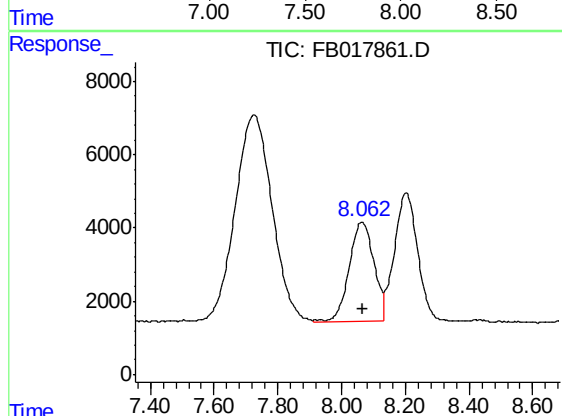


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 146951
Conc: 9.54 ng/ml

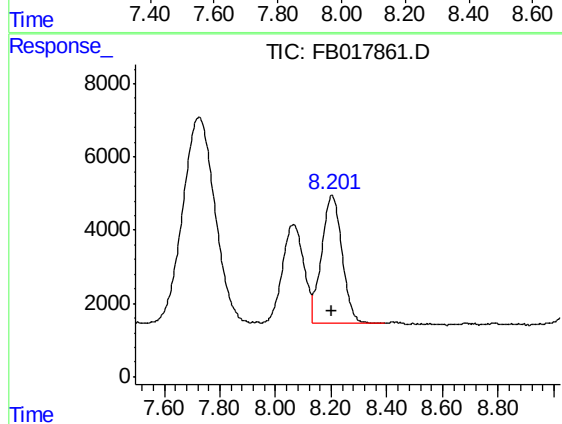

#4 Benzene


R.T.: 8.203 min
Delta R.T.: -0.001 min
Response: 178819
Conc: 9.39 ng/ml

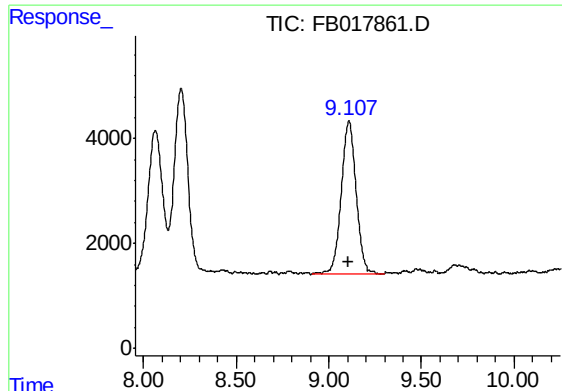

#5 AAA-TFT


R.T.: 9.109 min
Delta R.T.: 0.000 min
Response: 165066
Conc: 19.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0921S1

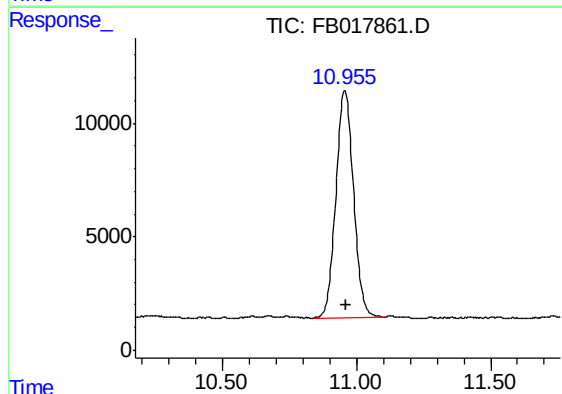


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.002 min
Response: 457052
Conc: 28.88 ng/ml

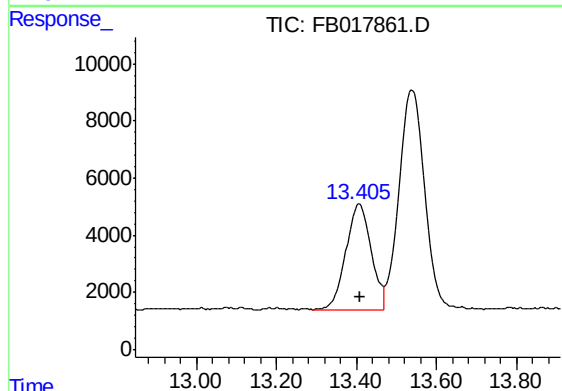


#7 Ethylbenzene

R.T.: 13.406 min
Delta R.T.: -0.002 min
Response: 162453
Conc: 9.94 ng/ml

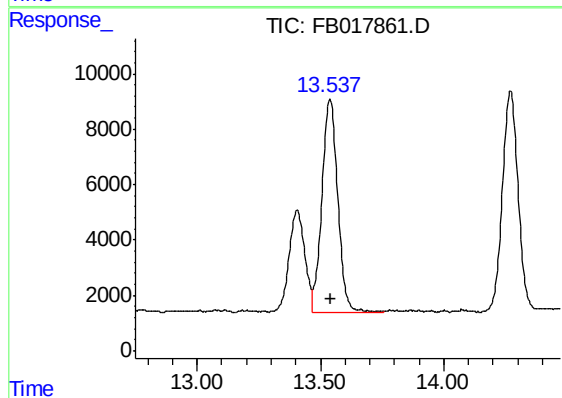

#8 m-Xylene


R.T.: 13.539 min
Delta R.T.: -0.002 min
Response: 342293
Conc: 19.79 ng/ml

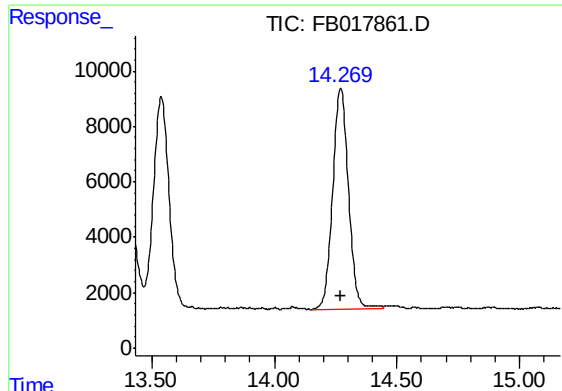

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.002 min
Response: 356958
Conc: 19.64 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0921S1

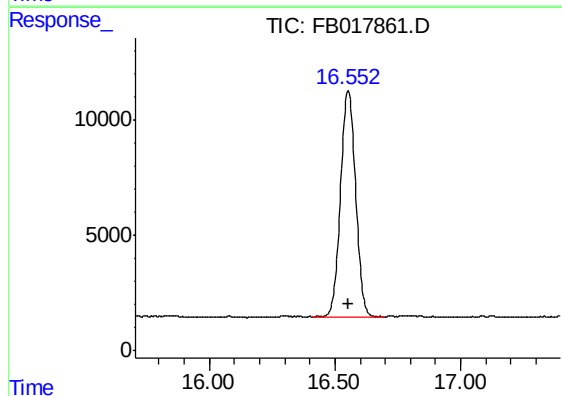

#10 1,2,4-Trimethylbenzene

R.T.: 16.553 min
Delta R.T.: -0.002 min
Response: 409446
Conc: 19.25 ng/ml