

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092120\
 Data File : FB024903.D
 Signal(s) : FID2B.CH
 Acq On : 21 Sep 2020 12:34
 Operator : DD/AJ
 Sample : BSF0921S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 22 01:11:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
 Quant Title :
 QLast Update : Tue Sep 15 13:37:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	381520	17.146 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	835973	28.424 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	882830	29.262 ng/ml
3) t n-Heptane	7.754	289429	9.554 ng/ml
4) t Benzene	7.889	347923	8.989 ng/ml
6) t Toluene	10.627	1004886	27.581 ng/ml
7) t Ethylbenzene	13.067	314343	9.352 ng/ml
8) t m-Xylene	13.200	618622	18.885 ng/ml
9) t O-Xylene	13.927	593923	18.594 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	504190	19.334 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092120\
Data File : FB024903.D
Signal(s) : FID2B.CH
Acq On : 21 Sep 2020 12:34
Operator : DD/AJ
Sample : BSF0921S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 22 01:11:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

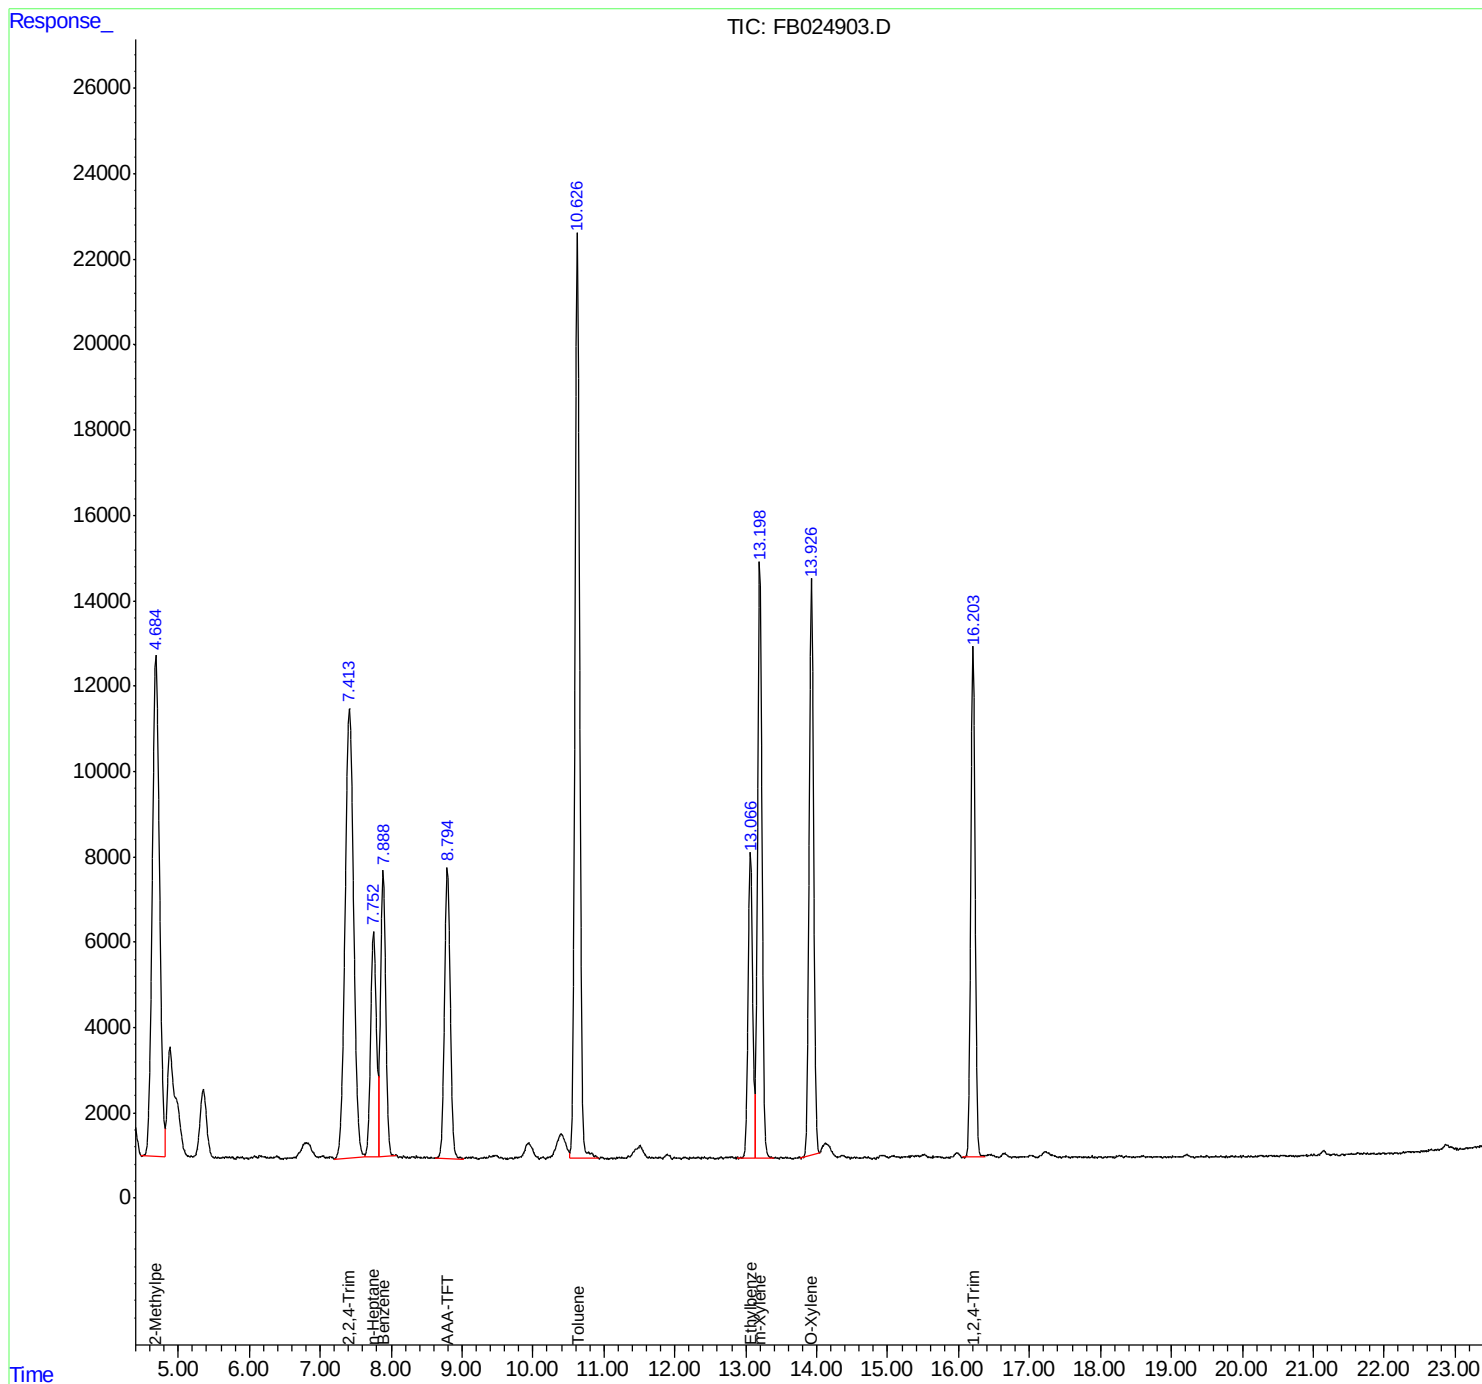


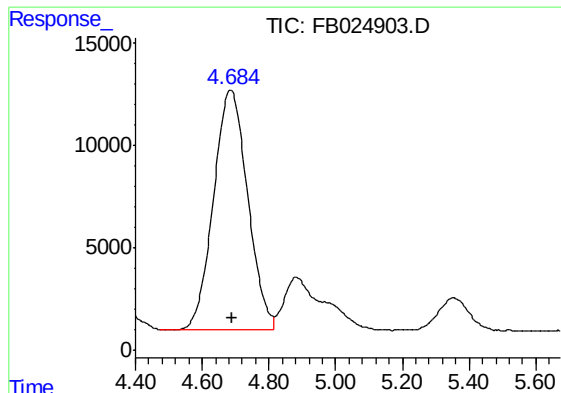

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.003 min
Response: 835973
Conc: 28.42 ng/ml

Instrument :
FID_B
ClientSampleId :

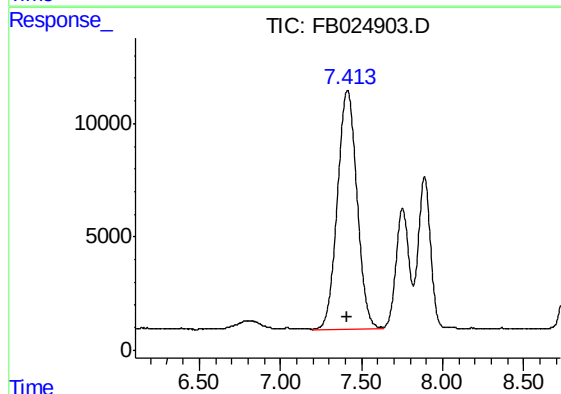


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.001 min
Response: 882830
Conc: 29.26 ng/ml

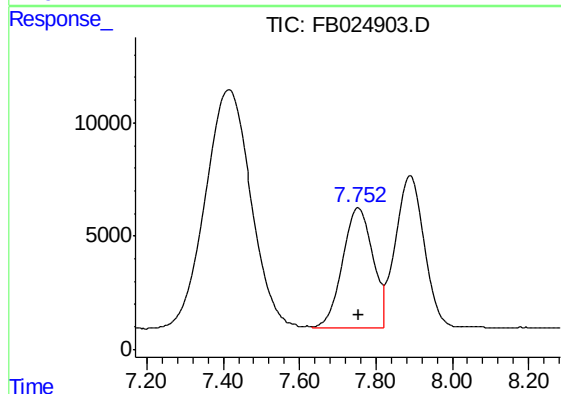


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.002 min
Response: 289429
Conc: 9.55 ng/ml

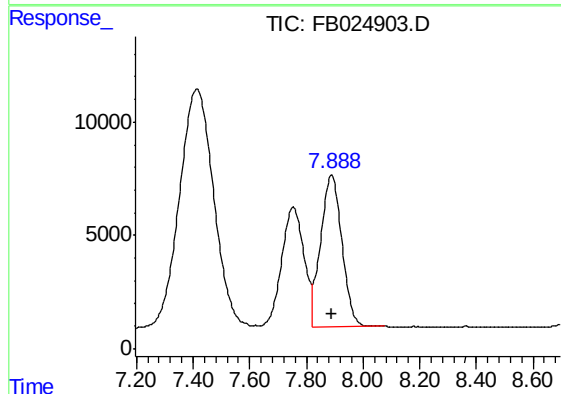

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.002 min
Response: 347923
Conc: 8.99 ng/ml

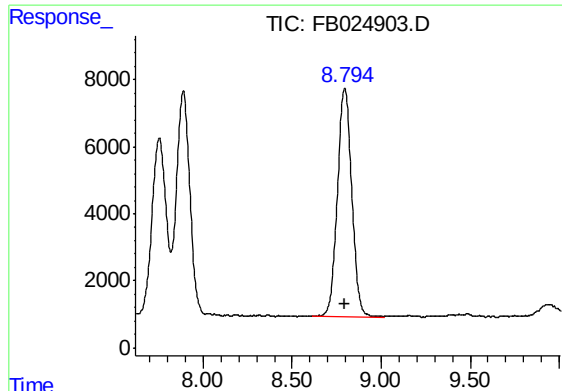

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 381520
Conc: 17.15 ng/ml

Instrument :
FID_B
ClientSampleId :

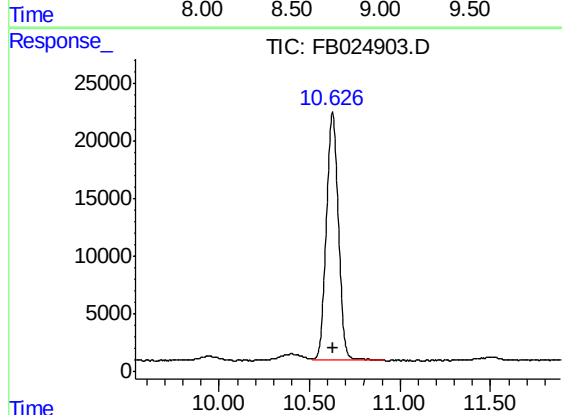


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.002 min
Response: 1004886
Conc: 27.58 ng/ml

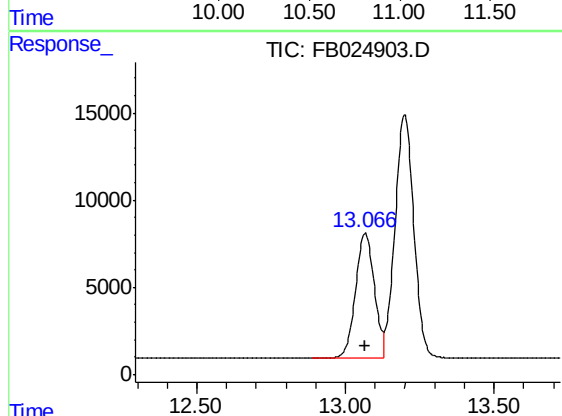


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.001 min
Response: 314343
Conc: 9.35 ng/ml

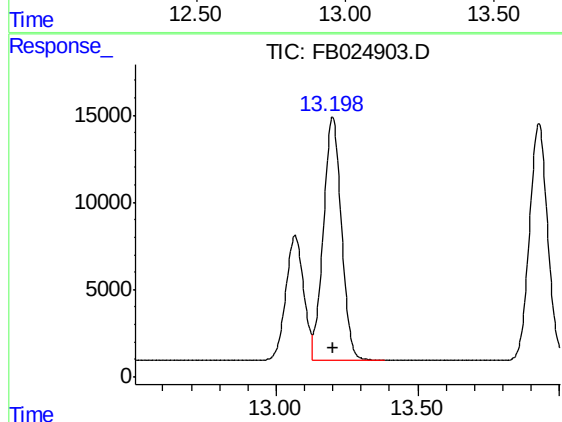

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.001 min
Response: 618622
Conc: 18.88 ng/ml

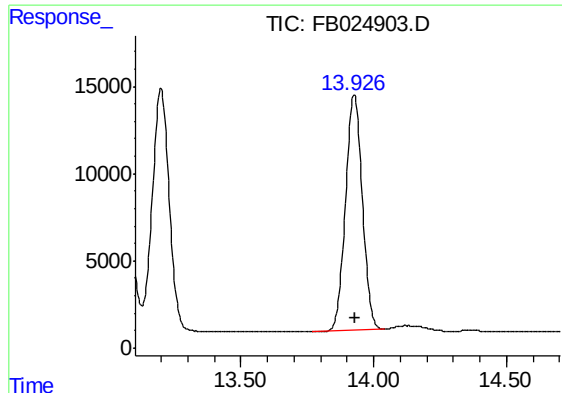

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.001 min
Response: 593923
Conc: 18.59 ng/ml

Instrument :
FID_B
ClientSampleId :

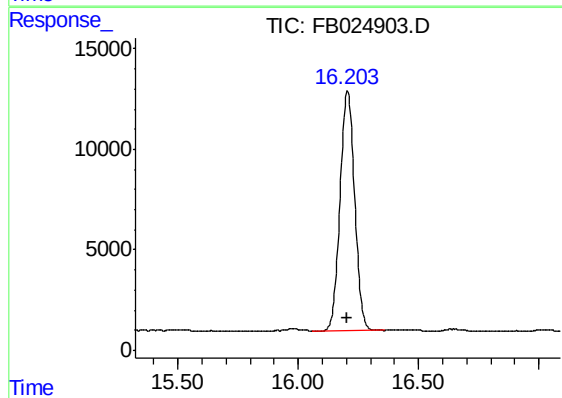

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.000 min
Response: 504190
Conc: 19.33 ng/ml