

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092120\
 Data File : FB024907.D
 Signal(s) : FID2B.CH
 Acq On : 21 Sep 2020 14:36
 Operator : DD/AJ
 Sample : L4095-03MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 22 01:11:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
 Quant Title :
 QLast Update : Tue Sep 15 13:37:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	449132	20.184 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	841213	28.603 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	805611	26.702 ng/ml
3) t n-Heptane	7.756	267413	8.828 ng/ml
4) t Benzene	7.890	369311	9.542 ng/ml
6) t Toluene	10.628	1027098	28.190 ng/ml
7) t Ethylbenzene	13.067	310393	9.234 ng/ml
8) t m-Xylene	13.201	614567	18.761 ng/ml
9) t O-Xylene	13.928	593068	18.567 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	482159	18.489 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092120\
Data File : FB024907.D
Signal(s) : FID2B.CH
Acq On : 21 Sep 2020 14:36
Operator : DD/AJ
Sample : L4095-03MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 22 01:11:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

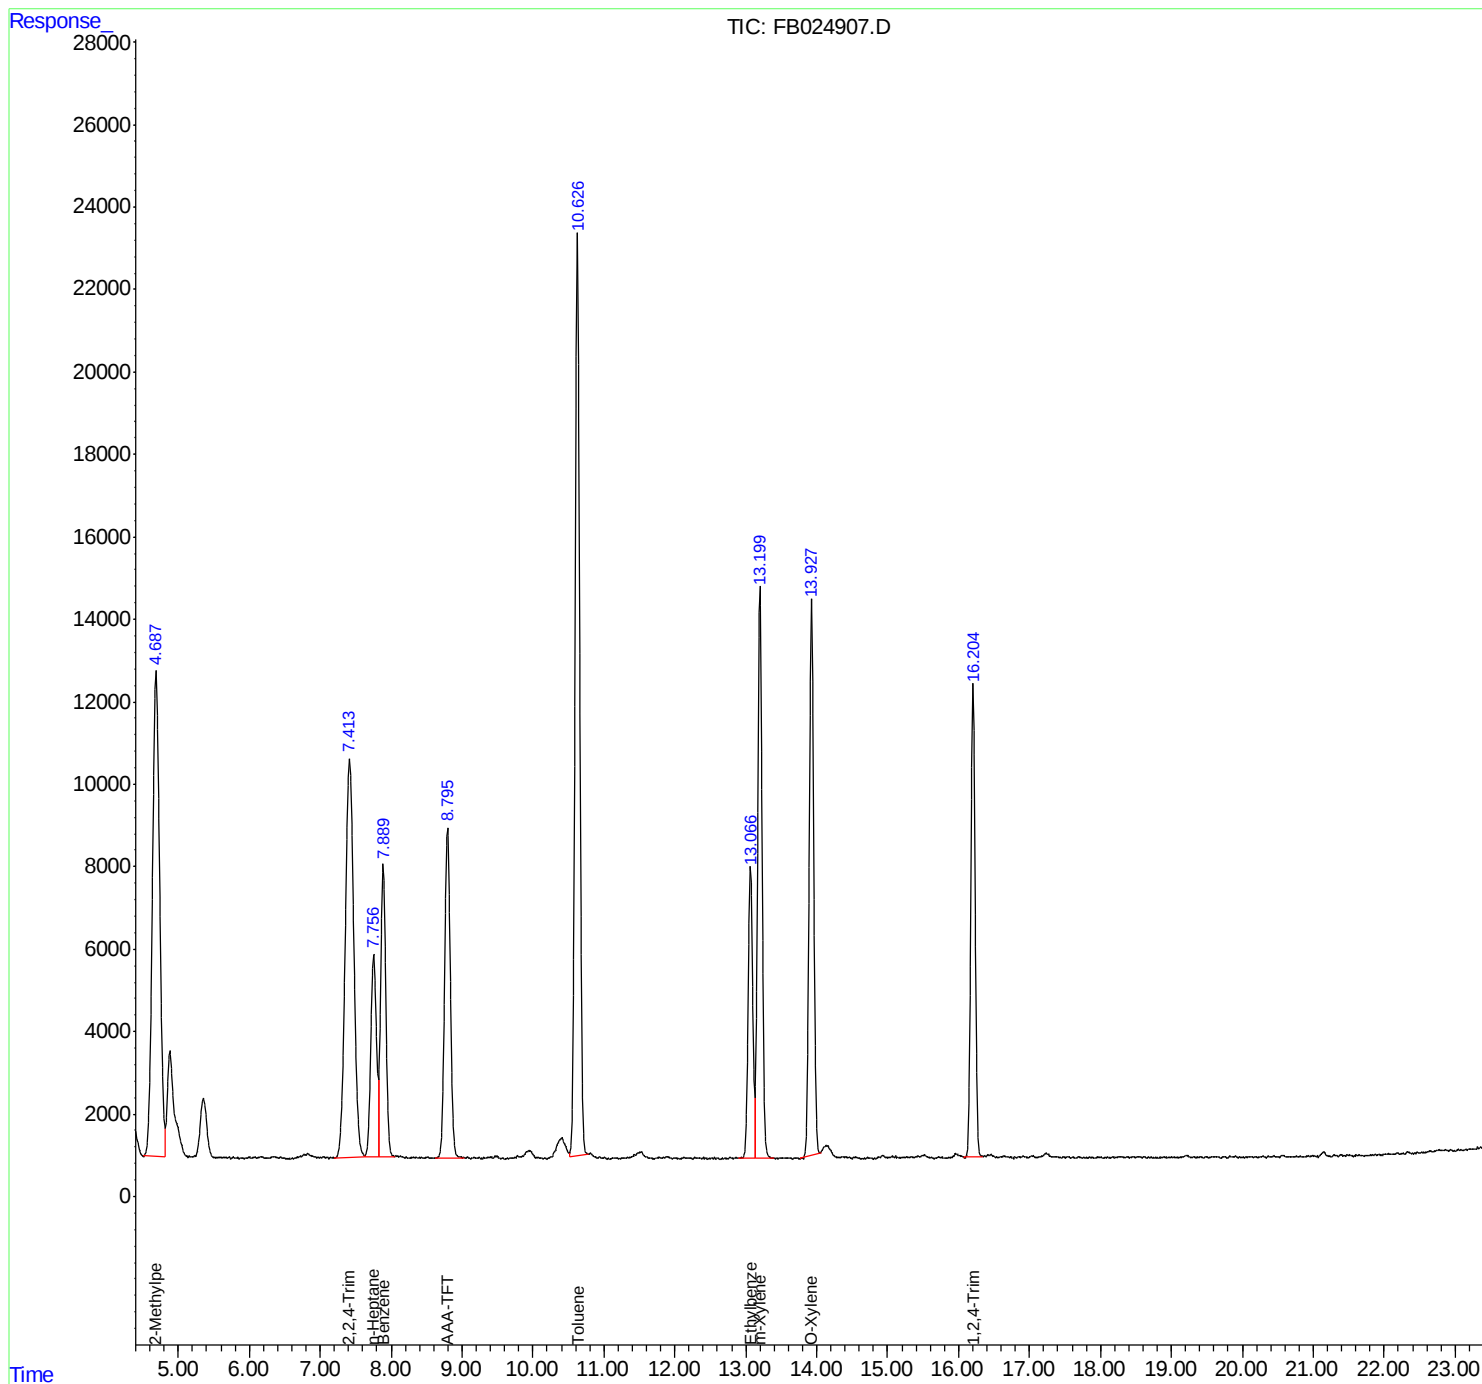


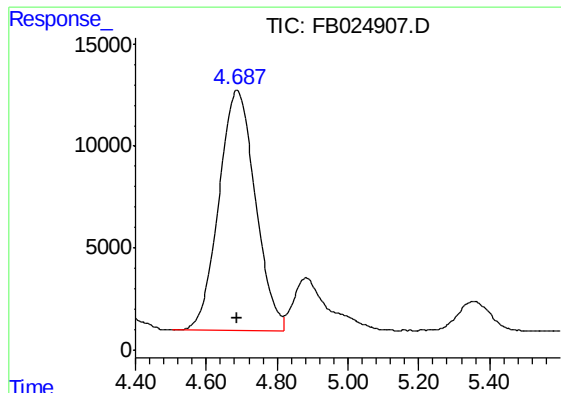

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 841213
Conc: 28.60 ng/ml

Instrument :
FID_B
ClientSampleId :

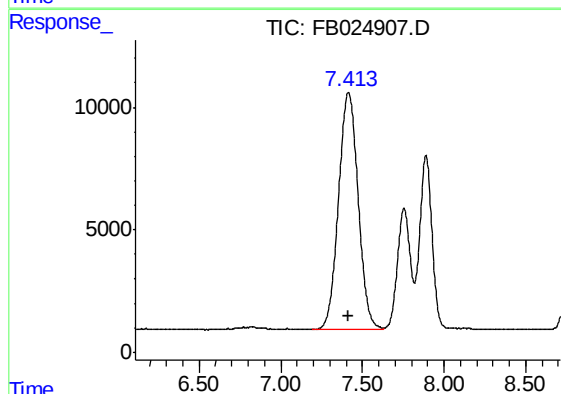


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.001 min
Response: 805611
Conc: 26.70 ng/ml

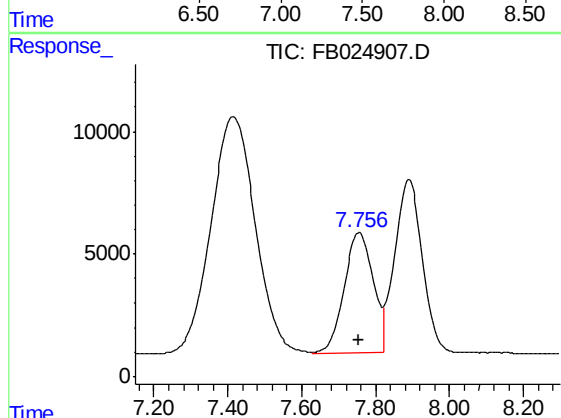


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 267413
Conc: 8.83 ng/ml

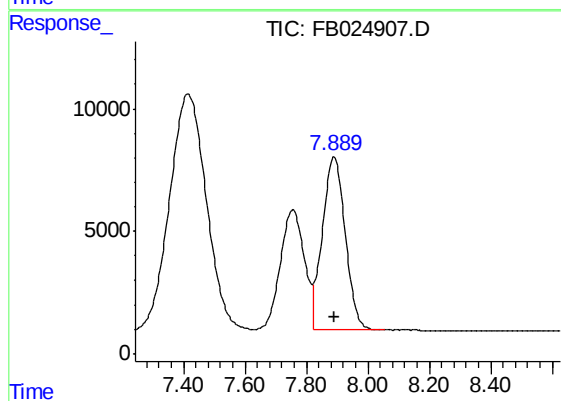

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 369311
Conc: 9.54 ng/ml

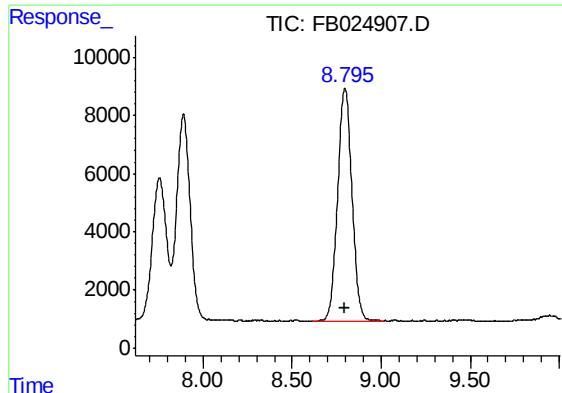

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 449132
Conc: 20.18 ng/ml

Instrument :
FID_B
ClientSampleId :

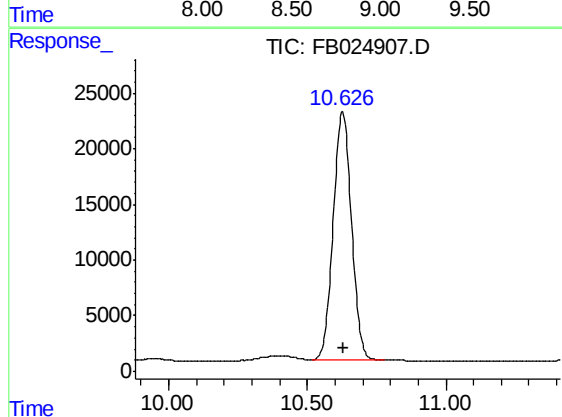


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 1027098
Conc: 28.19 ng/ml

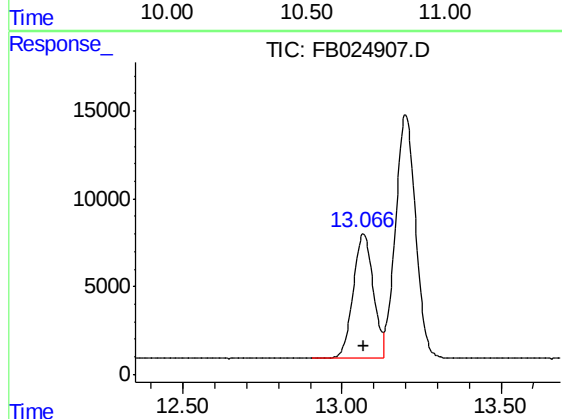


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.000 min
Response: 310393
Conc: 9.23 ng/ml

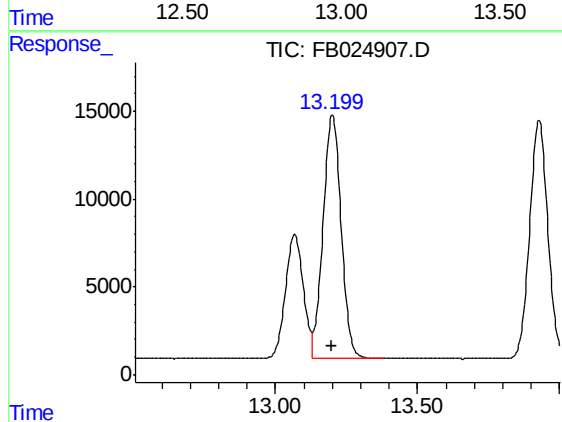

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 614567
Conc: 18.76 ng/ml

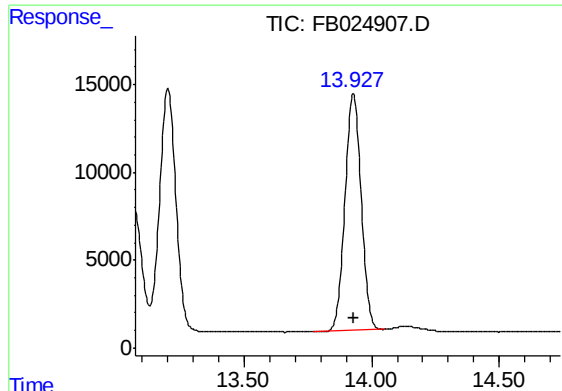

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.000 min
Response: 593068
Conc: 18.57 ng/ml

Instrument :
FID_B
ClientSampleId :

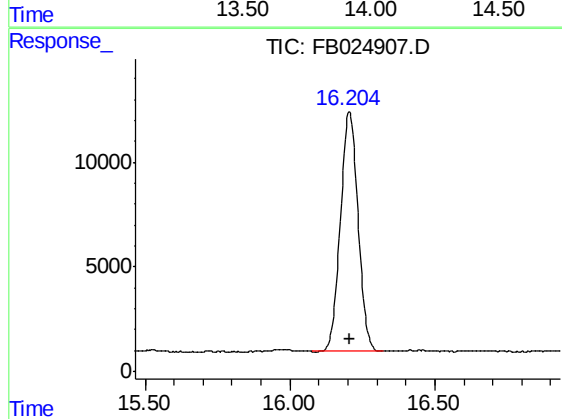

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.000 min
Response: 482159
Conc: 18.49 ng/ml