

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092120\
 Data File : FB024908.D
 Signal(s) : FID2B.CH
 Acq On : 21 Sep 2020 15:07
 Operator : DD/AJ
 Sample : L4059-03MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 22 01:12:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
 Quant Title :
 QLast Update : Tue Sep 15 13:37:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	467623	21.015 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	846089	28.768 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	776552	25.739 ng/ml
3) t n-Heptane	7.755	260253	8.591 ng/ml
4) t Benzene	7.890	381785	9.864 ng/ml
6) t Toluene	10.628	1045621	28.699 ng/ml
7) t Ethylbenzene	13.068	313362	9.323 ng/ml
8) t m-Xylene	13.201	623097	19.021 ng/ml
9) t O-Xylene	13.928	604690	18.931 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	491782	18.858 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092120\
Data File : FB024908.D
Signal(s) : FID2B.CH
Acq On : 21 Sep 2020 15:07
Operator : DD/AJ
Sample : L4059-03MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 22 01:12:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091520.M
Quant Title :
QLast Update : Tue Sep 15 13:37:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

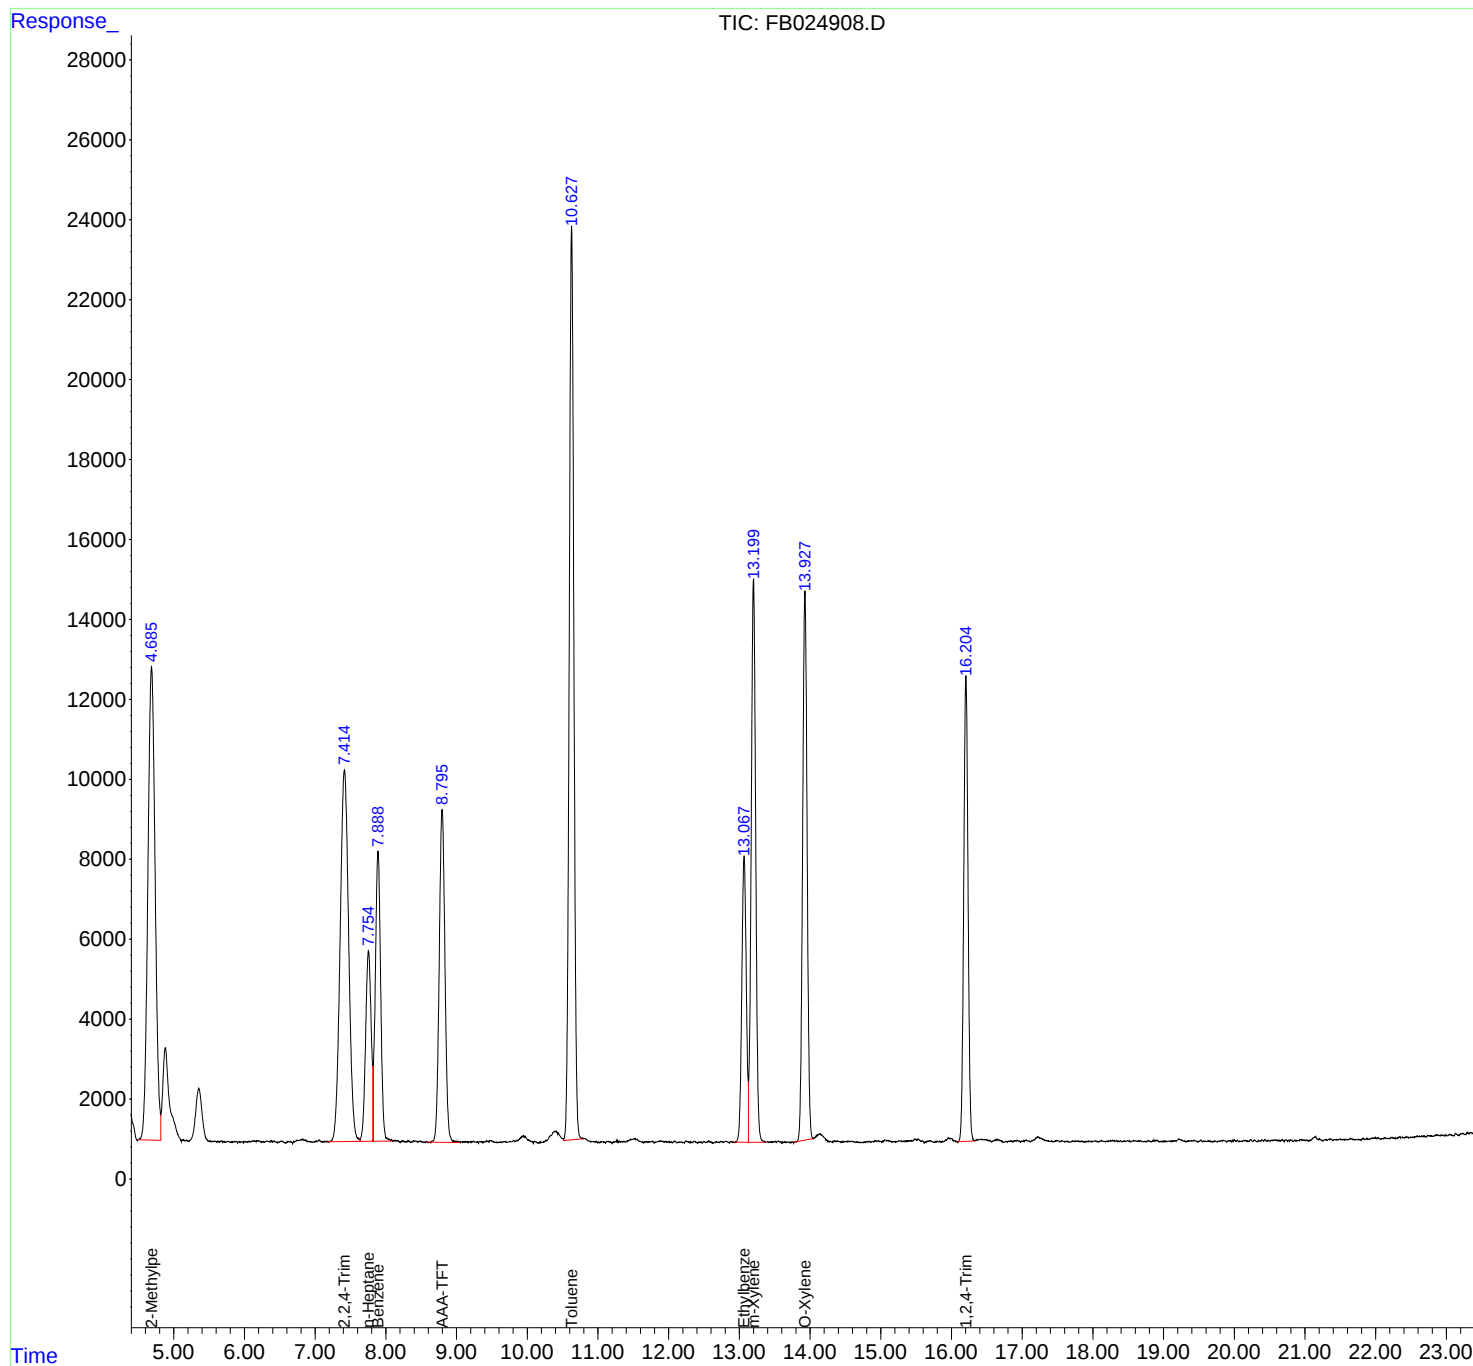


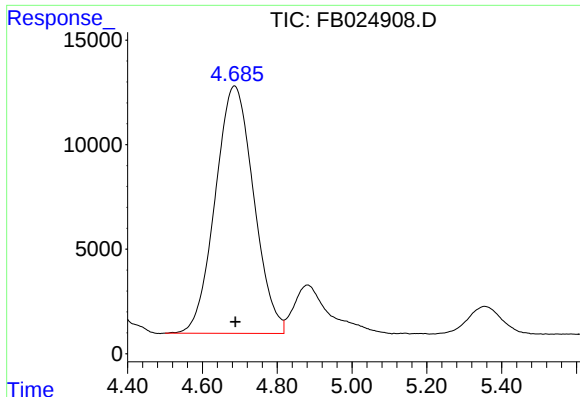

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.001 min
Response: 846089
Conc: 28.77 ng/ml

Instrument :
FID_B
ClientSampleId :

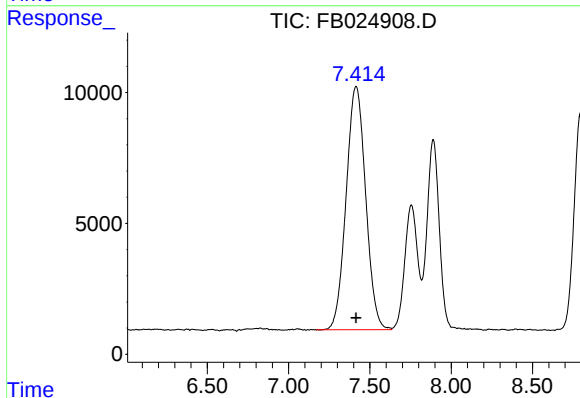


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 776552
Conc: 25.74 ng/ml

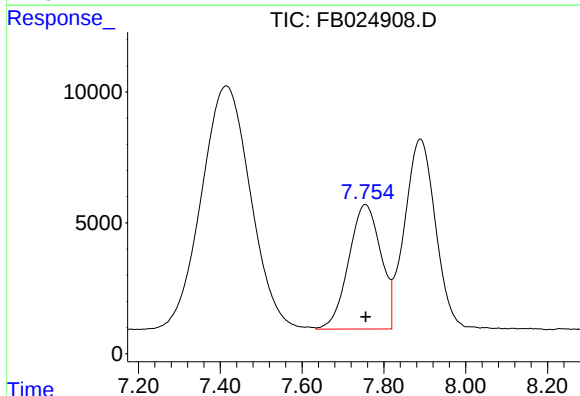


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 260253
Conc: 8.59 ng/ml

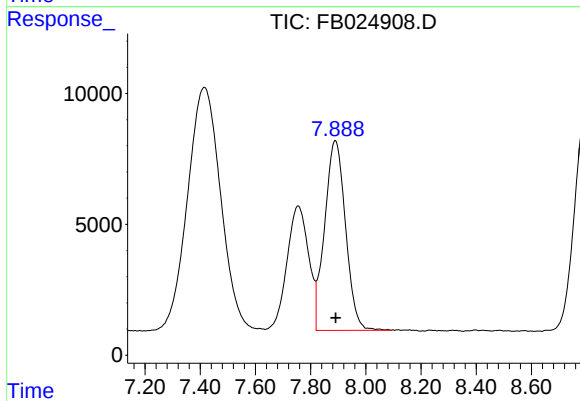

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 381785
Conc: 9.86 ng/ml

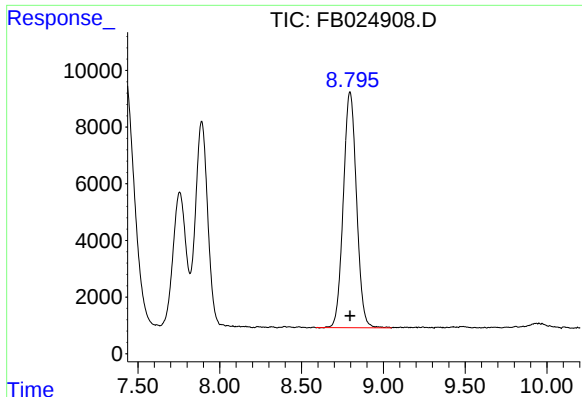

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.001 min
Response: 467623
Conc: 21.02 ng/ml

Instrument :
FID_B
ClientSampleId :

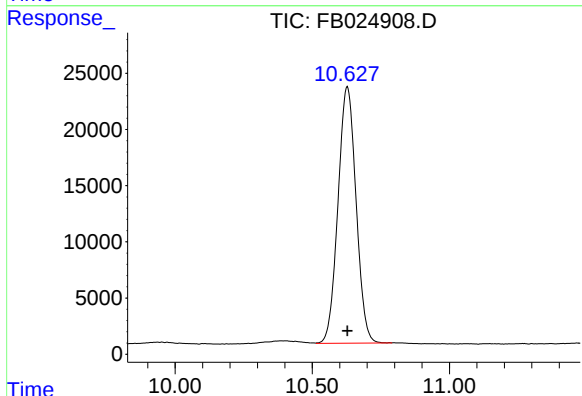


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 1045621
Conc: 28.70 ng/ml

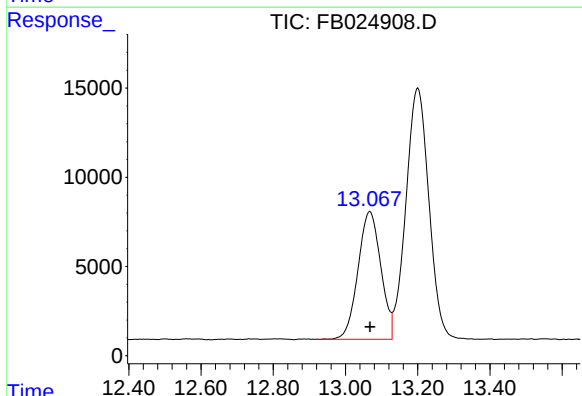


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.000 min
Response: 313362
Conc: 9.32 ng/ml

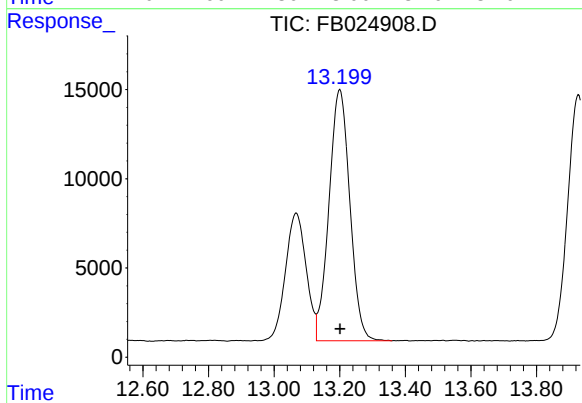

#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 623097
Conc: 19.02 ng/ml

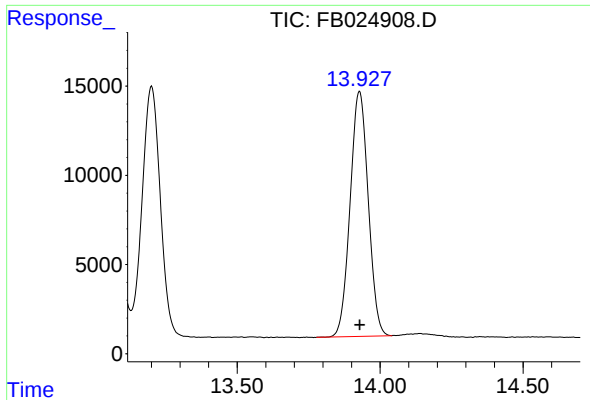

#9 O-Xylene


R.T.: 13.928 min

Delta R.T.: 0.000 min

Response: 604690

Conc: 18.93 ng/ml

Instrument :
FID_B
ClientSampleId :

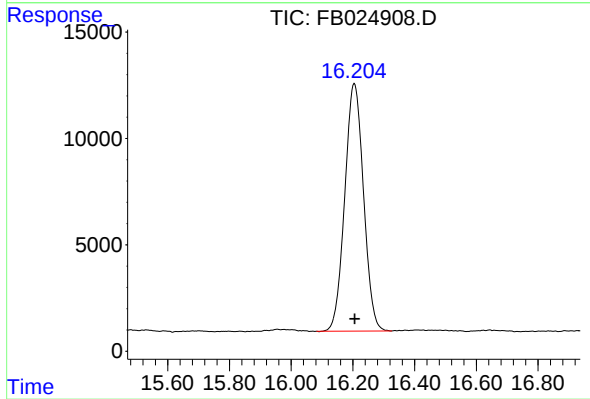

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min

Delta R.T.: 0.000 min

Response: 491782

Conc: 18.86 ng/ml