

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092121\
 Data File : FB026240.D
 Signal(s) : FID2B.CH
 Acq On : 21 Sep 2021 16:51
 Operator : AJ/MA
 Sample : M3823-03MS
 Misc : 5.08G/5.00ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 22 01:08:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:24:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.835	337437	19.813 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.825	559727	25.192 ng/ml
2) t 2,2,4-Trimethylpentane	7.489	521098	23.444 ng/ml
3) t n-Heptane	7.809	149455	5.787 ng/ml
4) t Benzene	7.946	250210	9.187 ng/ml
6) t Toluene	10.647	729642	27.839 ng/ml
7) t Ethylbenzene	13.067	206081	9.038 ng/ml
8) t m-Xylene	13.200	391302	17.454 ng/ml
9) t O-Xylene	13.924	398825	18.782 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	369104	16.368 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092121\
Data File : FB026240.D
Signal(s) : FID2B.CH
Acq On : 21 Sep 2021 16:51
Operator : AJ/MA
Sample : M3823-03MS
Misc : 5.08G/5.00ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 22 01:08:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:24:36 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

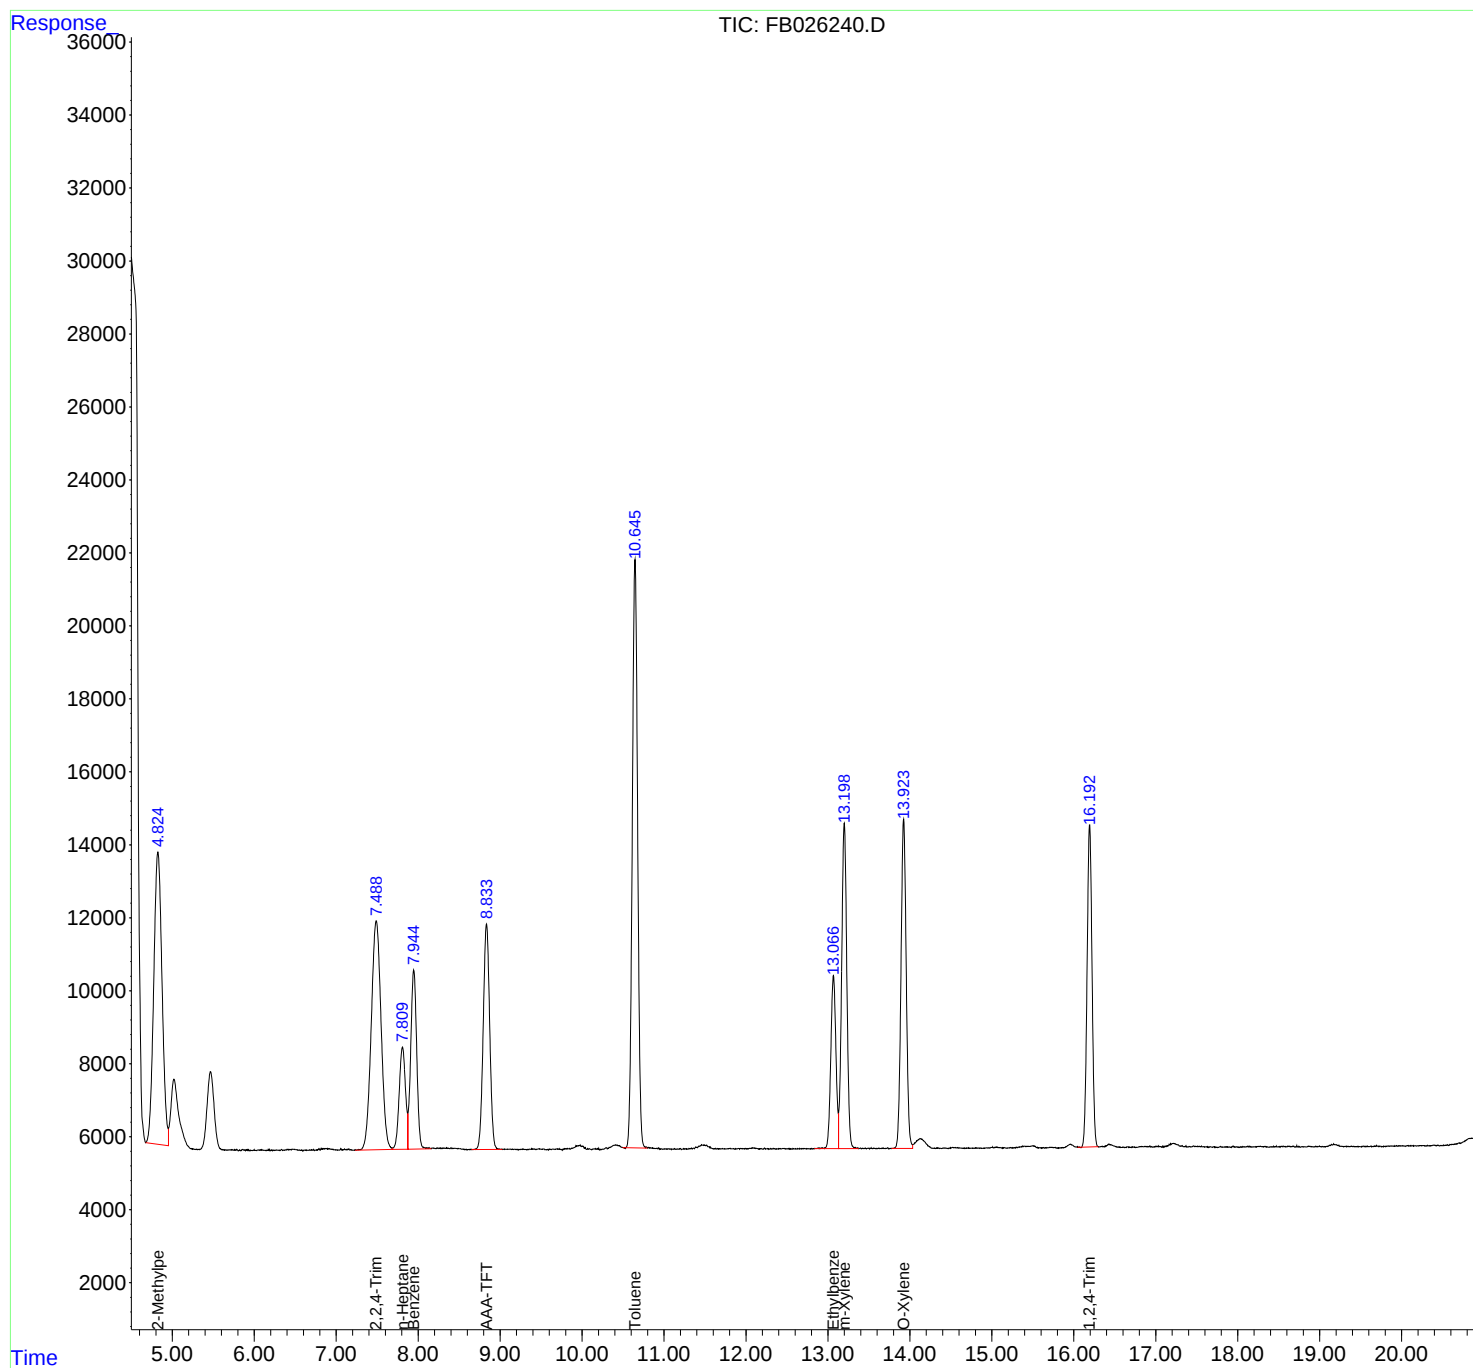

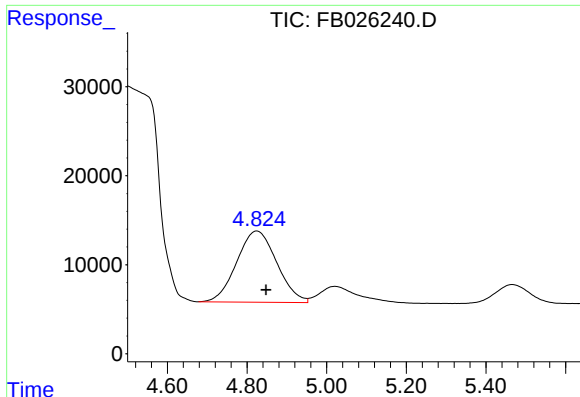


#1 2-Methylpentane

R.T.: 4.825 min
Delta R.T.: -0.023 min
Response: 559727
Conc: 25.19 ng/ml

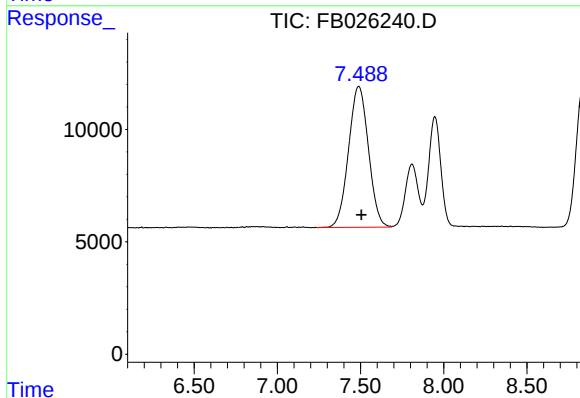


#2 2,2,4-Trimethylpentane

R.T.: 7.489 min
Delta R.T.: -0.017 min
Response: 521098
Conc: 23.44 ng/ml

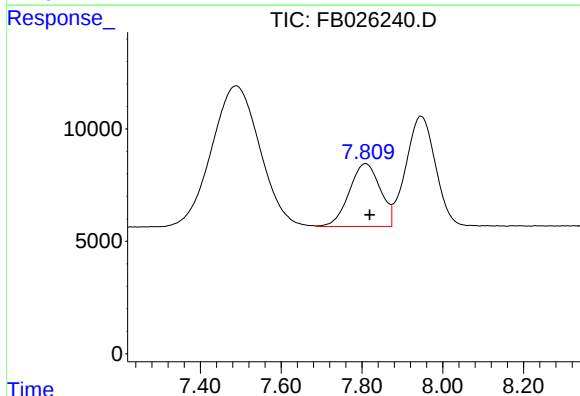


#3 n-Heptane

R.T.: 7.809 min
Delta R.T.: -0.010 min
Response: 149455
Conc: 5.79 ng/ml

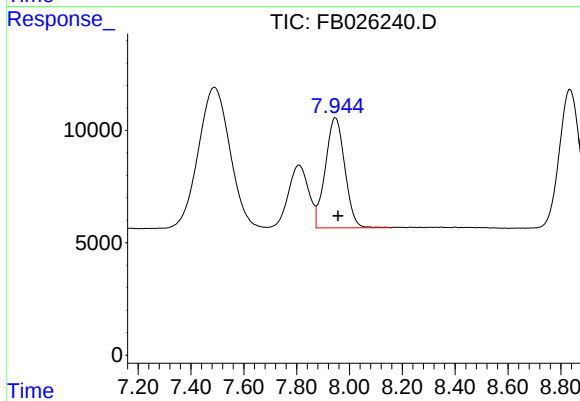


#4 Benzene

R.T.: 7.946 min
Delta R.T.: -0.011 min
Response: 250210
Conc: 9.19 ng/ml

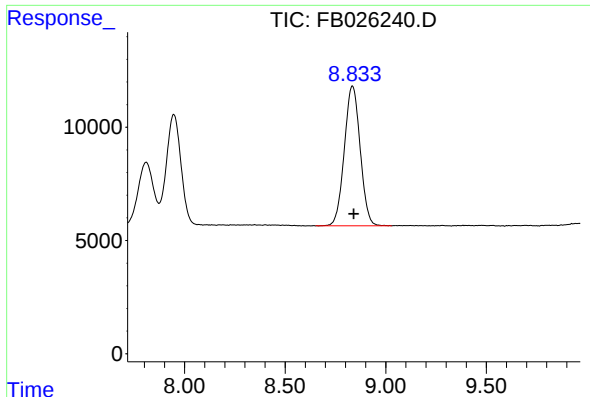


#5 AAA-TFT

R.T.: 8.835 min
Delta R.T.: -0.007 min
Response: 337437
Conc: 19.81 ng/ml

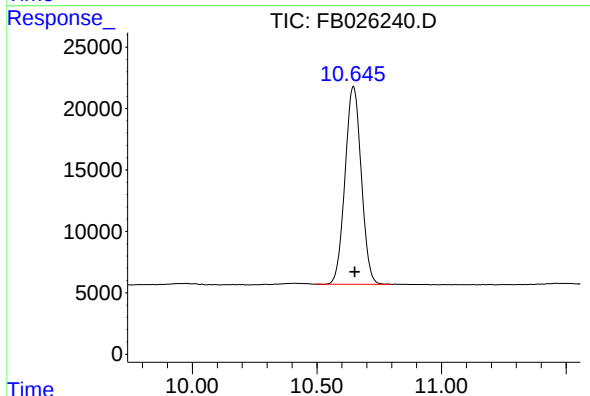


#6 Toluene

R.T.: 10.647 min
Delta R.T.: -0.005 min
Response: 729642
Conc: 27.84 ng/ml

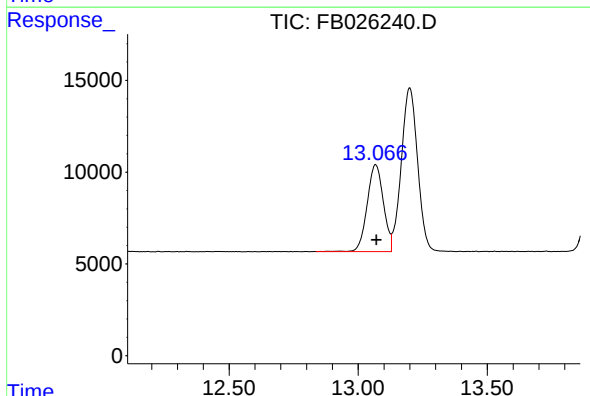


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.003 min
Response: 206081
Conc: 9.04 ng/ml

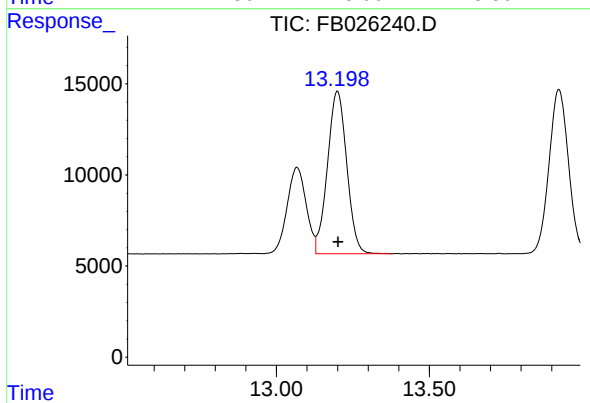


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.002 min
Response: 391302
Conc: 17.45 ng/ml

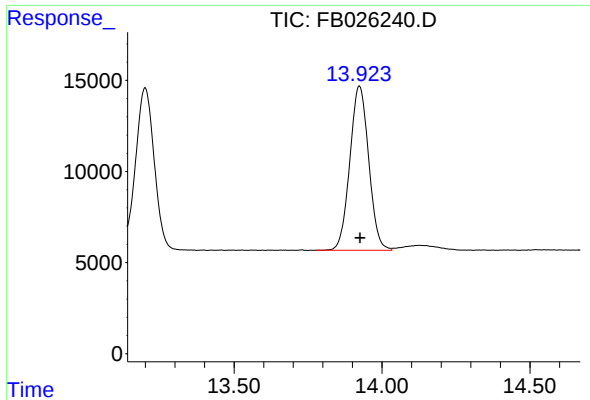

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.002 min
Response: 398825
Conc: 18.78 ng/ml

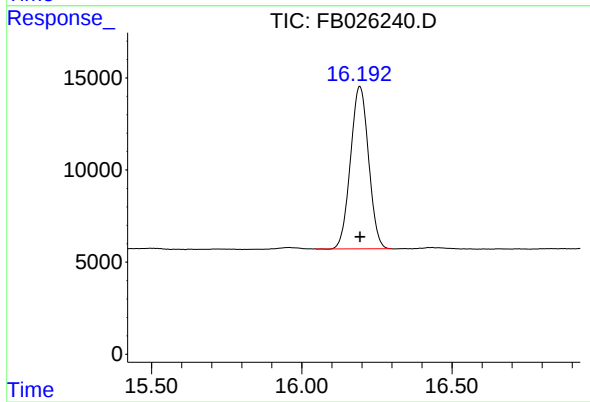

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 369104
Conc: 16.37 ng/ml