

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092121\
 Data File : FB026241.D
 Signal(s) : FID2B.CH
 Acq On : 21 Sep 2021 17:29
 Operator : AJ/MA
 Sample : M3823-03MSD
 Misc : 5.06G/5.00ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Sep 22 01:08:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
 Quant Title :
 QLast Update : Thu Sep 16 16:24:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.841	286681	16.833 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.842	409946	18.451 ng/ml
2) t 2,2,4-Trimethylpentane	7.497	366963	16.510 ng/ml
3) t n-Heptane	7.817	112302	4.349 ng/ml
4) t Benzene	7.956	198707	7.296 ng/ml
6) t Toluene	10.651	583705	22.271 ng/ml
7) t Ethylbenzene	13.070	160628	7.044 ng/ml
8) t m-Xylene	13.202	309620	13.811 ng/ml
9) t O-Xylene	13.926	324104	15.263 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	297412	13.189 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092121\
Data File : FB026241.D
Signal(s) : FID2B.CH
Acq On : 21 Sep 2021 17:29
Operator : AJ/MA
Sample : M3823-03MSD
Misc : 5.06G/5.00ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Sep 22 01:08:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091621.M
Quant Title :
QLast Update : Thu Sep 16 16:24:36 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

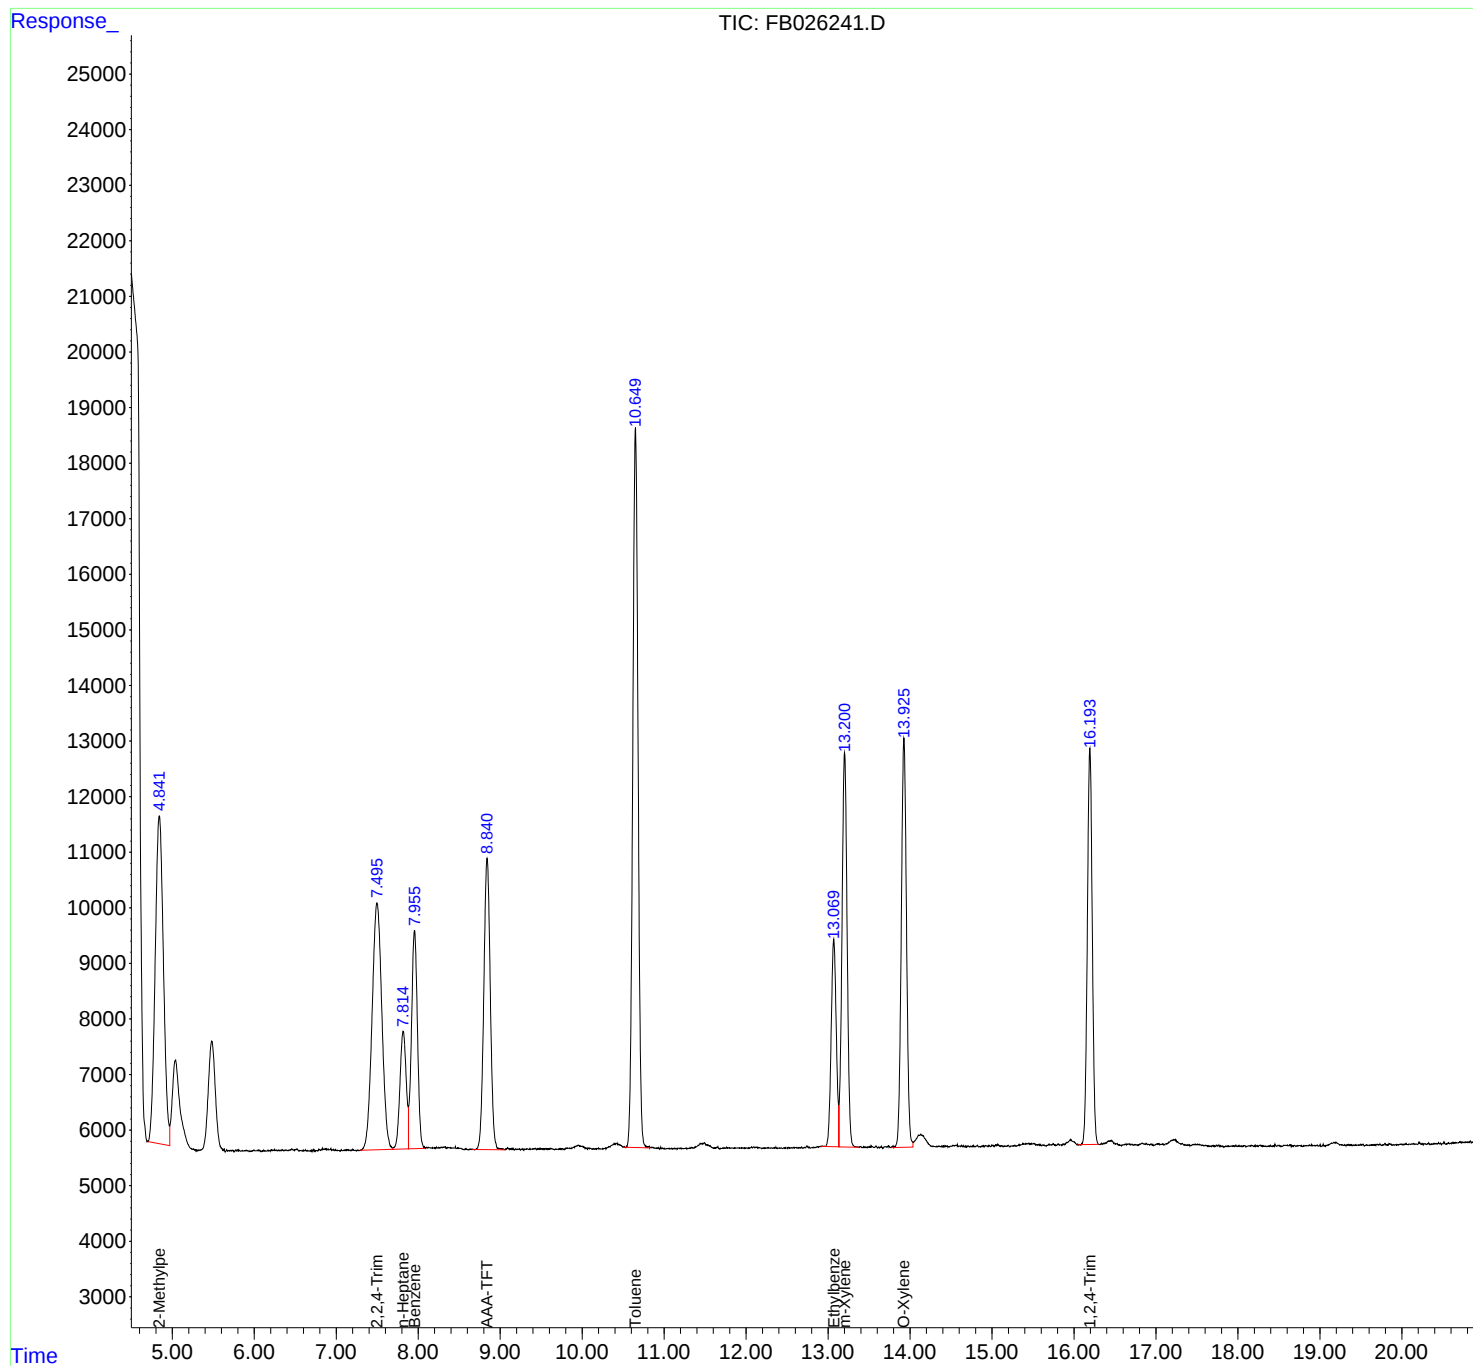

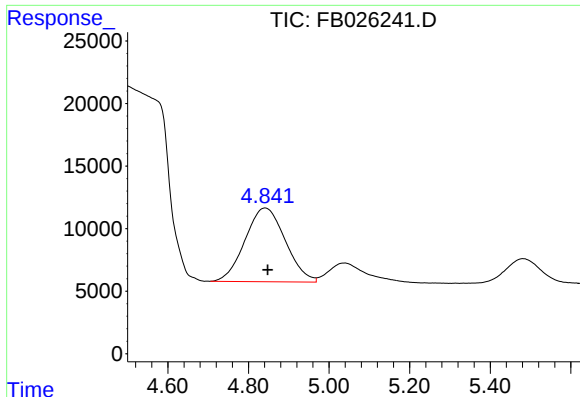


#1 2-Methylpentane

R.T.: 4.842 min
Delta R.T.: -0.006 min
Response: 409946
Conc: 18.45 ng/ml

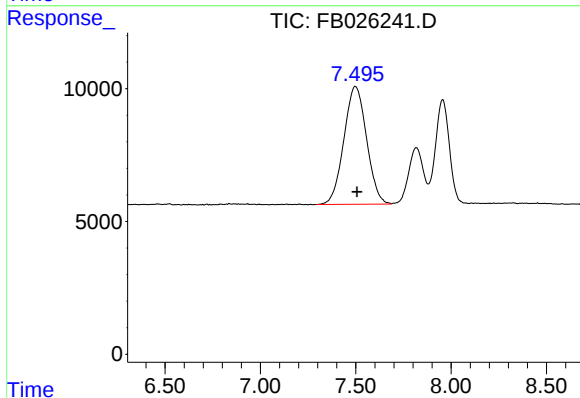


#2 2,2,4-Trimethylpentane

R.T.: 7.497 min
Delta R.T.: -0.010 min
Response: 366963
Conc: 16.51 ng/ml

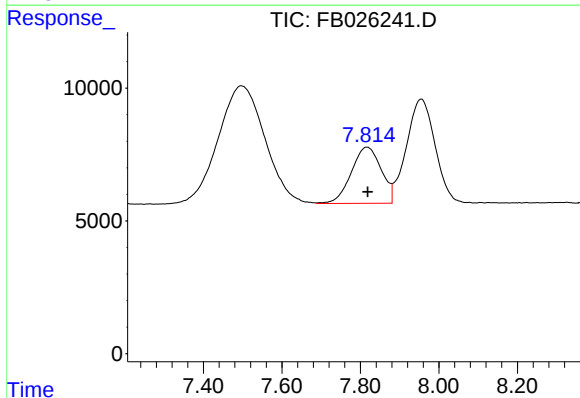


#3 n-Heptane

R.T.: 7.817 min
Delta R.T.: -0.002 min
Response: 112302
Conc: 4.35 ng/ml

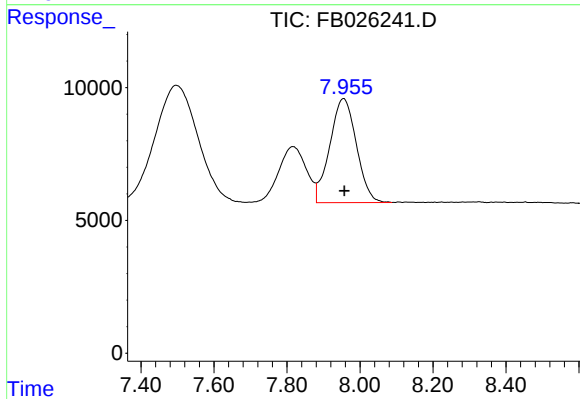


#4 Benzene

R.T.: 7.956 min
Delta R.T.: -0.001 min
Response: 198707
Conc: 7.30 ng/ml

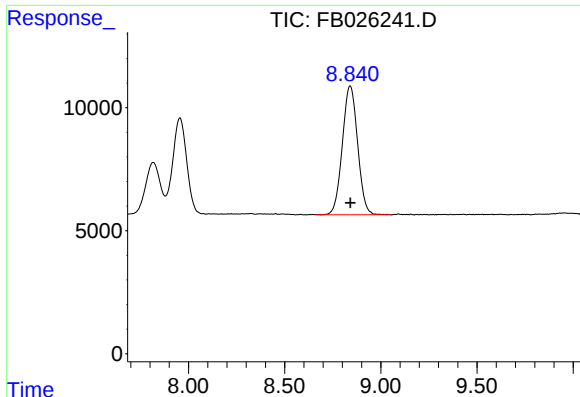


#5 AAA-TFT

R.T.: 8.841 min
Delta R.T.: -0.001 min
Response: 286681
Conc: 16.83 ng/ml

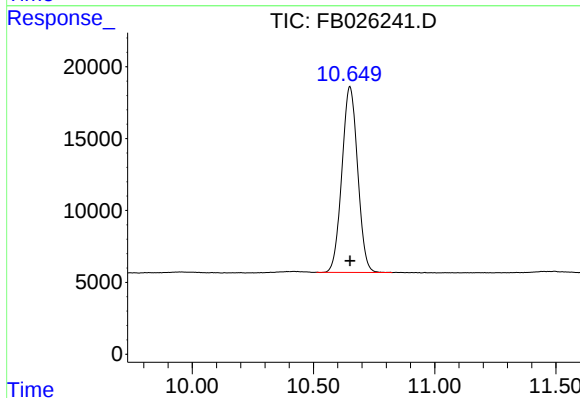


#6 Toluene

R.T.: 10.651 min
Delta R.T.: 0.000 min
Response: 583705
Conc: 22.27 ng/ml

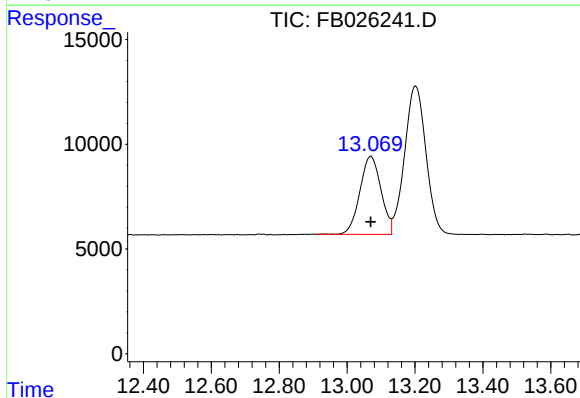


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 160628
Conc: 7.04 ng/ml

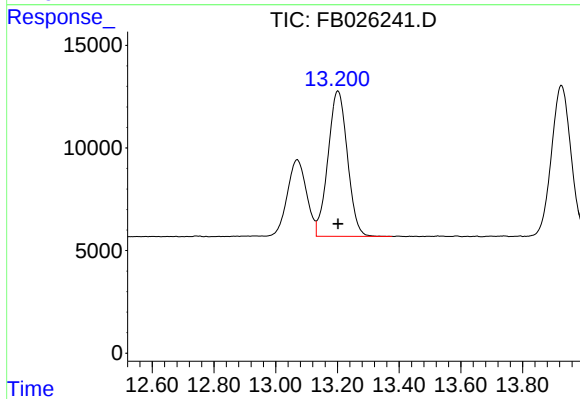


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 309620
Conc: 13.81 ng/ml

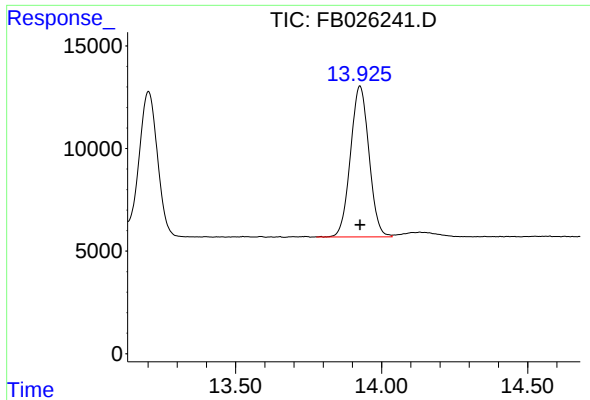

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.000 min
Response: 324104
Conc: 15.26 ng/ml

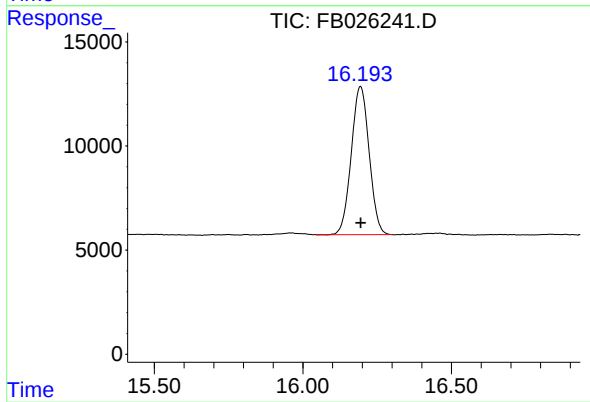

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 297412
Conc: 13.19 ng/ml