

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092222\
 Data File : FB028392.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2022 3:00
 Operator : AJ/MA
 Sample : N4724-16MS 50X
 Misc : 5.02G/5.00 ML MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-07-COMPMS

Integration File: Calibration.e
 Quant Time: Sep 23 05:15:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	260184	21.738 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	603038	29.784 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	639044	30.378 ng/ml
3) t n-Heptane	7.752	219206	10.197 ng/ml
4) t Benzene	7.889	279582	11.365 ng/ml
6) t Toluene	10.623	776927	33.371 ng/ml
7) t Ethylbenzene	13.060	236660	10.642 ng/ml
8) t m-Xylene	13.193	465360	21.325 ng/ml
9) t O-Xylene	13.920	449181	21.439 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	406377	20.211 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092222\
Data File : FB028392.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2022 3:00
Operator : AJ/MA
Sample : N4724-16MS 50X
Misc : 5.02G/5.00 ML MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

Integration File: Calibration.e
Quant Time: Sep 23 05:15:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

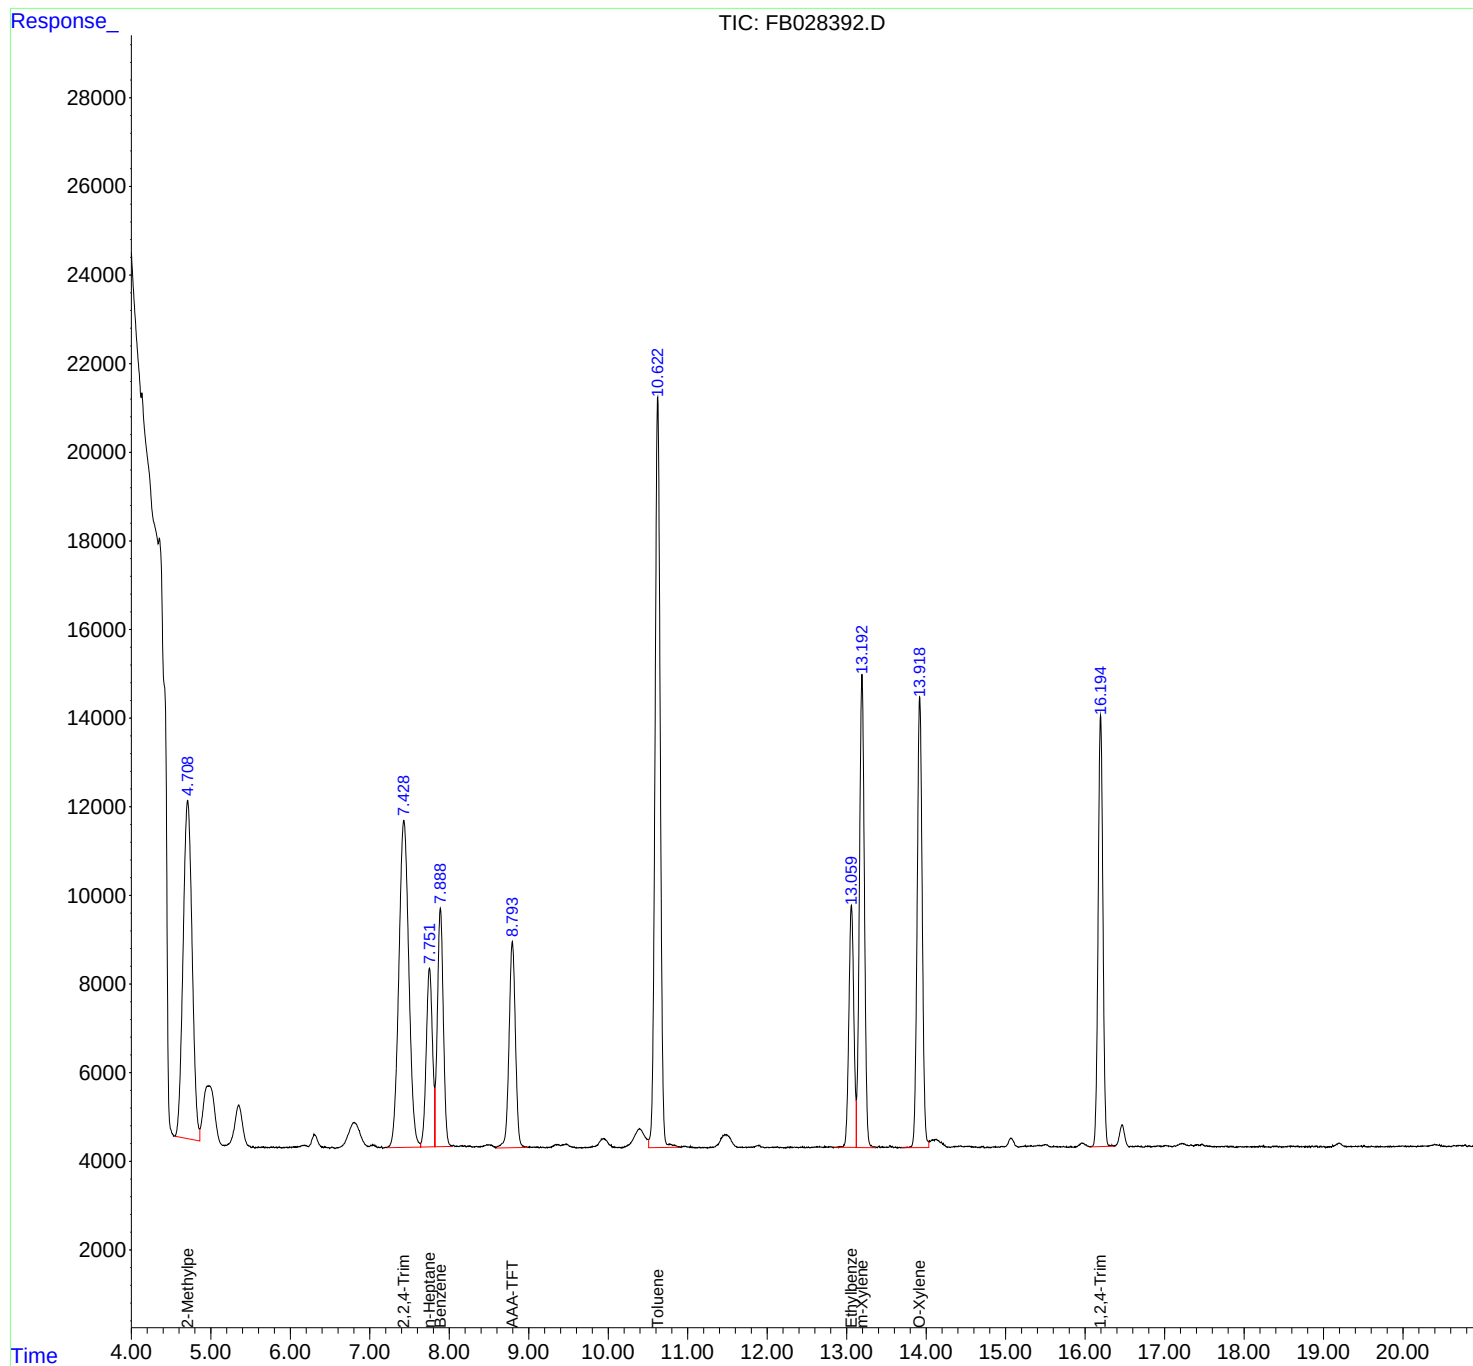


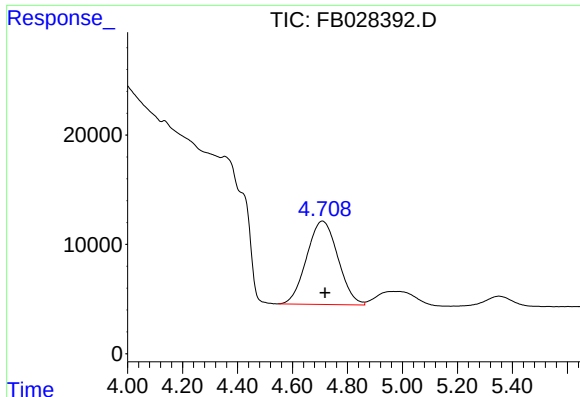

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: -0.009 min
Response: 603038
Conc: 29.78 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

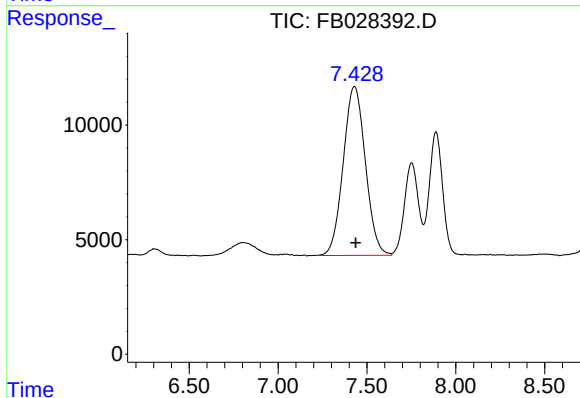


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: -0.007 min
Response: 639044
Conc: 30.38 ng/ml

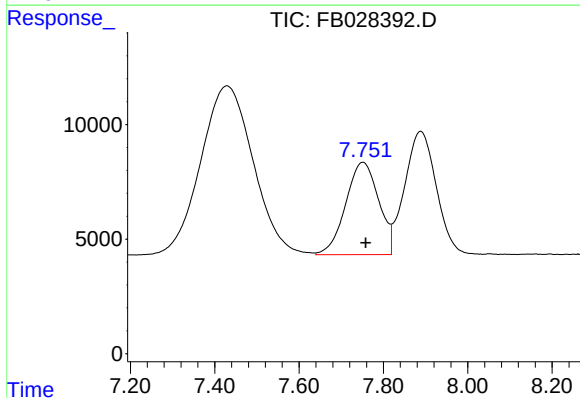


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 219206
Conc: 10.20 ng/ml

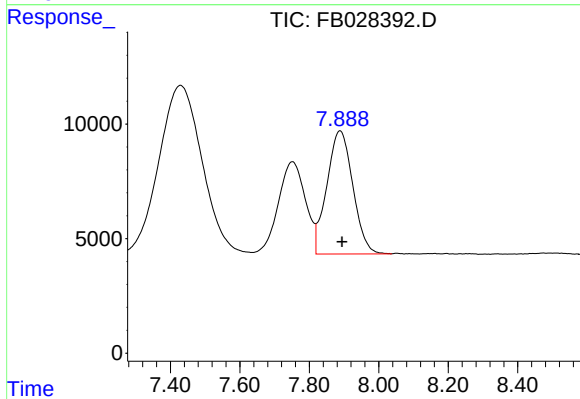

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.006 min
Response: 279582
Conc: 11.36 ng/ml

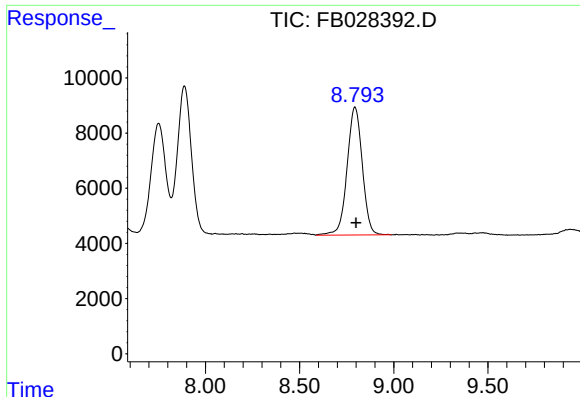

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.006 min
Response: 260184
Conc: 21.74 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

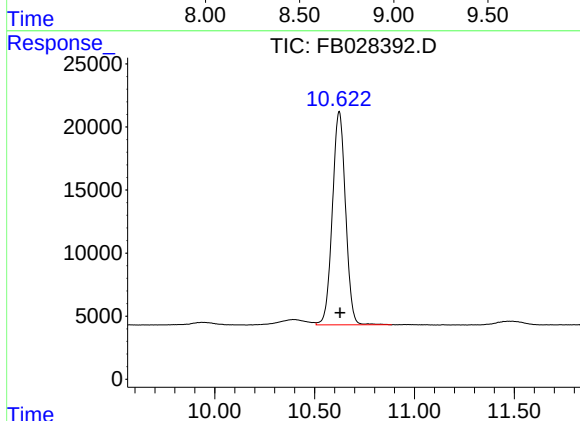


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.005 min
Response: 776927
Conc: 33.37 ng/ml

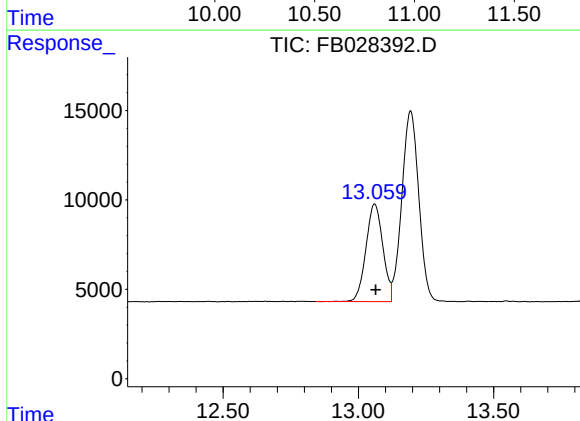


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.004 min
Response: 236660
Conc: 10.64 ng/ml

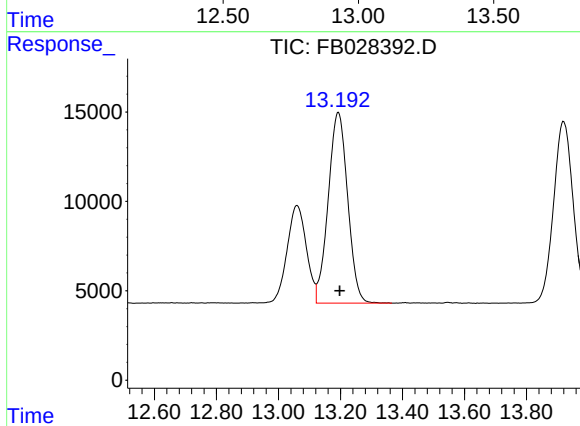

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.004 min
Response: 465360
Conc: 21.32 ng/ml

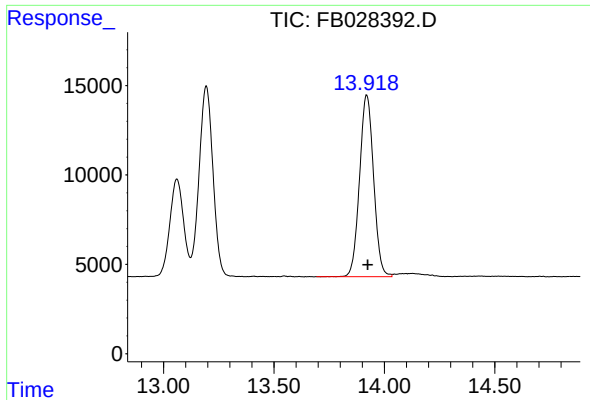

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 449181
Conc: 21.44 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

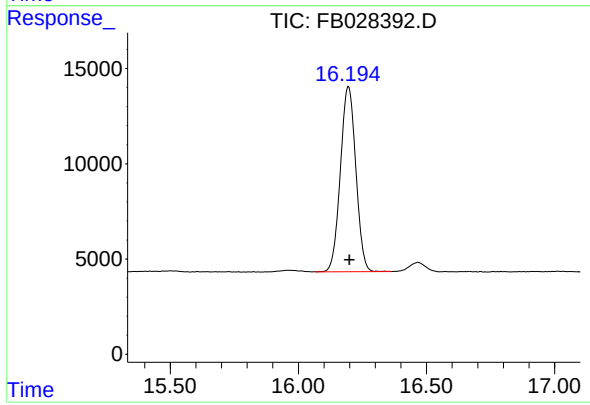

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.004 min
Response: 406377
Conc: 20.21 ng/ml