

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092222\
 Data File : FB028393.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2022 3:37
 Operator : AJ/MA
 Sample : N4724-16MSD 50X
 Misc : 5.08G/5.00 ML MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-07-COMPMSD

Integration File: Calibration.e
 Quant Time: Sep 23 05:15:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	245487	20.511 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	568091	28.058 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	594978	28.284 ng/ml
3) t n-Heptane	7.751	208588	9.703 ng/ml
4) t Benzene	7.888	255270	10.376 ng/ml
6) t Toluene	10.622	710006	30.497 ng/ml
7) t Ethylbenzene	13.060	219457	9.868 ng/ml
8) t m-Xylene	13.192	431952	19.794 ng/ml
9) t O-Xylene	13.920	414200	19.769 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	373145	18.558 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092222\
Data File : FB028393.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2022 3:37
Operator : AJ/MA
Sample : N4724-16MSD 50X
Misc : 5.08G/5.00 ML MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMSD

Integration File: Calibration.e
Quant Time: Sep 23 05:15:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

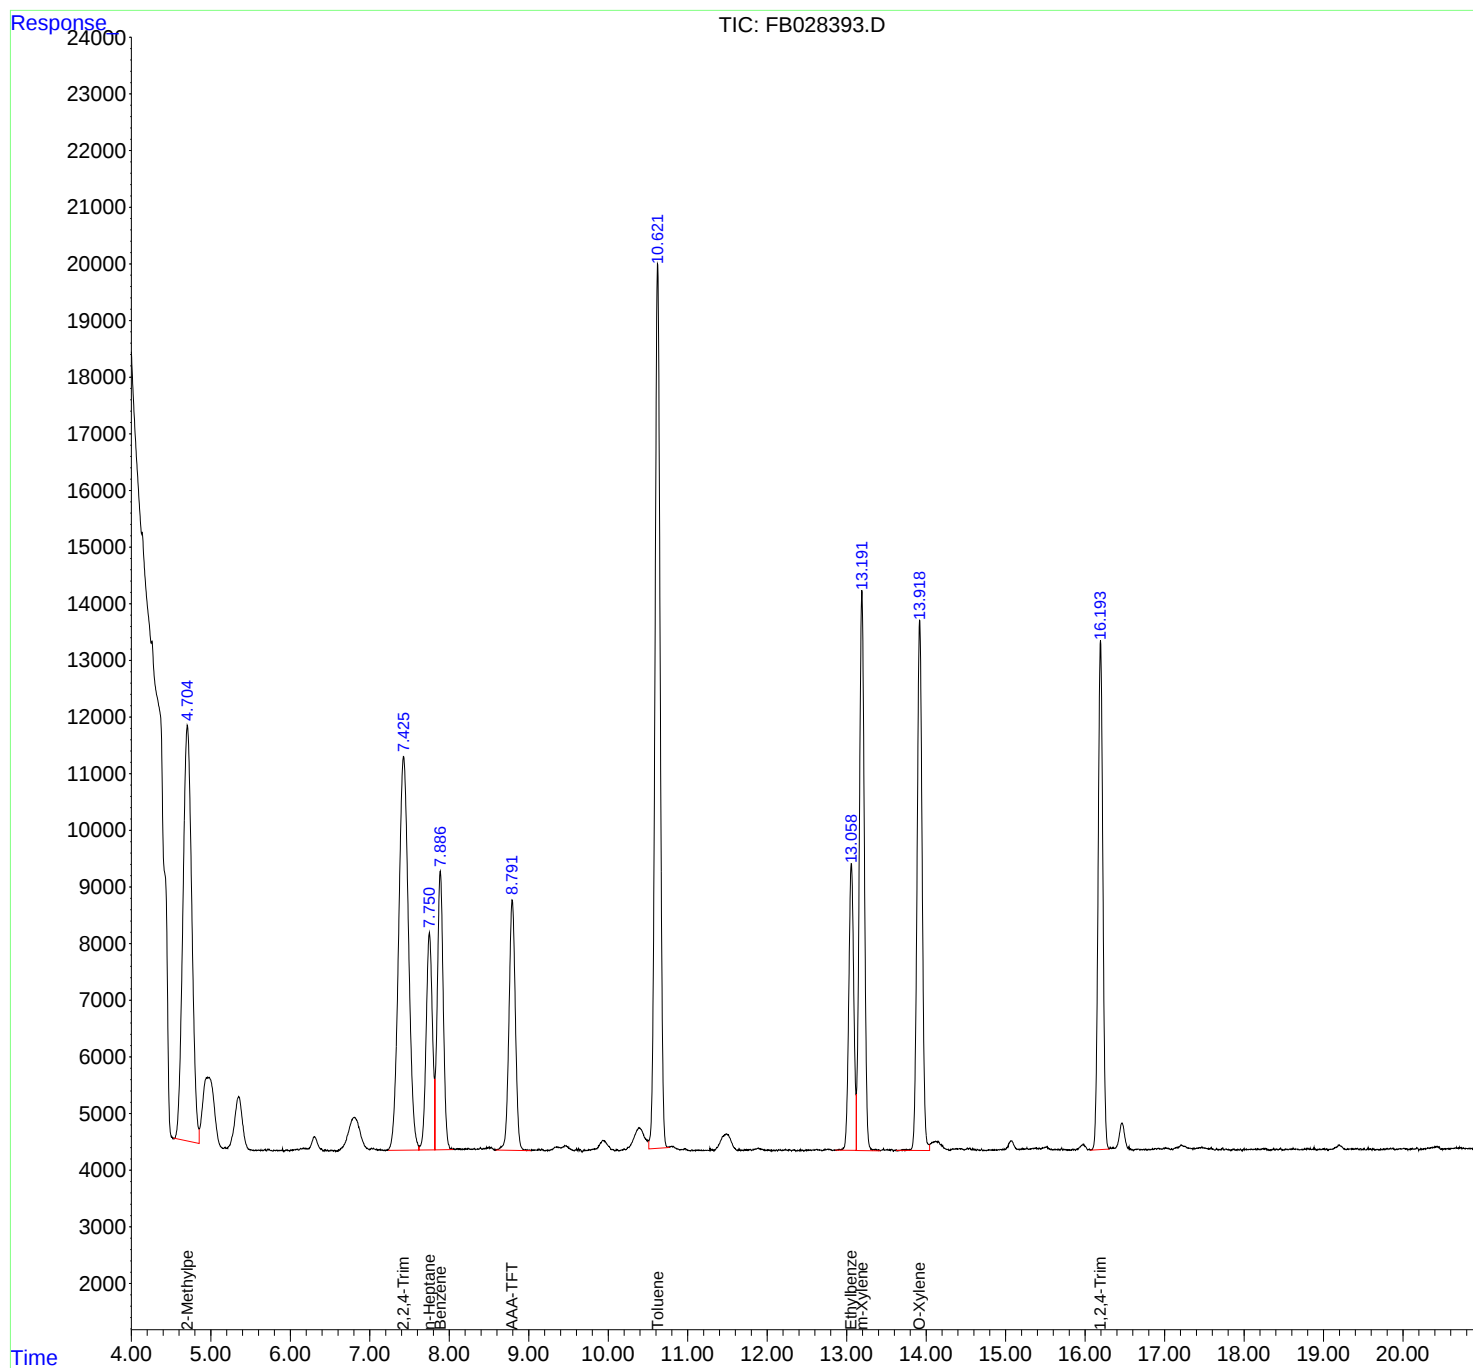


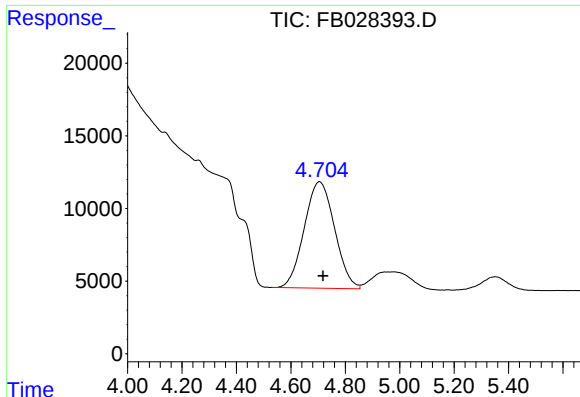

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.012 min
Response: 568091
Conc: 28.06 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMSD

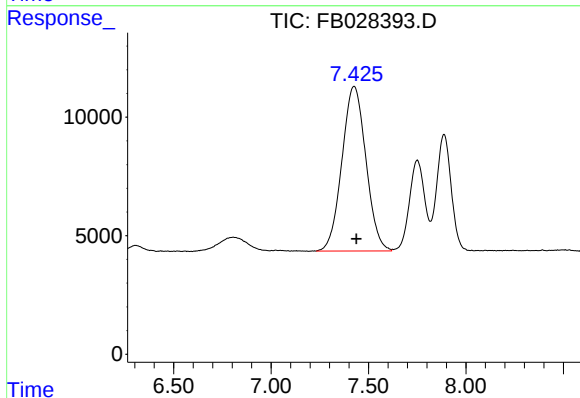


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: -0.011 min
Response: 594978
Conc: 28.28 ng/ml

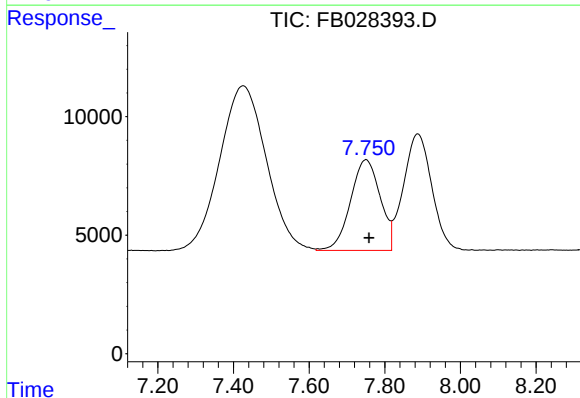


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.007 min
Response: 208588
Conc: 9.70 ng/ml

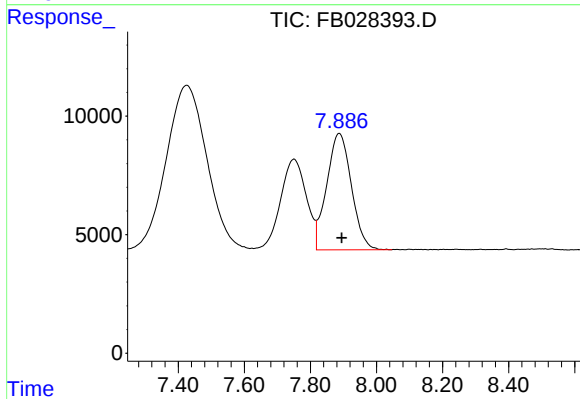

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.007 min
Response: 255270
Conc: 10.38 ng/ml

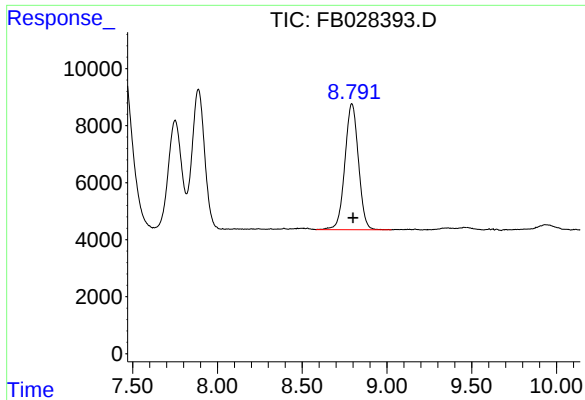

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.007 min
Response: 245487
Conc: 20.51 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMSD

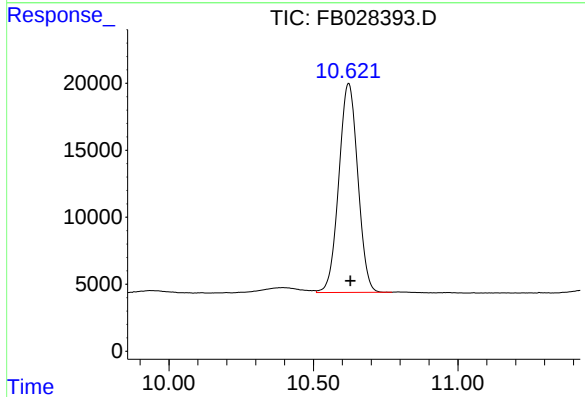


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.006 min
Response: 710006
Conc: 30.50 ng/ml

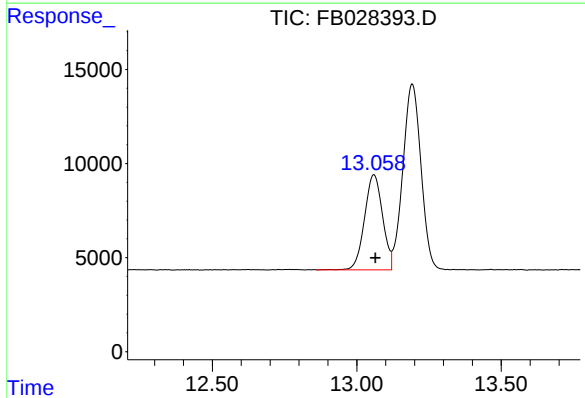


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.005 min
Response: 219457
Conc: 9.87 ng/ml

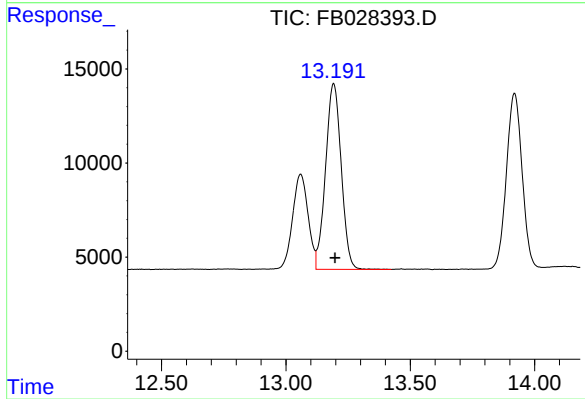

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.005 min
Response: 431952
Conc: 19.79 ng/ml

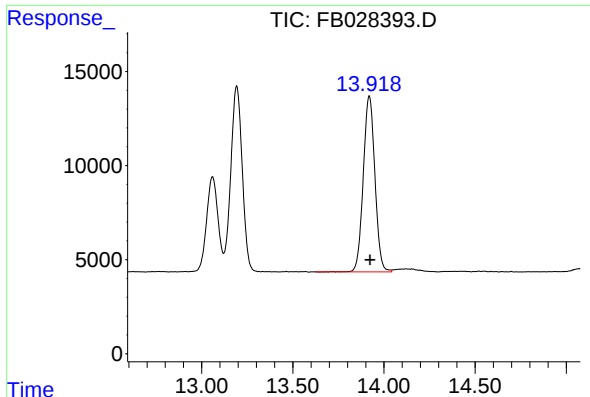

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 414200
Conc: 19.77 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMSD

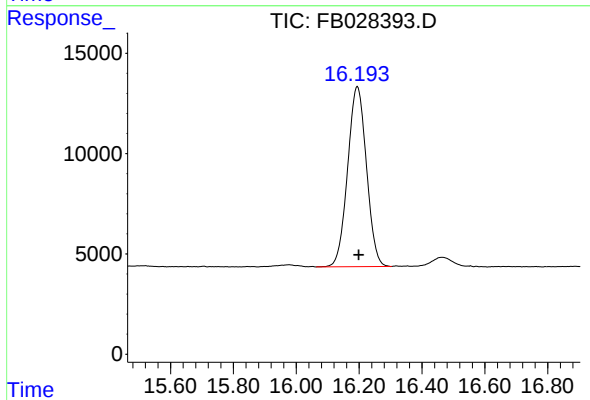

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.004 min
Response: 373145
Conc: 18.56 ng/ml