

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092320\
 Data File : FB024925.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2020 10:00
 Operator : DD/AJ
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 23 11:17:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:17:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	380954	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	802698	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	807624	30.000 ng/ml
3) t n-Heptane	7.759	267727	10.000 ng/ml
4) t Benzene	7.895	349240	10.000 ng/ml
6) t Toluene	10.632	975145	30.000 ng/ml
7) t Ethylbenzene	13.071	301635	10.000 ng/ml
8) t m-Xylene	13.204	599192	20.000 ng/ml
9) t O-Xylene	13.932	578524	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	482913	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092320\
Data File : FB024925.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2020 10:00
Operator : DD/AJ
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 23 11:17:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:17:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

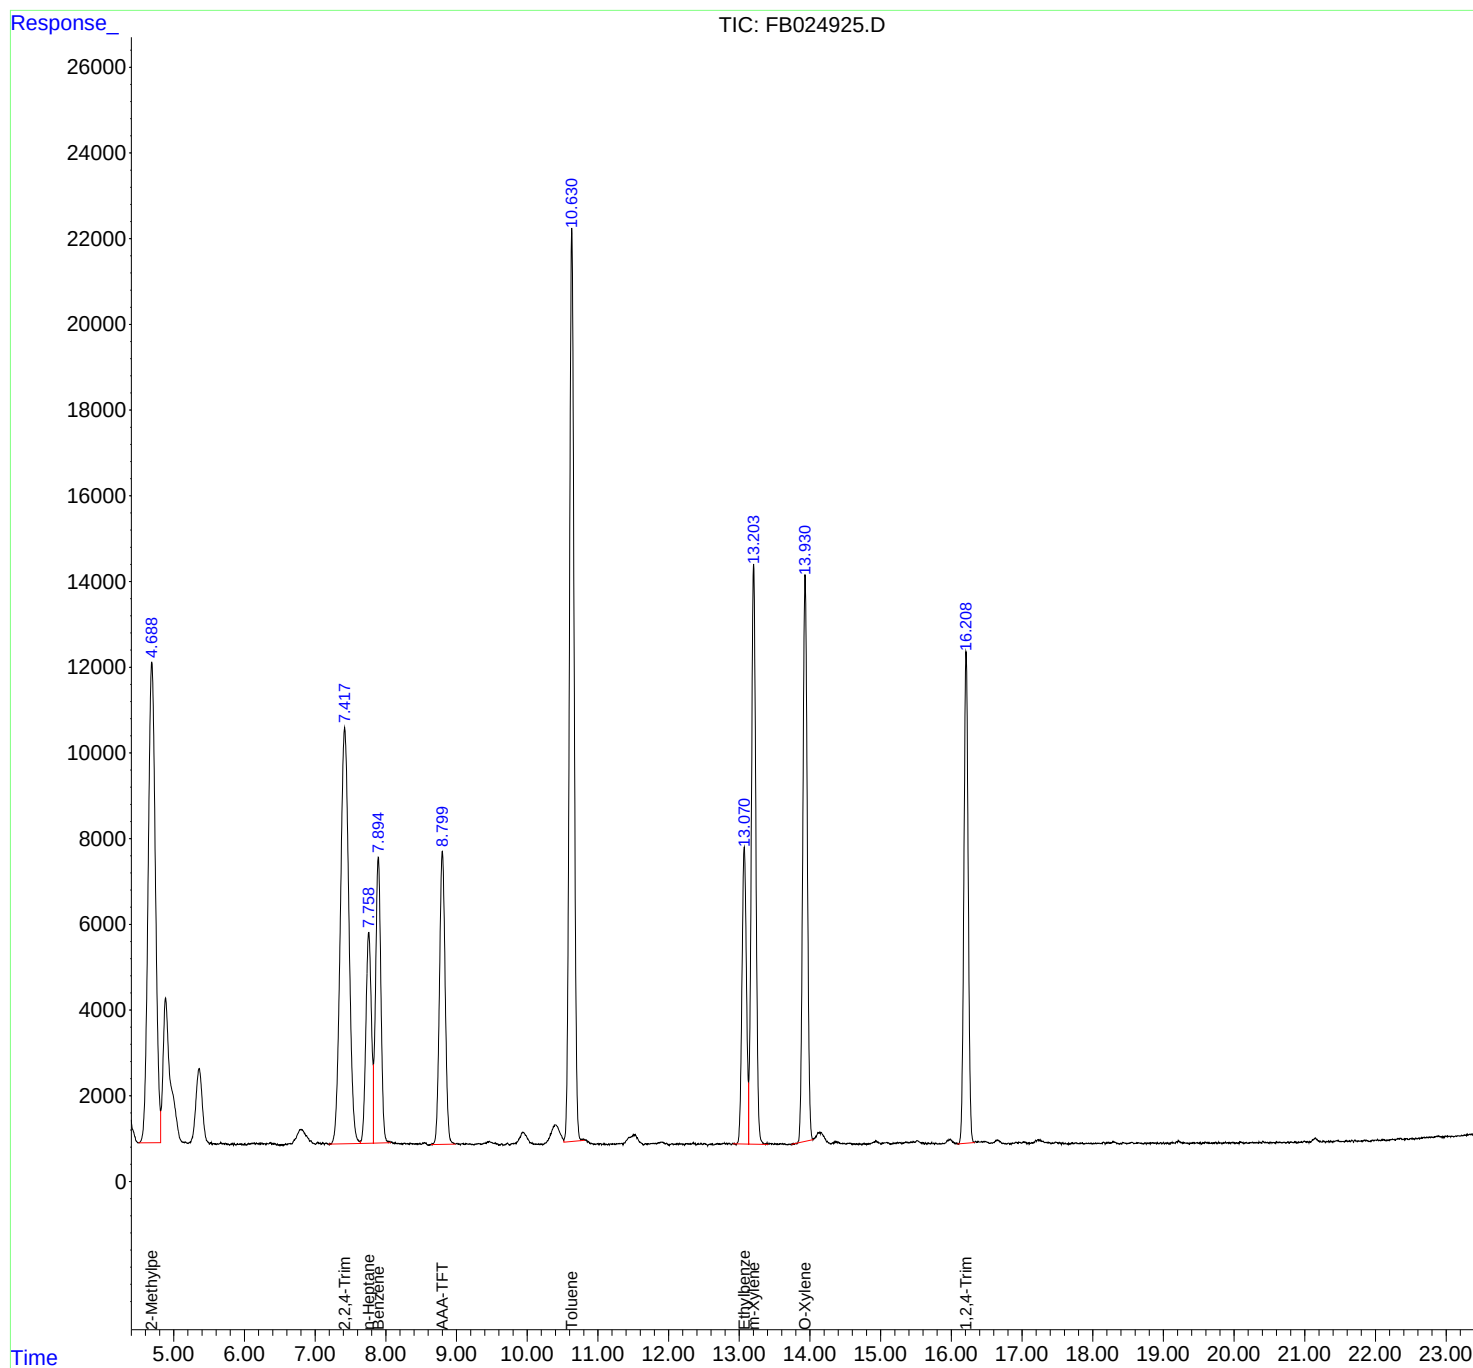


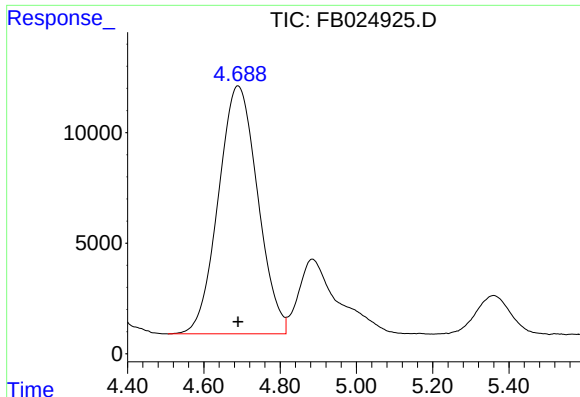

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 802698
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :

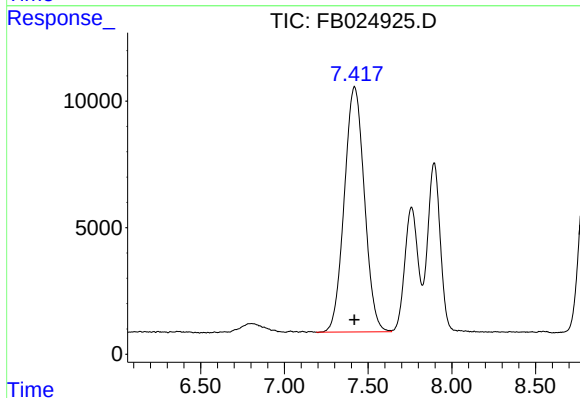


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 807624
Conc: 30.00 ng/ml

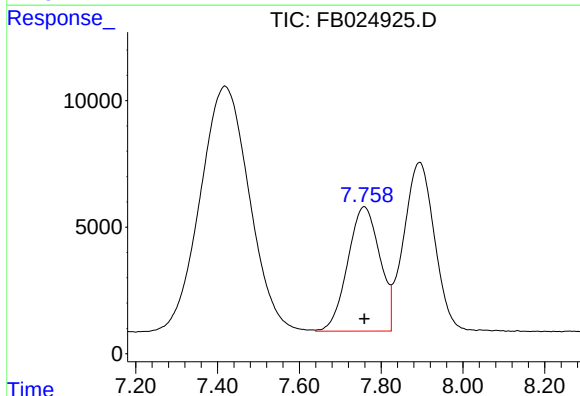


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 267727
Conc: 10.00 ng/ml

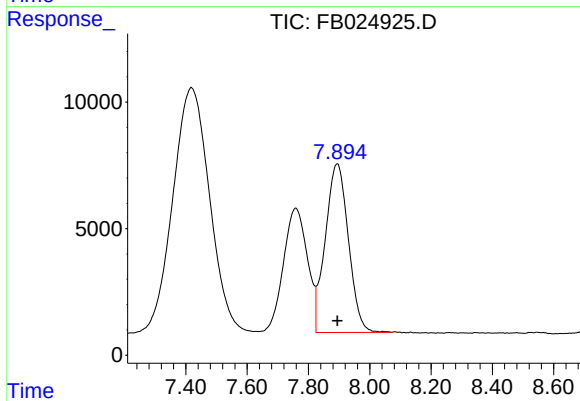

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 349240
Conc: 10.00 ng/ml

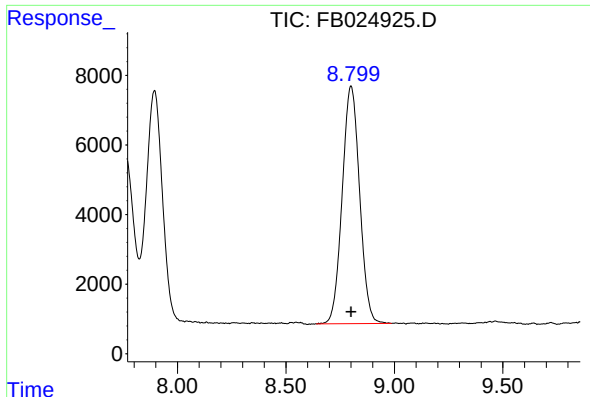

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 380954
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

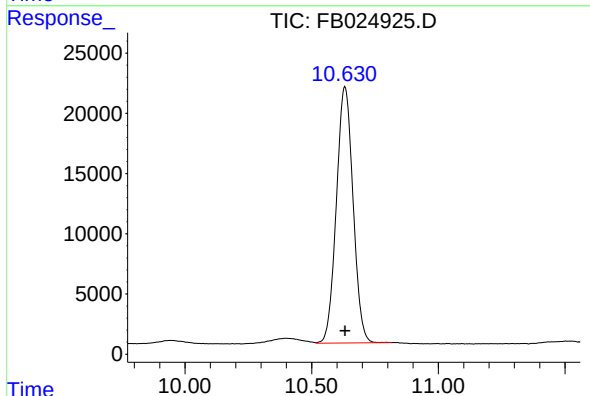


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 975145
Conc: 30.00 ng/ml

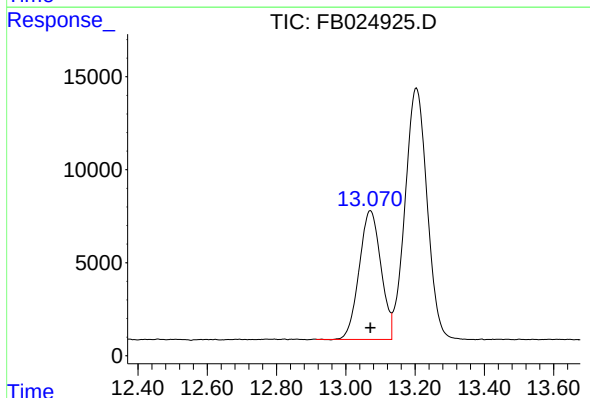


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 301635
Conc: 10.00 ng/ml

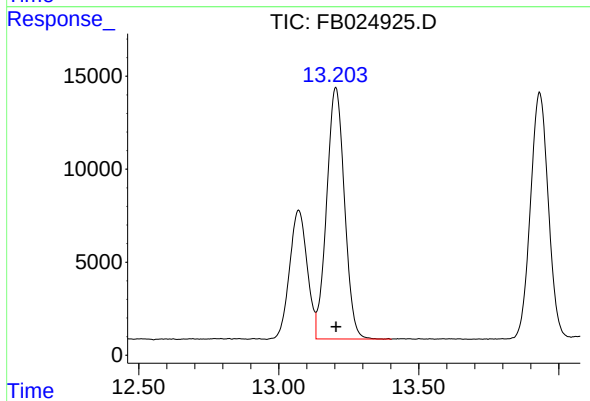

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 599192
Conc: 20.00 ng/ml

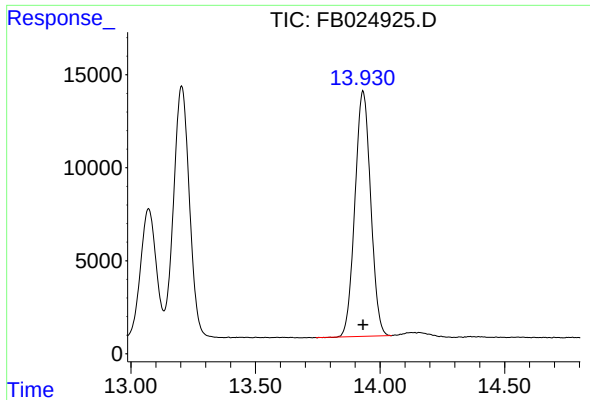

#9 O-Xylene


R.T.: 13.932 min

Delta R.T.: 0.000 min

Response: 578524

Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

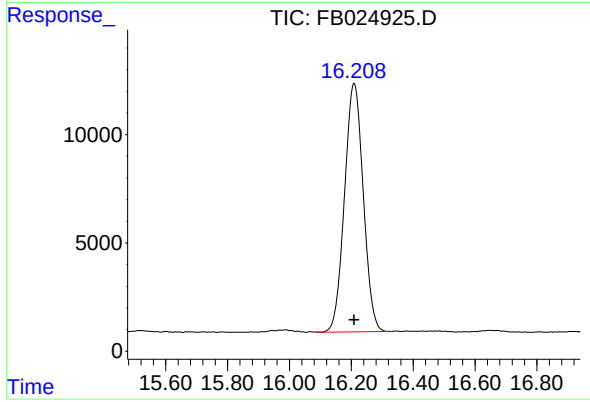

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min

Delta R.T.: 0.000 min

Response: 482913

Conc: 20.00 ng/ml