

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092320\
 Data File : FB024926.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2020 10:30
 Operator : DD/AJ
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 23 11:18:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:17:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	1038879	54.541 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	2326870	86.964 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	2432085	90.342 ng/ml
3) t n-Heptane	7.757	807272	30.153 ng/ml
4) t Benzene	7.892	952731	27.280 ng/ml
6) t Toluene	10.631	2696845	82.967 ng/ml
7) t Ethylbenzene	13.071	830484	27.533 ng/ml
8) t m-Xylene	13.204	1610100	53.742 ng/ml
9) t O-Xylene	13.932	1556727	53.817 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	1337287	55.384 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092320\
Data File : FB024926.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2020 10:30
Operator : DD/AJ
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 23 11:18:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:17:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

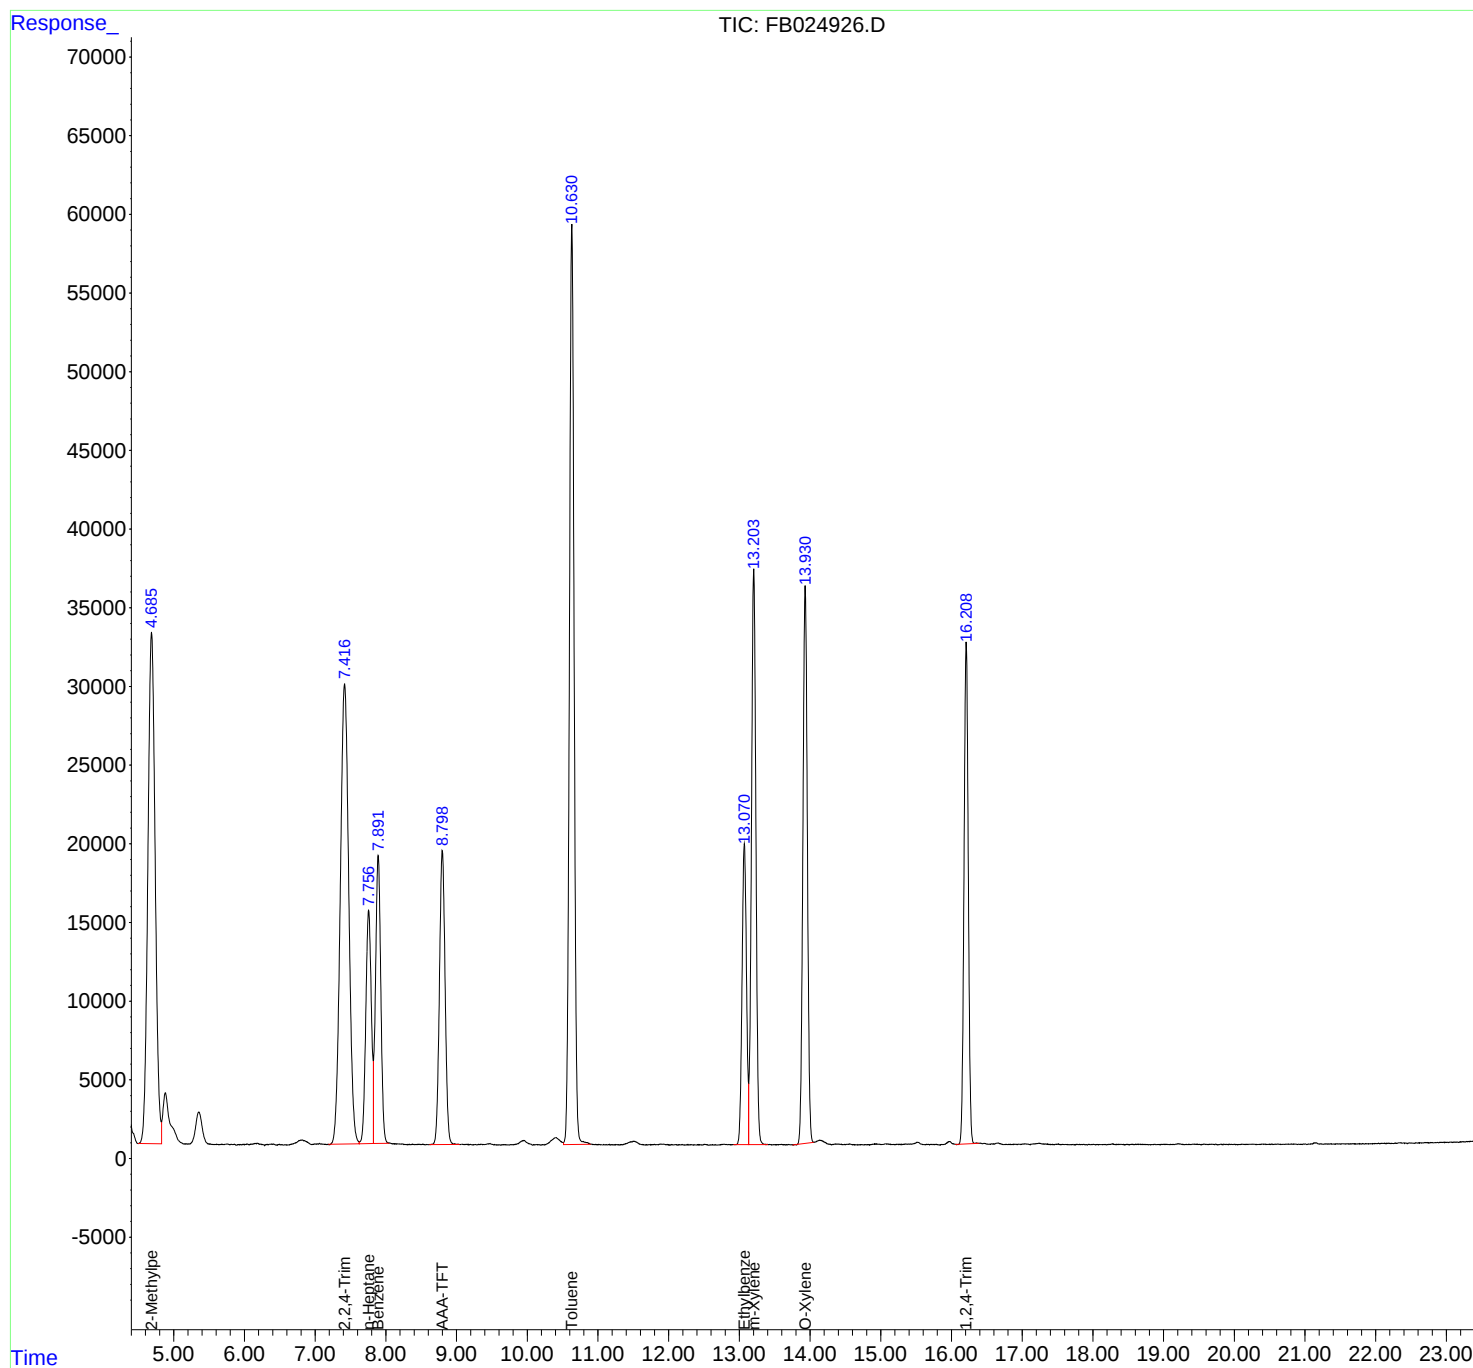


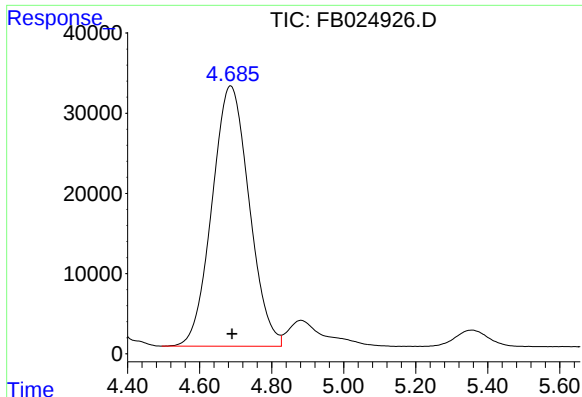

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.003 min
Response: 2326870
Conc: 86.96 ng/ml

Instrument :
FID_B
ClientSampleId :

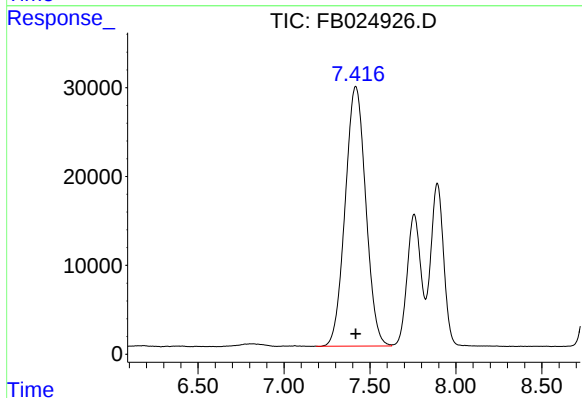


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 2432085
Conc: 90.34 ng/ml

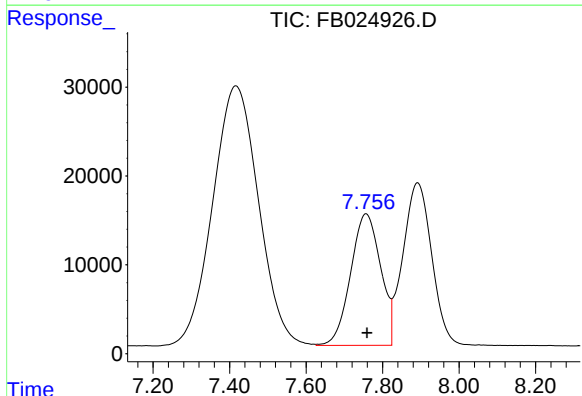


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 807272
Conc: 30.15 ng/ml

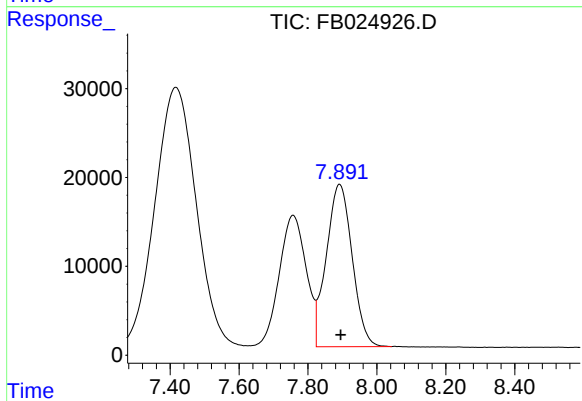

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 952731
Conc: 27.28 ng/ml

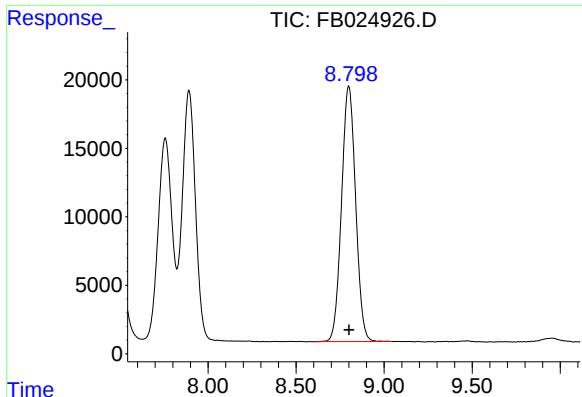

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: -0.001 min
Response: 1038879
Conc: 54.54 ng/ml

Instrument :
FID_B
ClientSampleId :

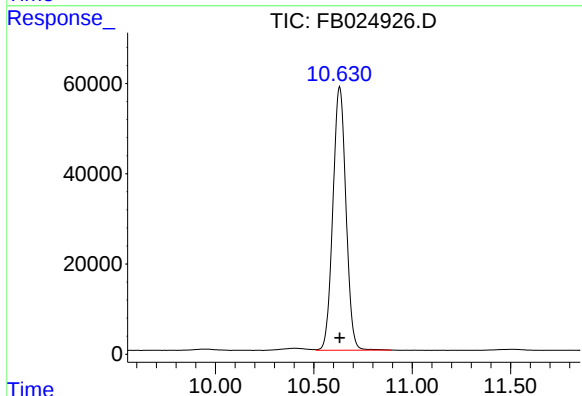


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 2696845
Conc: 82.97 ng/ml

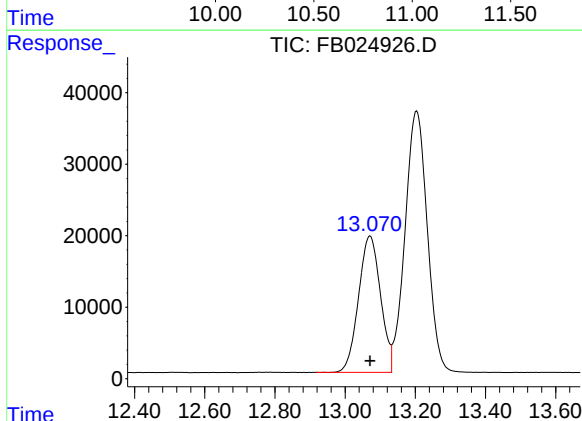


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 830484
Conc: 27.53 ng/ml

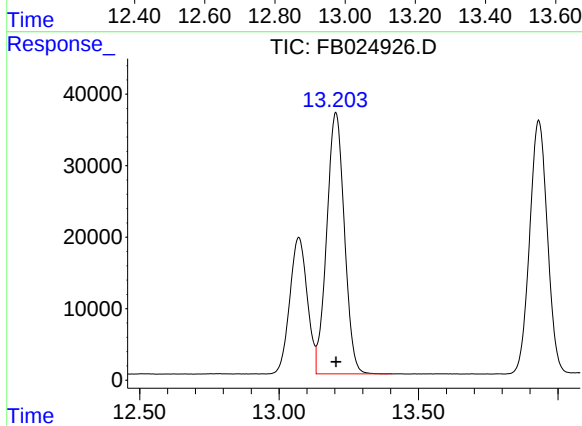

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 1610100
Conc: 53.74 ng/ml

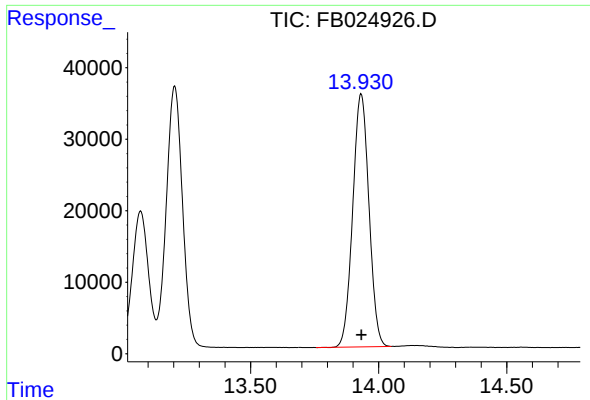

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 1556727
Conc: 53.82 ng/ml

Instrument :
FID_B
ClientSampleId :

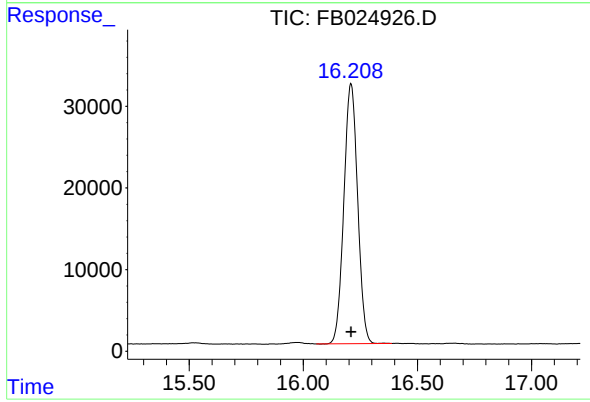

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 1337287
Conc: 55.38 ng/ml