

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092322\
 Data File : FB028403.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2022 11:12
 Operator : AJ/MA
 Sample : BSF0923S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0923S1

Integration File: Calibration.e
 Quant Time: Sep 24 15:40:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	262182	21.905 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	658279	32.512 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	677636	32.213 ng/ml
3) t n-Heptane	7.751	225805	10.504 ng/ml
4) t Benzene	7.888	259509	10.549 ng/ml
6) t Toluene	10.621	750468	32.235 ng/ml
7) t Ethylbenzene	13.058	240040	10.794 ng/ml
8) t m-Xylene	13.190	471709	21.616 ng/ml
9) t O-Xylene	13.917	452895	21.616 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	447792	22.270 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092322\
Data File : FB028403.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2022 11:12
Operator : AJ/MA
Sample : BSF0923S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0923S1

Integration File: Calibration.e
Quant Time: Sep 24 15:40:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

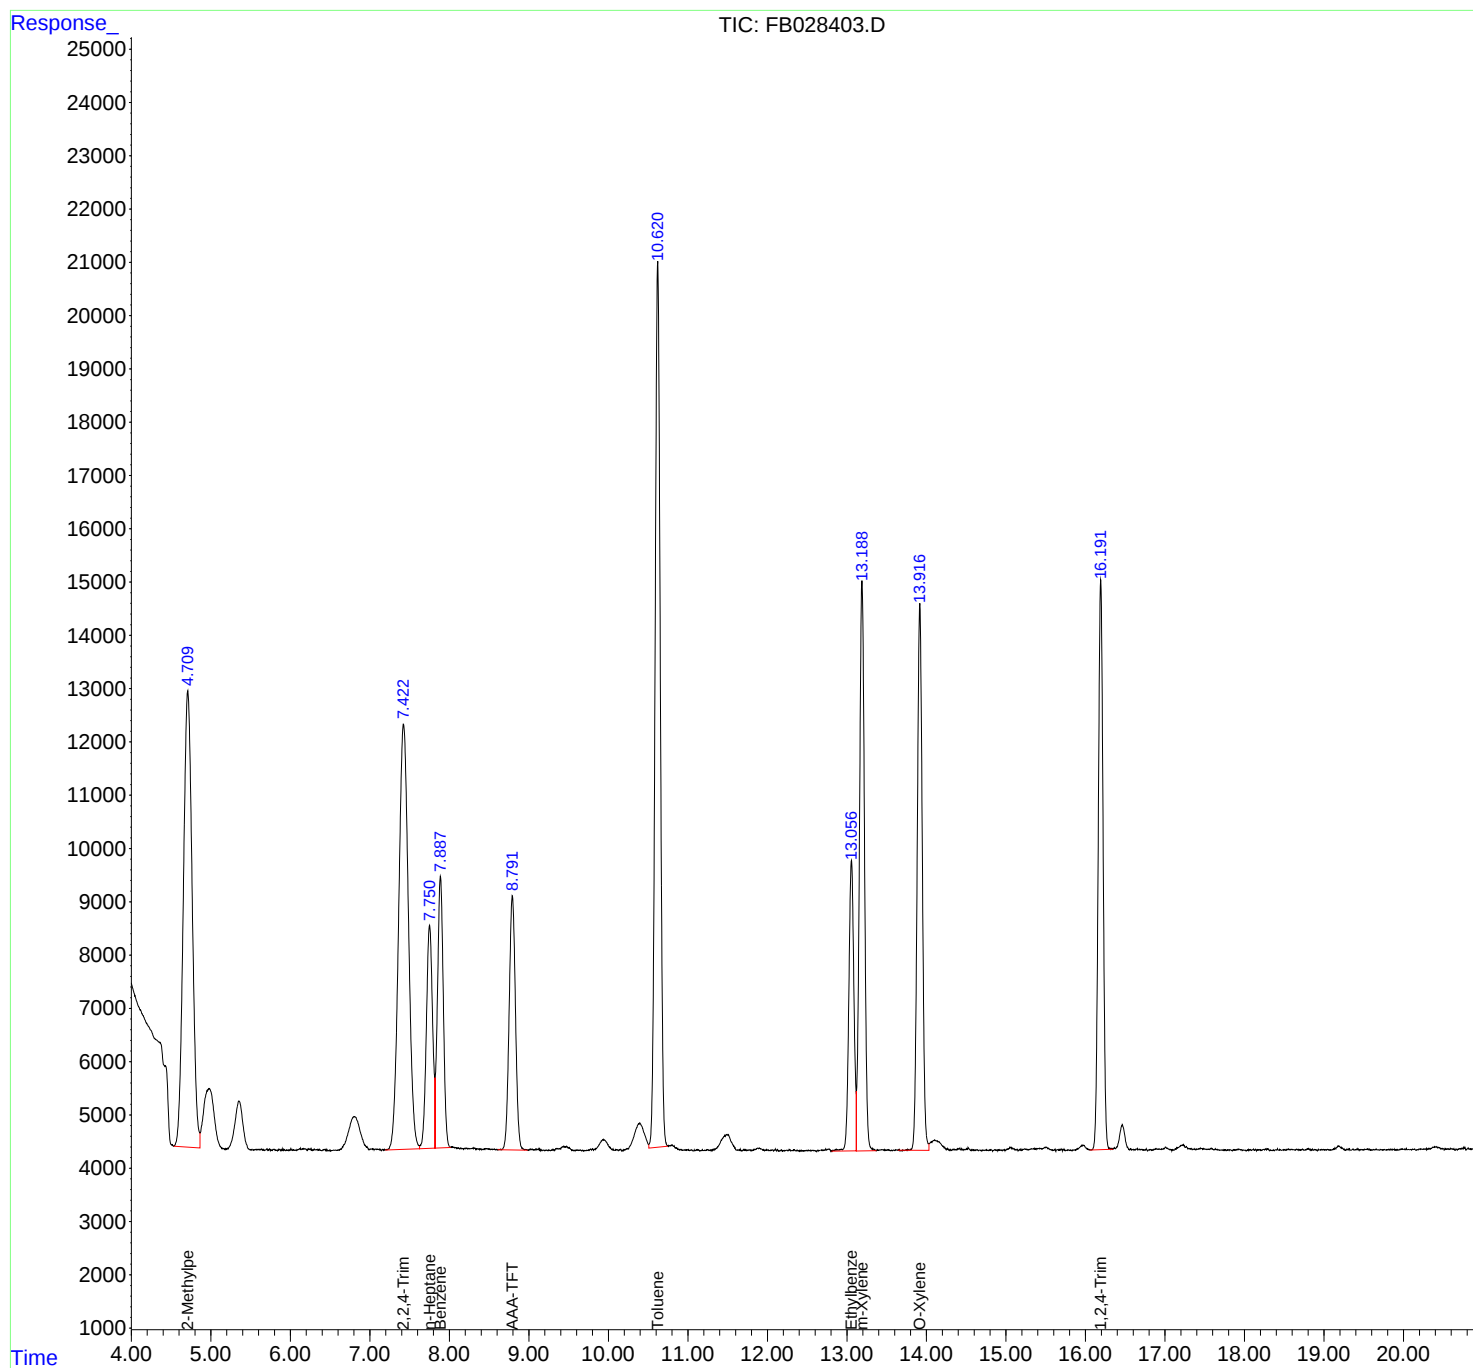


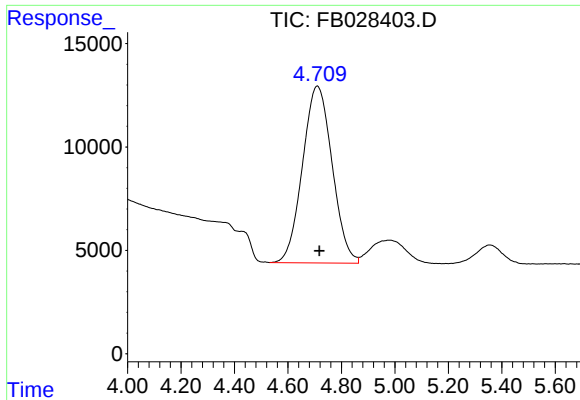

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: -0.007 min
Response: 658279
Conc: 32.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S1

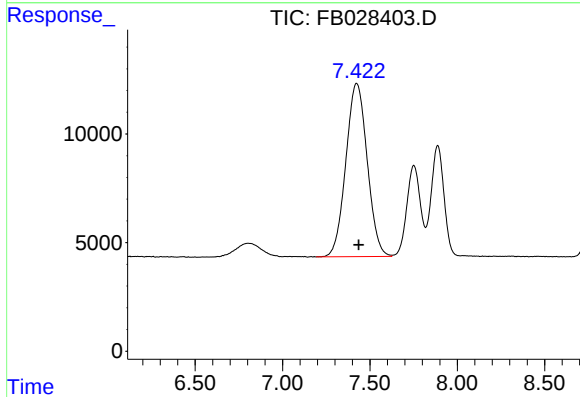


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.014 min
Response: 677636
Conc: 32.21 ng/ml

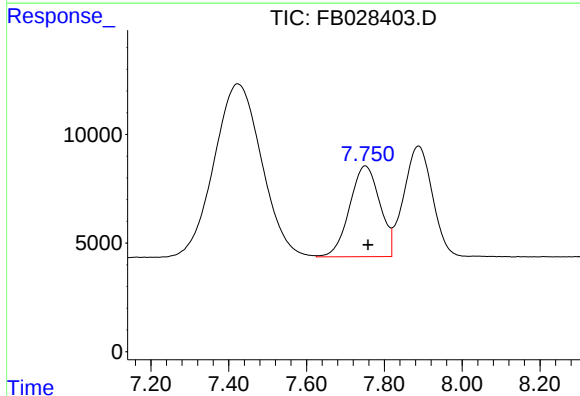


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.007 min
Response: 225805
Conc: 10.50 ng/ml

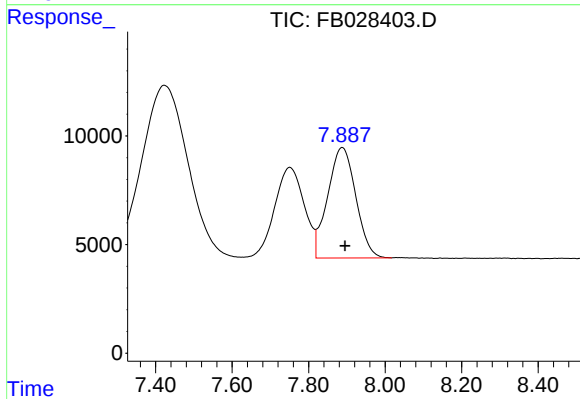

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.007 min
Response: 259509
Conc: 10.55 ng/ml

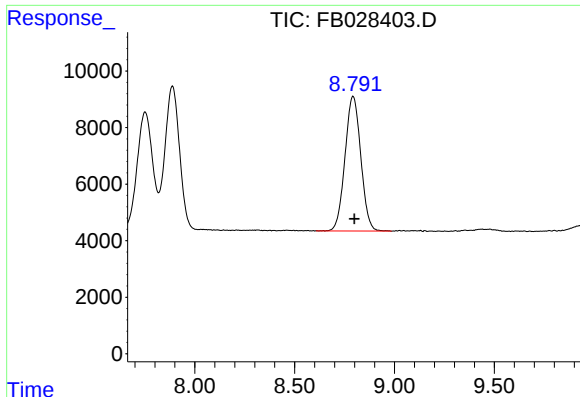

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.007 min
Response: 262182
Conc: 21.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S1

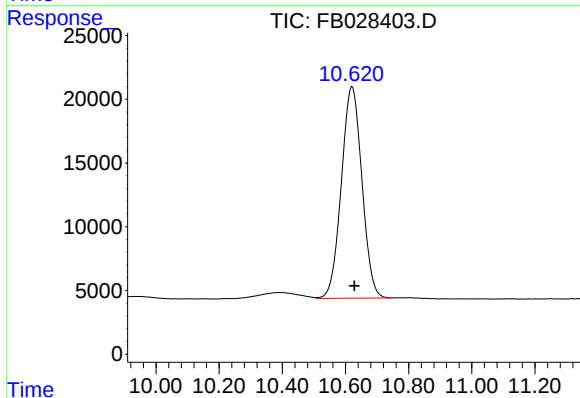


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.007 min
Response: 750468
Conc: 32.23 ng/ml

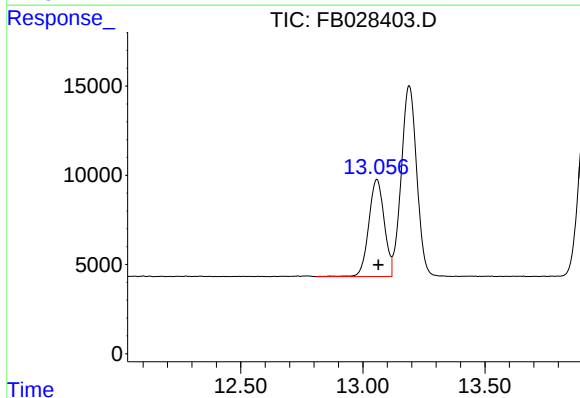


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.007 min
Response: 240040
Conc: 10.79 ng/ml

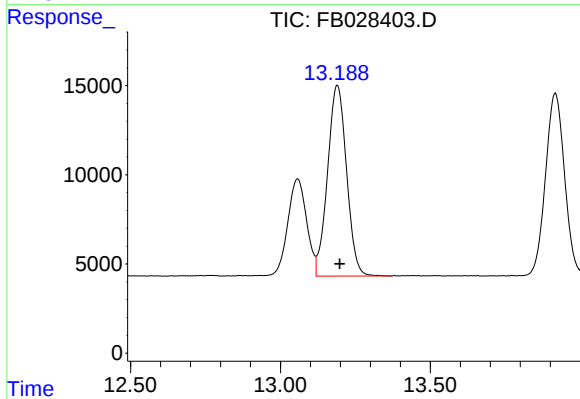

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.007 min
Response: 471709
Conc: 21.62 ng/ml

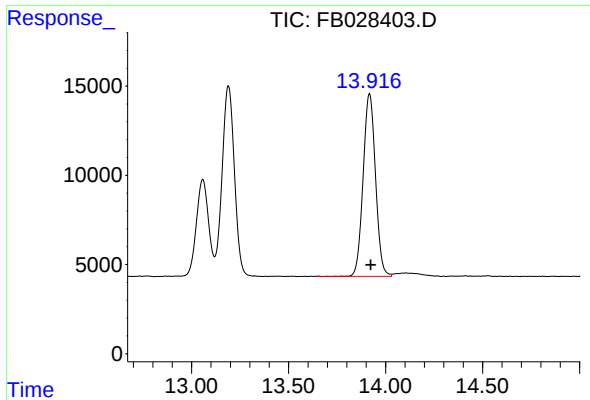

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.007 min
Response: 452895
Conc: 21.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S1

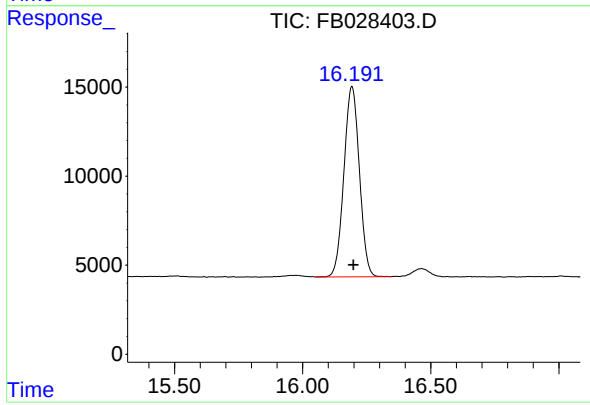

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: -0.006 min
Response: 447792
Conc: 22.27 ng/ml