

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB092322\  
 Data File : FB028404.D  
 Signal(s) : FID2B.CH  
 Acq On : 23 Sep 2022 11:49  
 Operator : AJ/MA  
 Sample : N4733-01  
 Misc : 5.01G/5.00 ML DI WATER  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
 FID\_B  
**ClientSampleId :**  
 AU-05-092122

Integration File: Calibration.e  
 Quant Time: Sep 24 15:40:09 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090822.M  
 Quant Title :  
 QLast Update : Thu Sep 08 15:28:37 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

-----  
 System Monitoring Compounds

Target Compounds  
 -----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB092322\  
Data File : FB028404.D  
Signal(s) : FID2B.CH  
Acq On : 23 Sep 2022 11:49  
Operator : AJ/MA  
Sample : N4733-01  
Misc : 5.01G/5.00 ML DI WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
AU-05-092122

Integration File: Calibration.e  
Quant Time: Sep 24 15:40:09 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090822.M  
Quant Title :  
QLast Update : Thu Sep 08 15:28:37 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

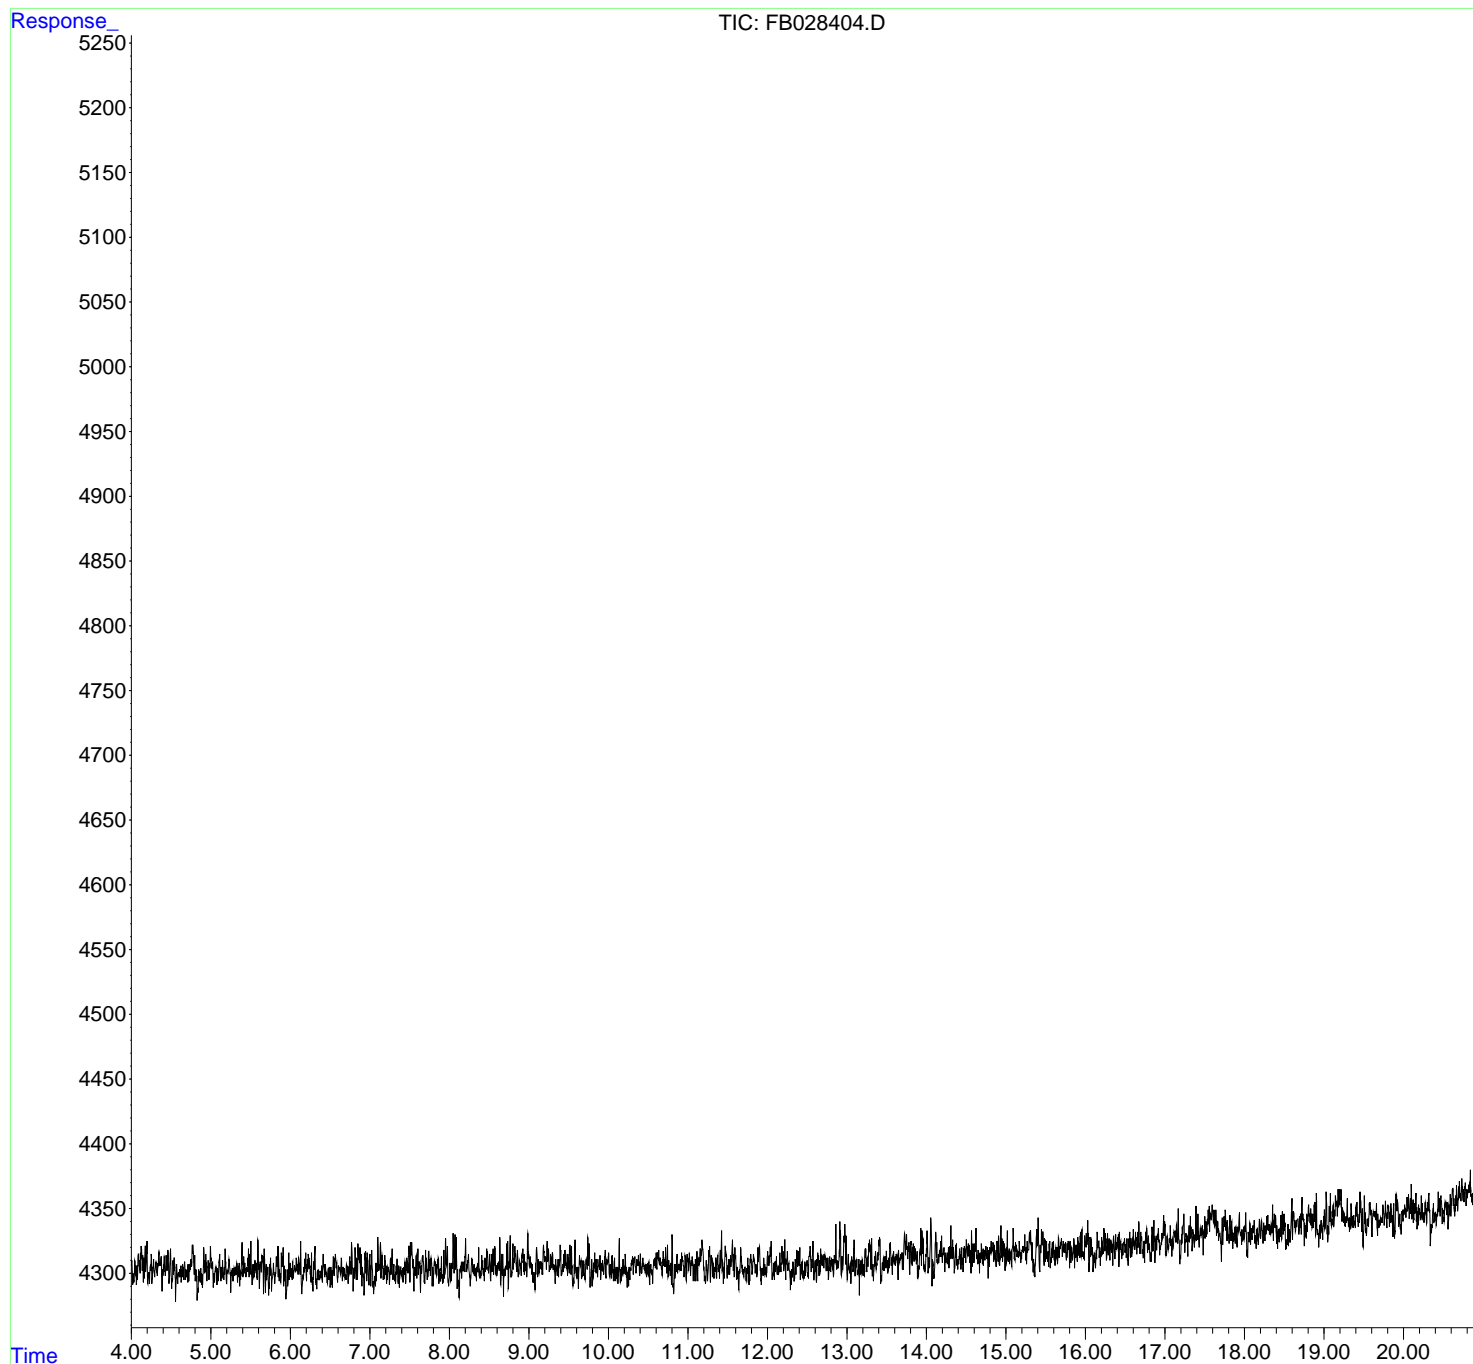

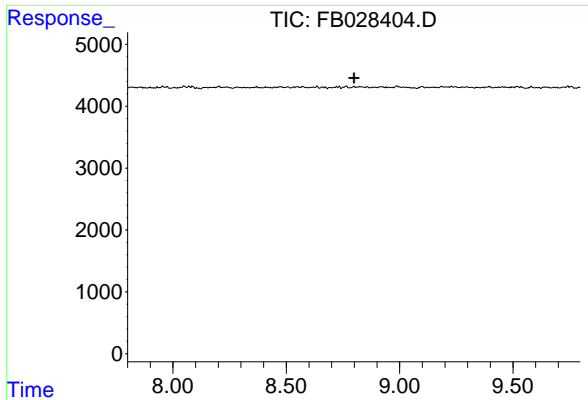

#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T.: 8.800 min  
Response: 0  
Conc: N.D.

Instrument : FID\_B  
ClientSampleId : AU-05-092122