

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092322\
 Data File : FB028411.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2022 16:49
 Operator : AJ/MA
 Sample : N4733-01MS 50X
 Misc : 5.09G/5.00 ML MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-05-092122MS

Integration File: Calibration.e
 Quant Time: Sep 24 15:40:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	224868	18.788 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	591990	29.238 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	616892	29.325 ng/ml
3) t n-Heptane	7.754	214615	9.984 ng/ml
4) t Benzene	7.891	268009	10.894 ng/ml
6) t Toluene	10.625	748899	32.167 ng/ml
7) t Ethylbenzene	13.063	235194	10.576 ng/ml
8) t m-Xylene	13.196	459163	21.041 ng/ml
9) t O-Xylene	13.922	435842	20.802 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	394028	19.596 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092322\
Data File : FB028411.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2022 16:49
Operator : AJ/MA
Sample : N4733-01MS 50X
Misc : 5.09G/5.00 ML MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-05-092122MS

Integration File: Calibration.e
Quant Time: Sep 24 15:40:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

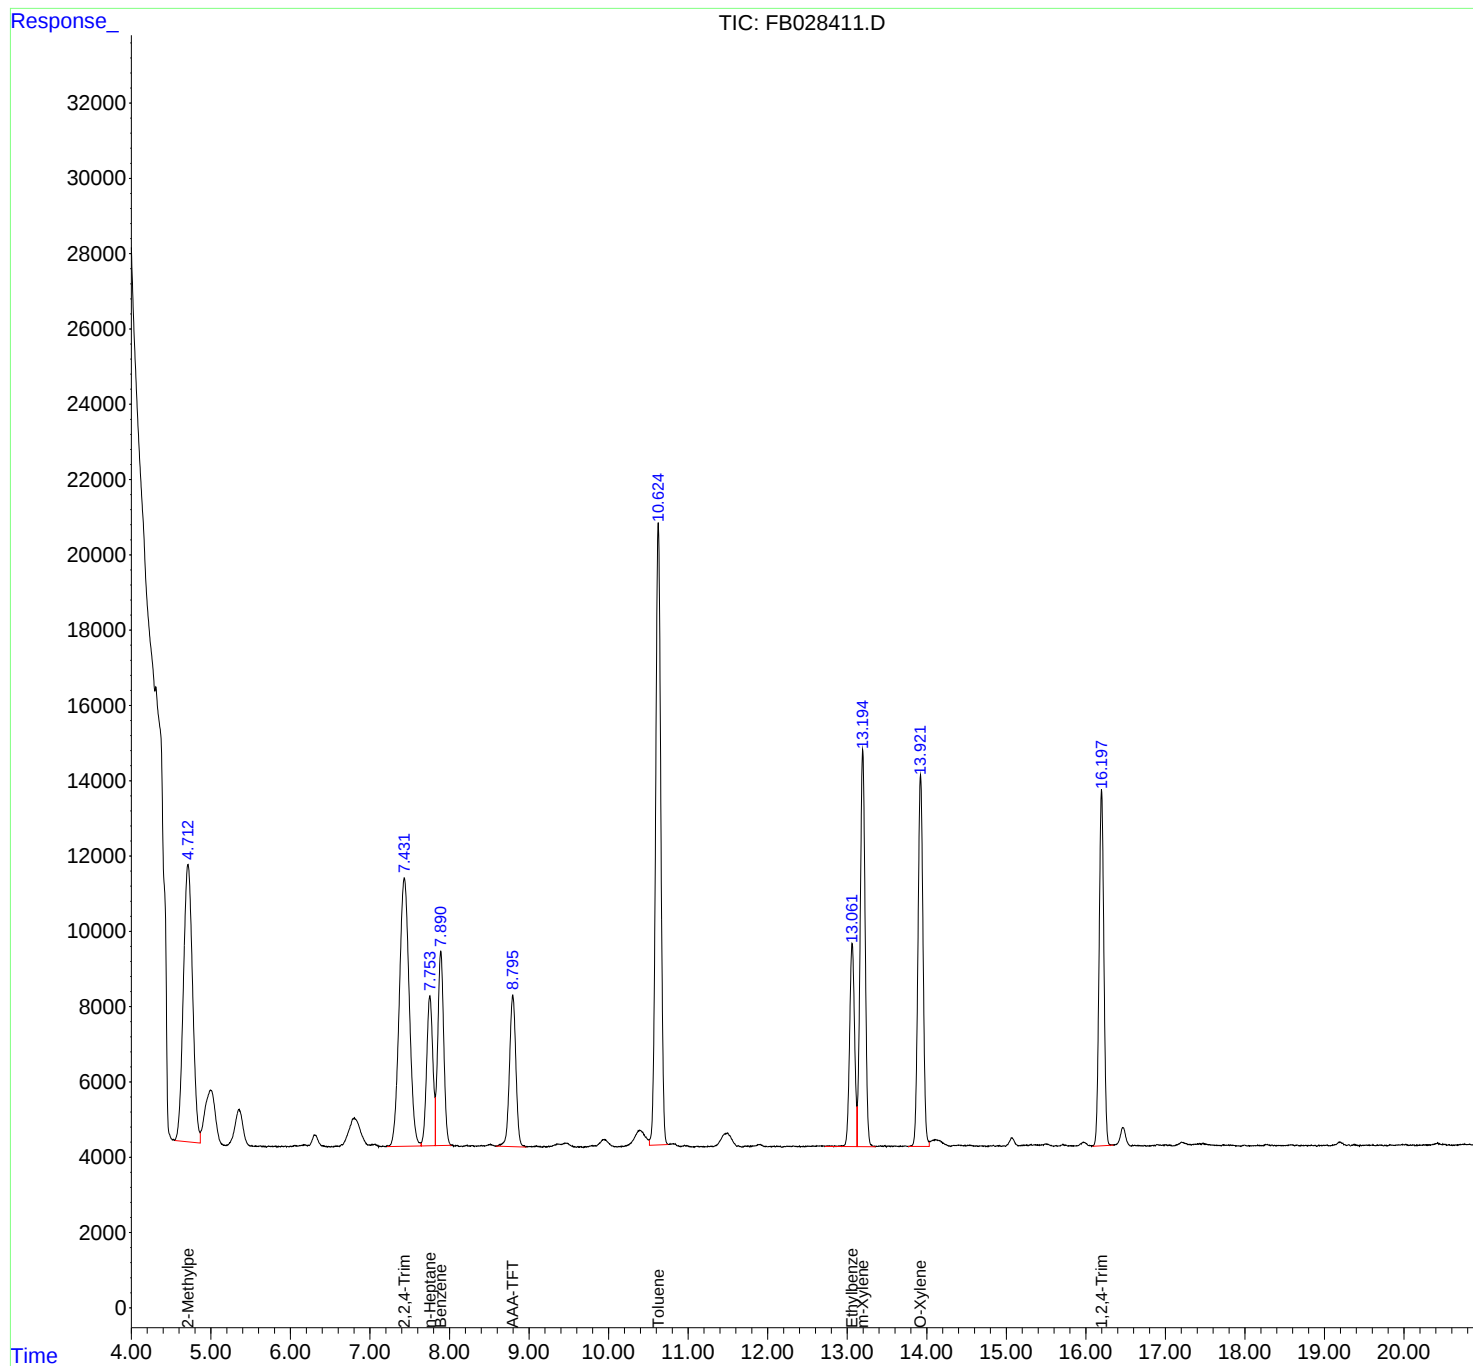


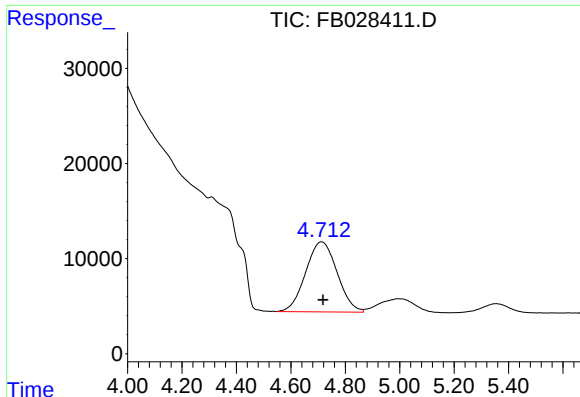

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: -0.005 min
Response: 591990
Conc: 29.24 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-05-092122MS

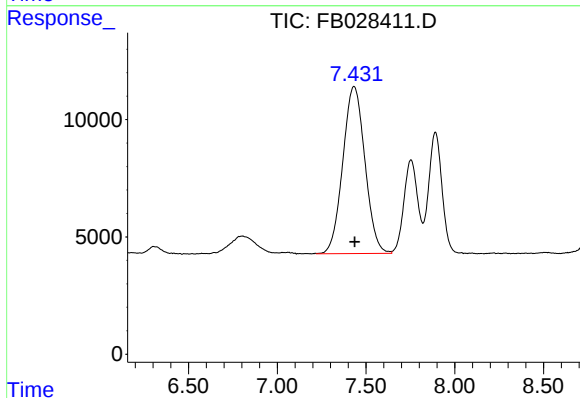


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: -0.005 min
Response: 616892
Conc: 29.33 ng/ml

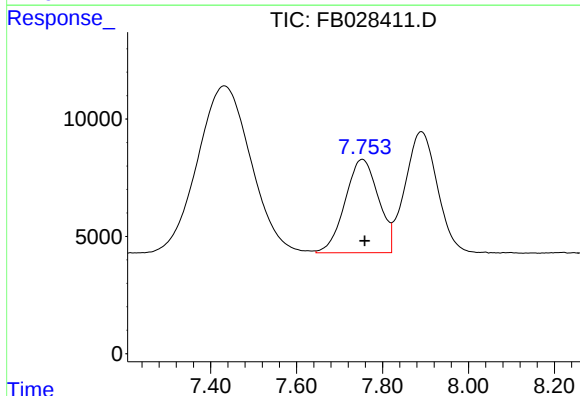


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 214615
Conc: 9.98 ng/ml

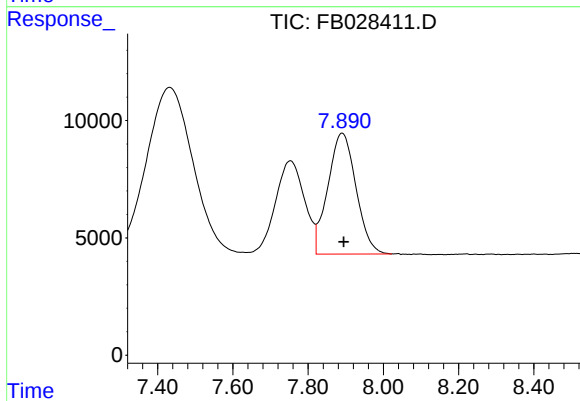

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.004 min
Response: 268009
Conc: 10.89 ng/ml

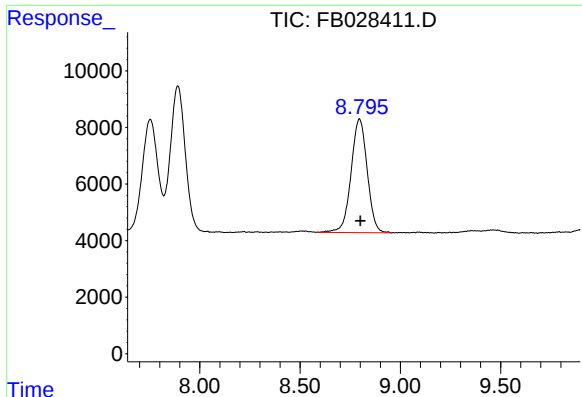

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 224868
Conc: 18.79 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-05-092122MS

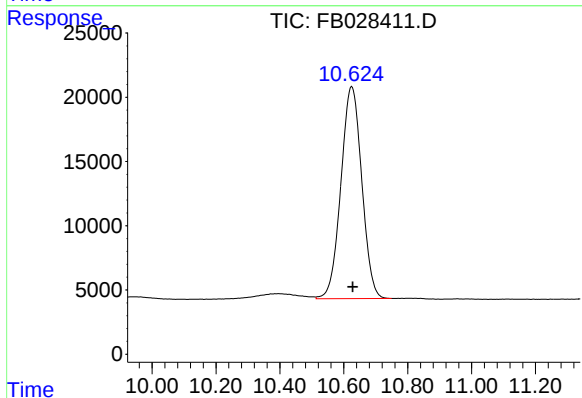


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 748899
Conc: 32.17 ng/ml

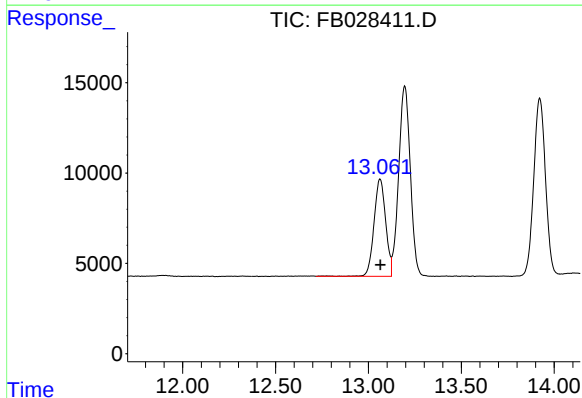


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.002 min
Response: 235194
Conc: 10.58 ng/ml

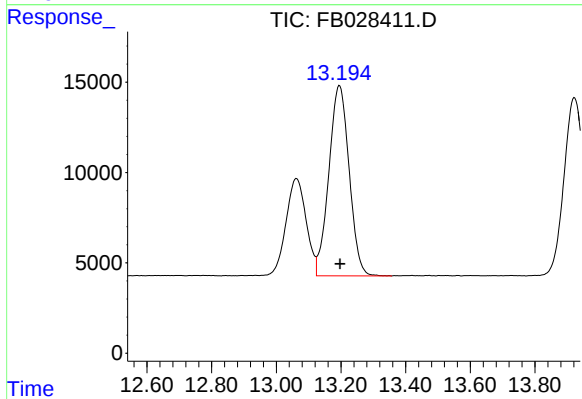

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.002 min
Response: 459163
Conc: 21.04 ng/ml

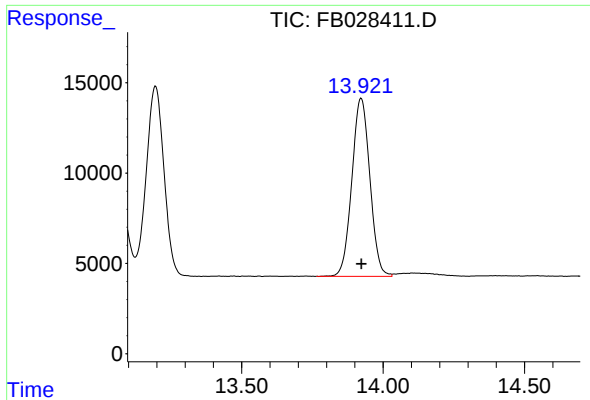

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.001 min
Response: 435842
Conc: 20.80 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-05-092122MS

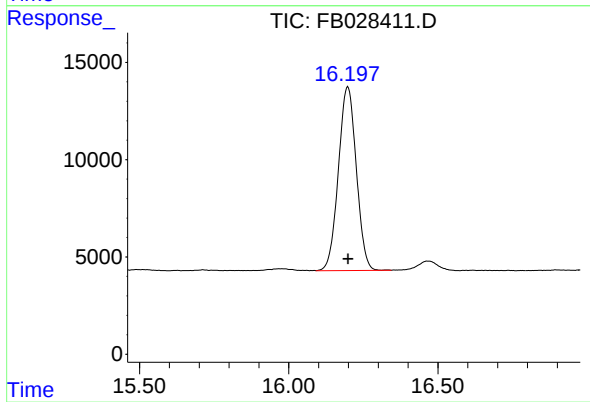

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.001 min
Response: 394028
Conc: 19.60 ng/ml