

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092322\
 Data File : FB028412.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2022 17:26
 Operator : AJ/MA
 Sample : N4733-01MSD 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-05-092122MSD

Integration File: Calibration.e
 Quant Time: Sep 24 15:40:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	293027	24.482 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	604090	29.836 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	642865	30.560 ng/ml
3) t n-Heptane	7.753	229885	10.694 ng/ml
4) t Benzene	7.890	295279	12.003 ng/ml
6) t Toluene	10.624	807259	34.674 ng/ml
7) t Ethylbenzene	13.063	251349	11.302 ng/ml
8) t m-Xylene	13.195	494187	22.646 ng/ml
9) t O-Xylene	13.922	470907	22.476 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	415478	20.663 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092322\
 Data File : FB028412.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2022 17:26
 Operator : AJ/MA
 Sample : N4733-01MSD 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-05-092122MSD

Integration File: Calibration.e
 Quant Time: Sep 24 15:40:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

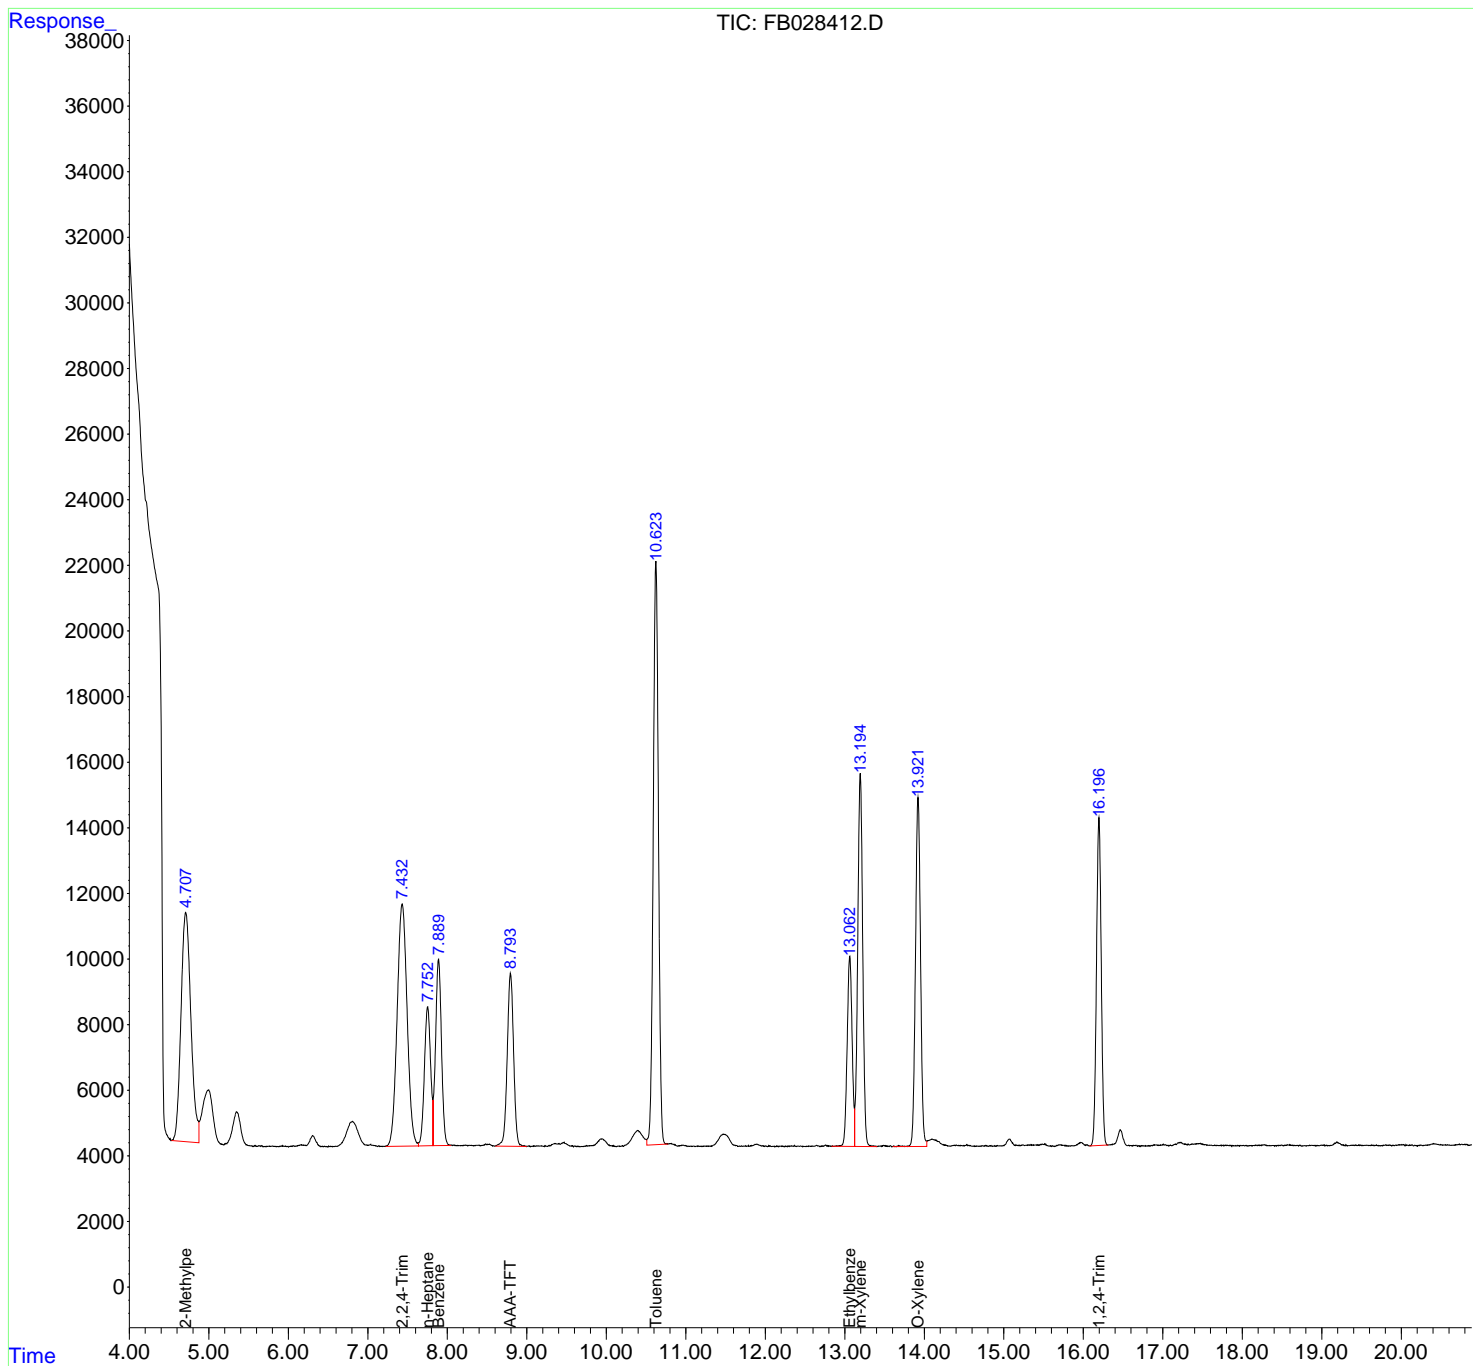


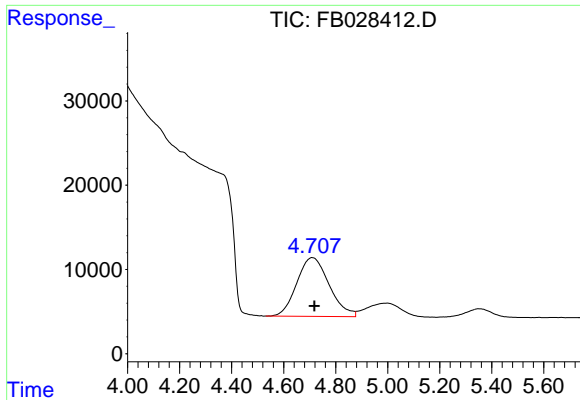

#1 2-Methylpentane


R.T.: 4.709 min
 Delta R.T.: -0.009 min
 Response: 604090
 Conc: 29.84 ng/ml

Instrument : FID_B
 ClientSampleId : AU-05-092122MSD

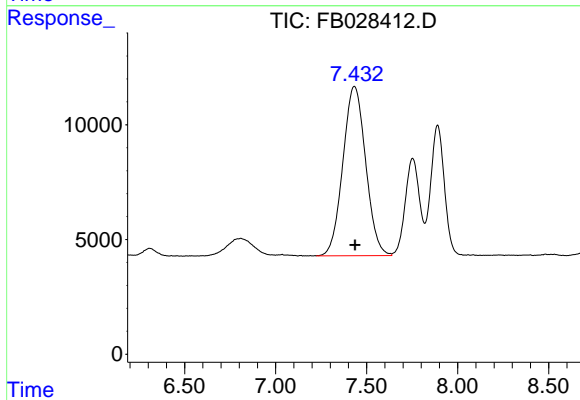


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
 Delta R.T.: -0.004 min
 Response: 642865
 Conc: 30.56 ng/ml

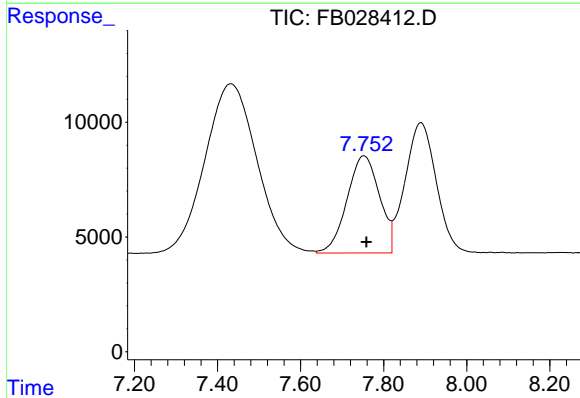


#3 n-Heptane

R.T.: 7.753 min
 Delta R.T.: -0.006 min
 Response: 229885
 Conc: 10.69 ng/ml

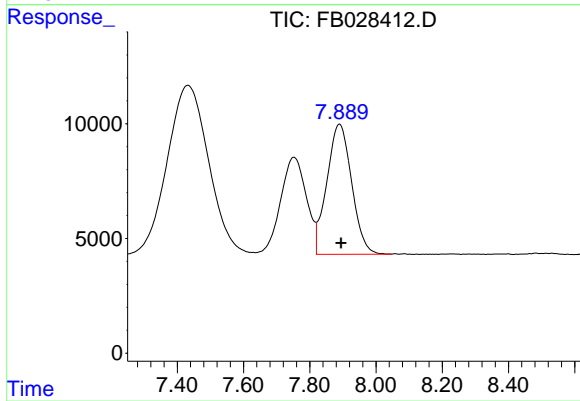

#4 Benzene


R.T.: 7.890 min
 Delta R.T.: -0.005 min
 Response: 295279
 Conc: 12.00 ng/ml

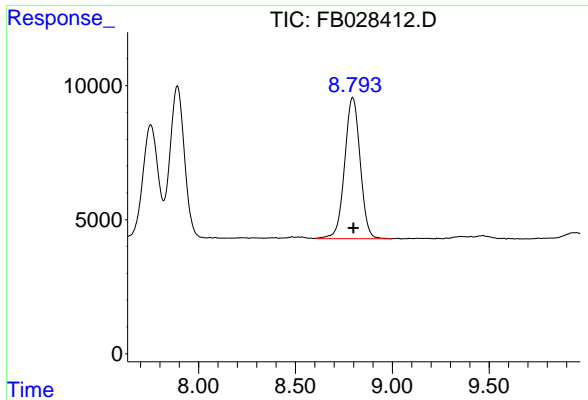

#5 AAA-TFT


R.T.: 8.795 min
 Delta R.T.: -0.005 min
 Response: 293027
 Conc: 24.48 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 AU-05-092122MSD

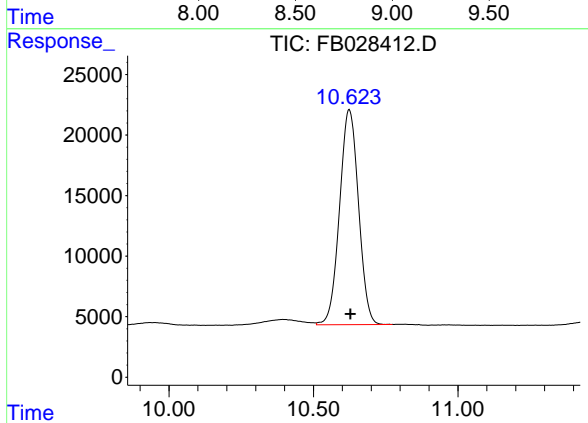


#6 Toluene

R.T.: 10.624 min
 Delta R.T.: -0.004 min
 Response: 807259
 Conc: 34.67 ng/ml

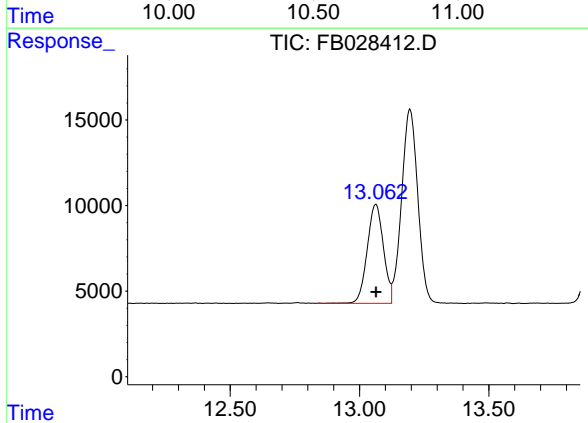


#7 Ethylbenzene

R.T.: 13.063 min
 Delta R.T.: -0.001 min
 Response: 251349
 Conc: 11.30 ng/ml

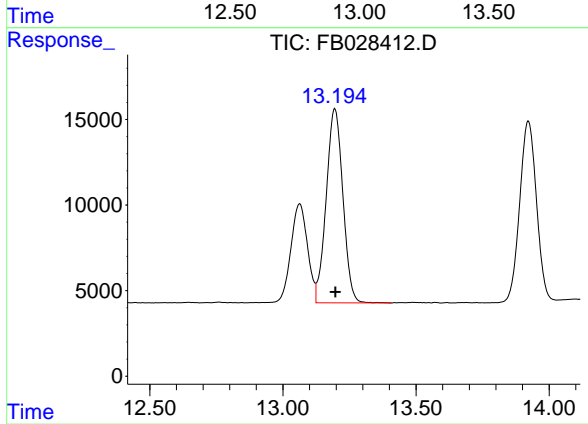

#8 m-Xylene


R.T.: 13.195 min
 Delta R.T.: -0.002 min
 Response: 494187
 Conc: 22.65 ng/ml

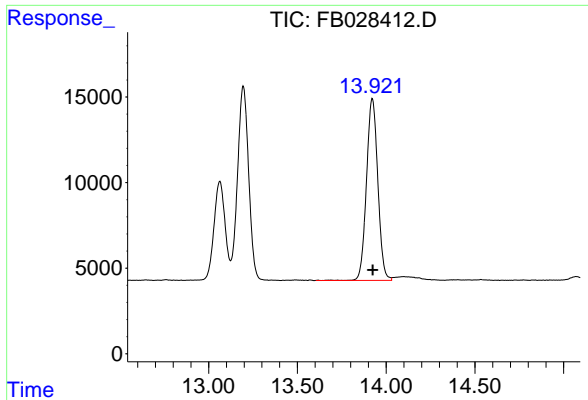

#9 O-Xylene

R.T.: 13.922 min
 Delta R.T.: -0.002 min
 Response: 470907
 Conc: 22.48 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 AU-05-092122MSD

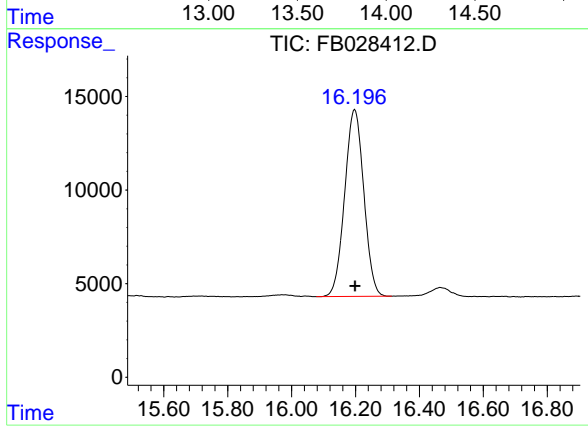

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
 Delta R.T.: -0.001 min
 Response: 415478
 Conc: 20.66 ng/ml