

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092322\
 Data File : FB028420.D
 Signal(s) : FID2B.CH
 Acq On : 23 Sep 2022 22:26
 Operator : AJ/MA
 Sample : BSF0923S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0923S2

Integration File: Calibration.e
 Quant Time: Sep 24 15:41:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	224886	18.789 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	616532	30.450 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	649666	30.883 ng/ml
3) t n-Heptane	7.752	208907	9.718 ng/ml
4) t Benzene	7.889	248880	10.117 ng/ml
6) t Toluene	10.623	697842	29.974 ng/ml
7) t Ethylbenzene	13.059	218003	9.803 ng/ml
8) t m-Xylene	13.192	432517	19.820 ng/ml
9) t O-Xylene	13.919	423789	20.227 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	402370	20.011 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092322\
Data File : FB028420.D
Signal(s) : FID2B.CH
Acq On : 23 Sep 2022 22:26
Operator : AJ/MA
Sample : BSF0923S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0923S2

Integration File: Calibration.e
Quant Time: Sep 24 15:41:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

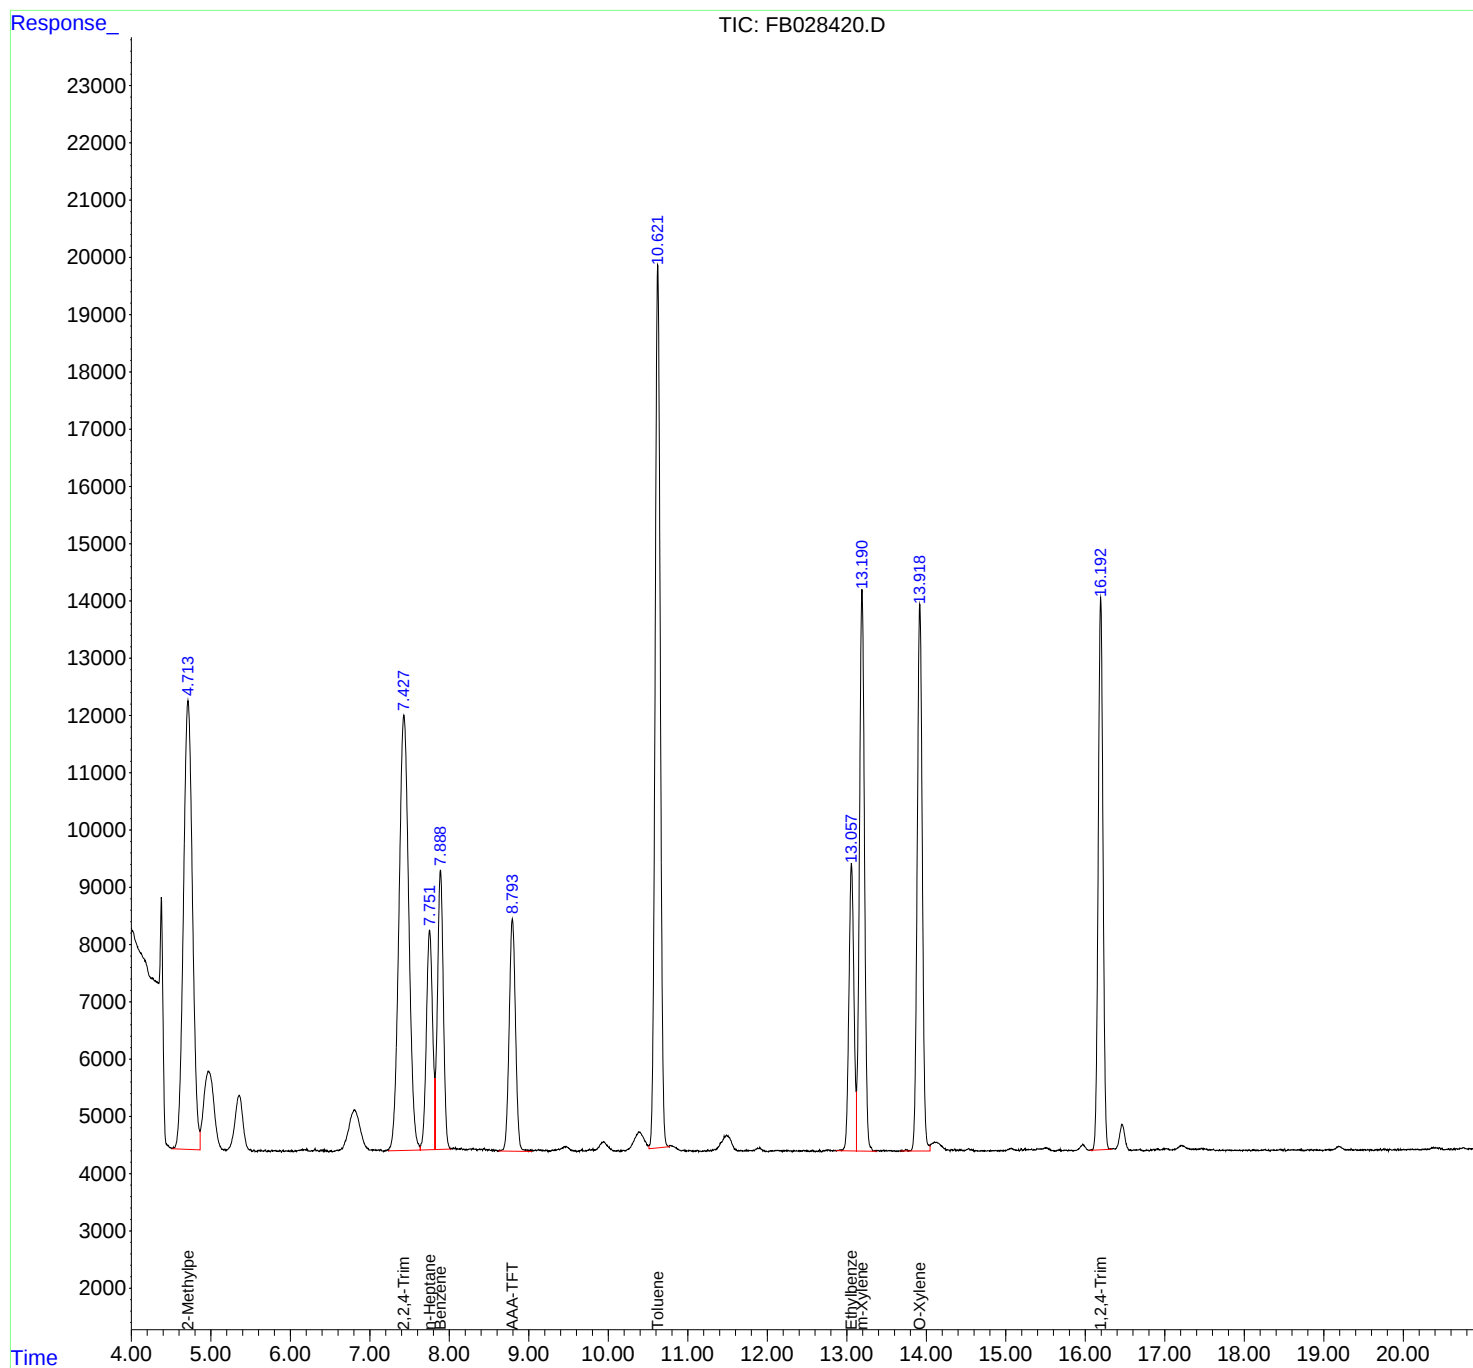


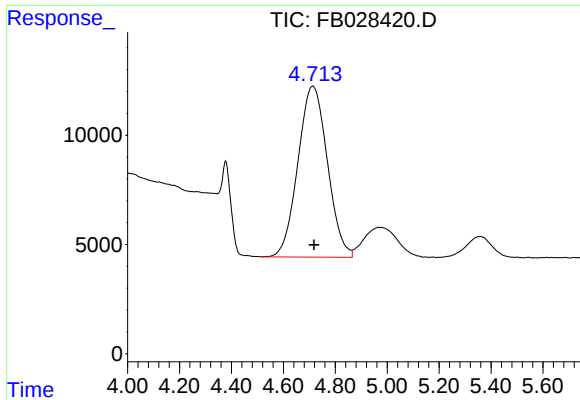

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: -0.004 min
Response: 616532
Conc: 30.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S2

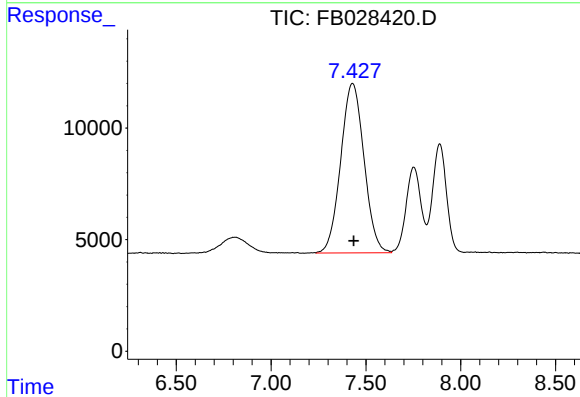


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: -0.008 min
Response: 649666
Conc: 30.88 ng/ml

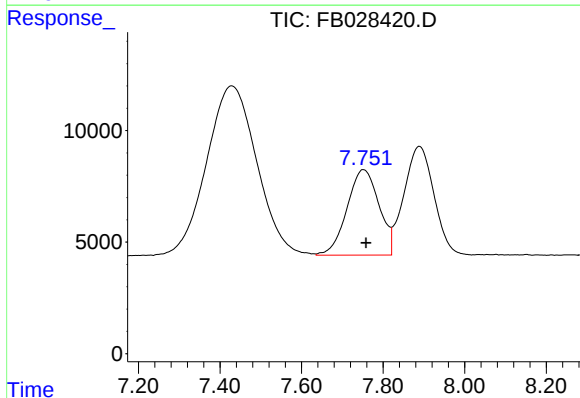


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 208907
Conc: 9.72 ng/ml

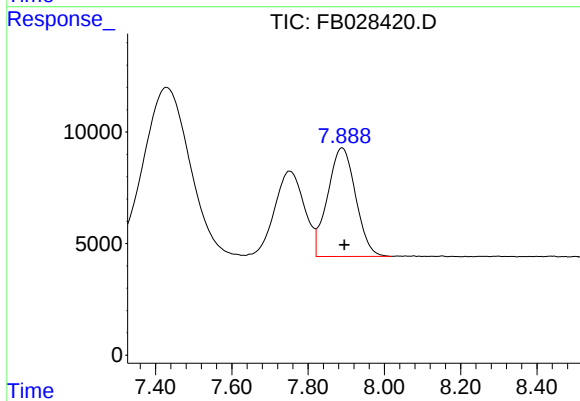

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.005 min
Response: 248880
Conc: 10.12 ng/ml

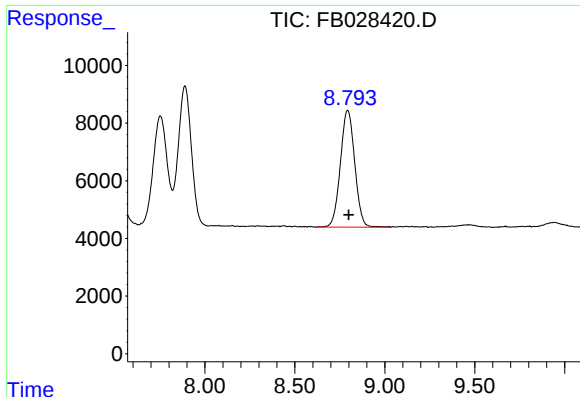

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.006 min
Response: 224886
Conc: 18.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S2

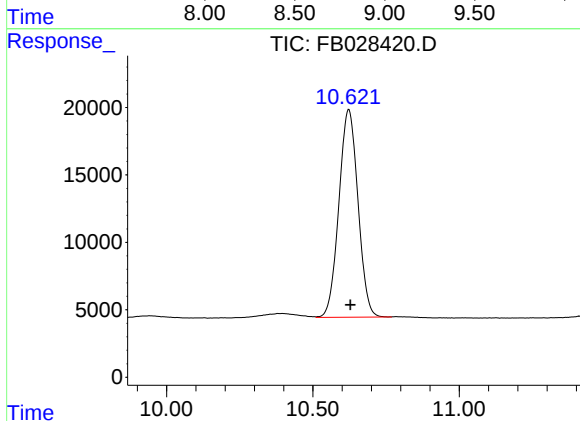


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.005 min
Response: 697842
Conc: 29.97 ng/ml

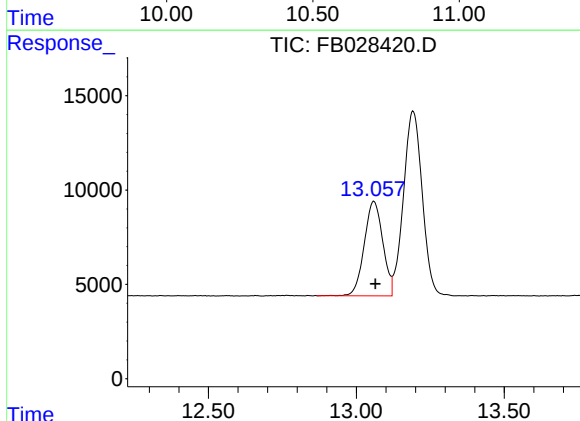


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: -0.005 min
Response: 218003
Conc: 9.80 ng/ml

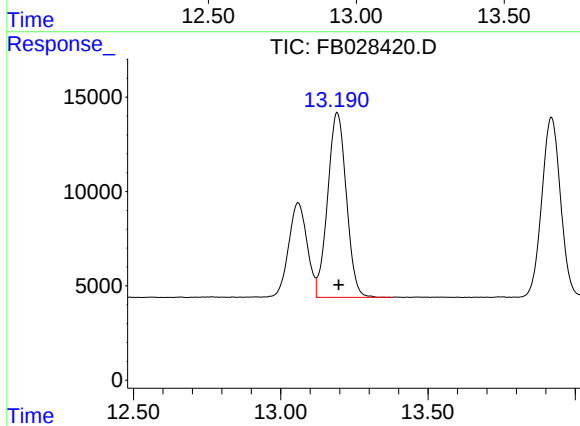

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.005 min
Response: 432517
Conc: 19.82 ng/ml

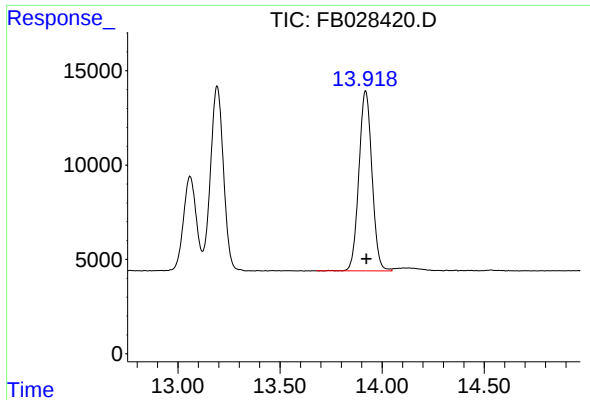

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.005 min
Response: 423789
Conc: 20.23 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0923S2

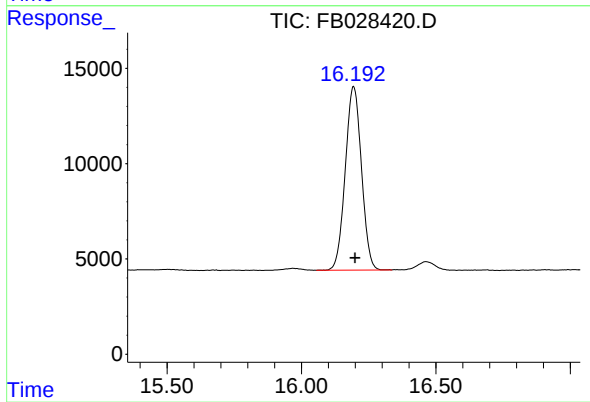

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.005 min
Response: 402370
Conc: 20.01 ng/ml