

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092419\
 Data File : FB022585.D
 Signal(s) : FID2B.CH
 Acq On : 24 Sep 2019 9:28
 Operator : DD/AJ
 Sample : BSF0924S1
 Misc : 5.00g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 24 12:49:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.968	597773	20.551 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.833	1081456	22.011 ng/ml
2) t	2,2,4-Trimethylpentane	7.585	1239461	24.003 ng/ml
3) t	n-Heptane	7.925	402389	7.995 ng/ml
4) t	Benzene	8.060	500752	8.437 ng/ml
6) t	Toluene	10.809	1489344	31.306 ng/ml
7) t	Ethylbenzene	13.256	480142	16.016 ng/ml
8) t	m-Xylene	13.389	952239	35.844 ng/ml
9) t	O-Xylene	14.118	901257	37.150 ng/ml
10) t	1,2,4-Trimethylbenzene	16.399	632077	24.244 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092419\
Data File : FB022585.D
Signal(s) : FID2B.CH
Acq On : 24 Sep 2019 9:28
Operator : DD/AJ
Sample : BSF0924S1
Misc : 5.00g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 24 12:49:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

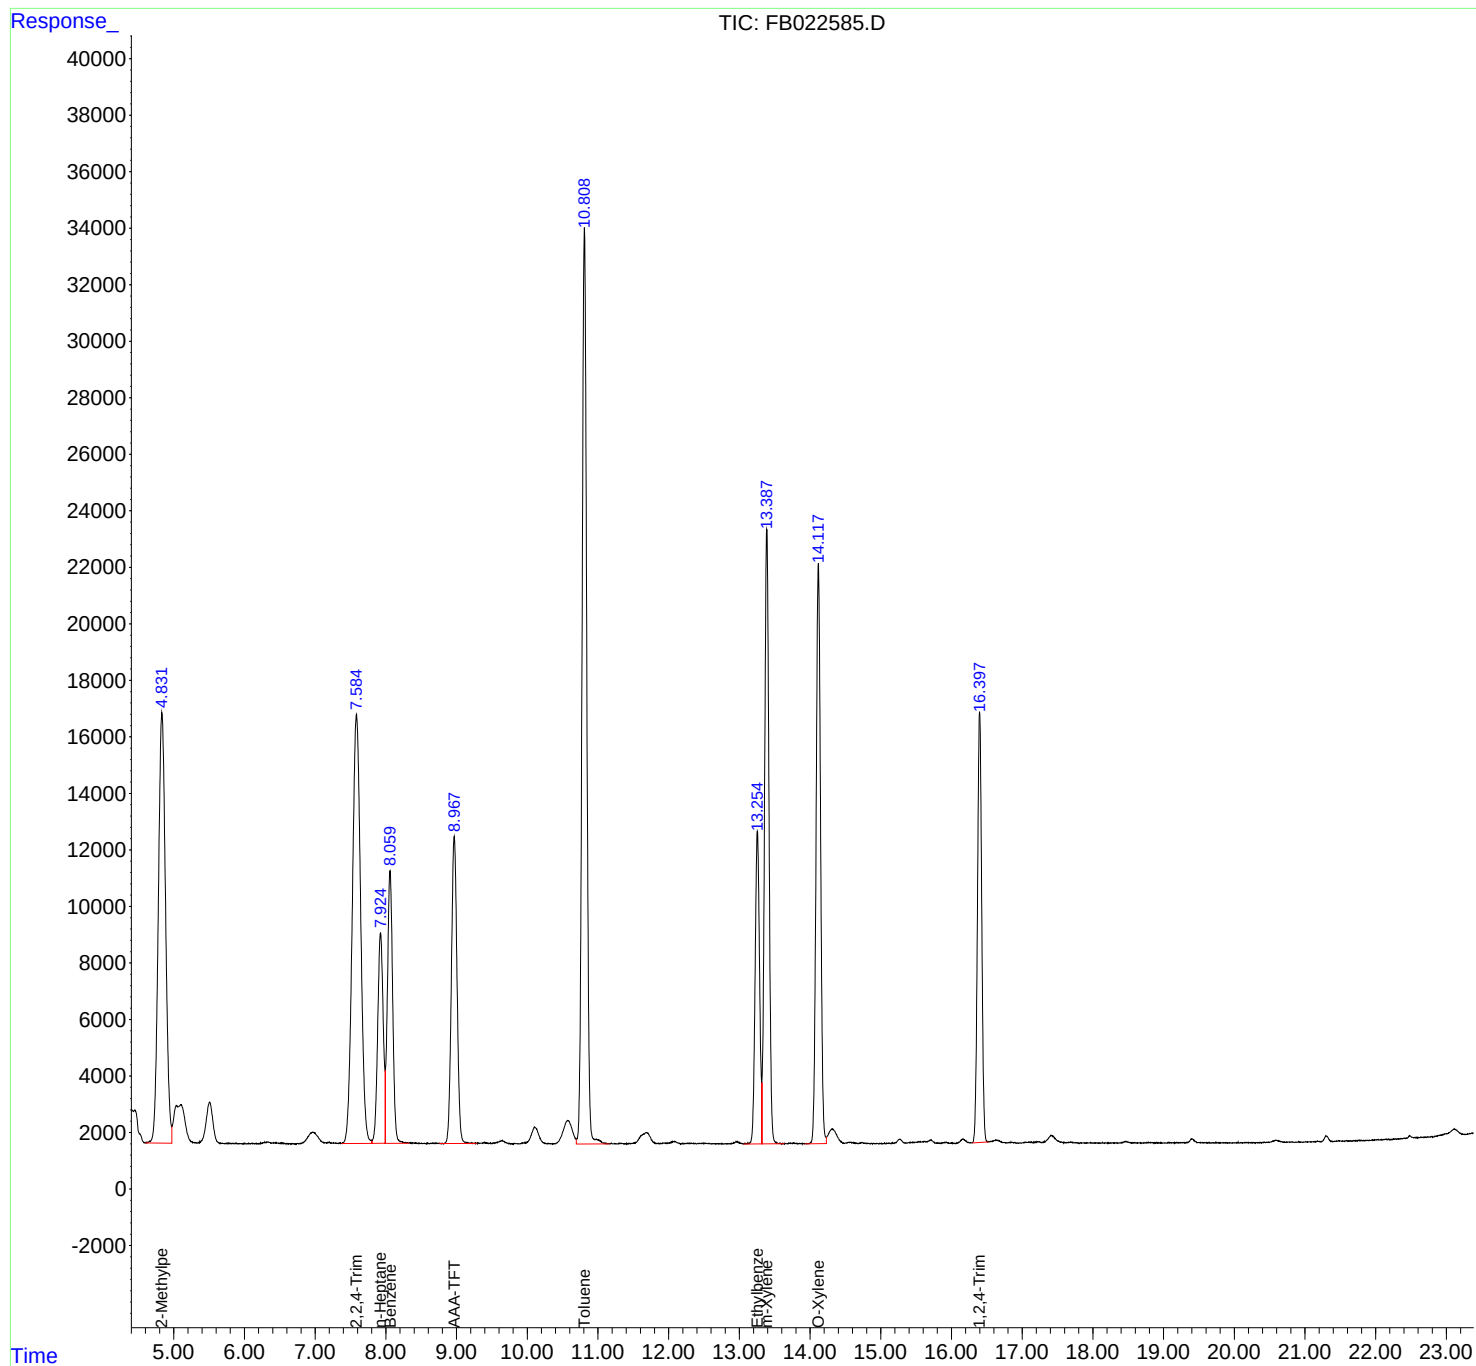

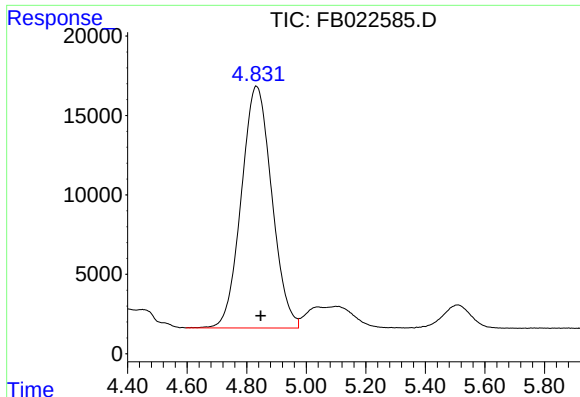


#1 2-Methylpentane

R.T.: 4.833 min
Delta R.T.: -0.014 min
Response: 1081456
Conc: 22.01 ng/ml

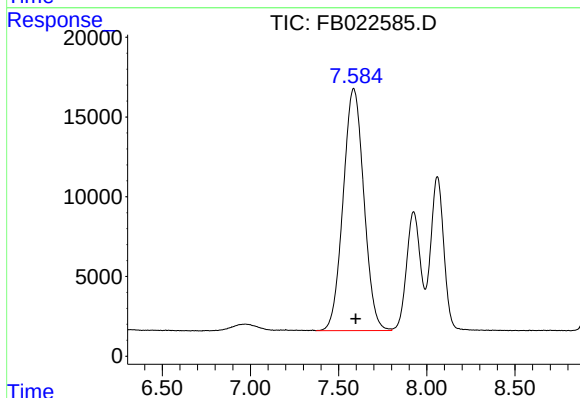


#2 2,2,4-Trimethylpentane

R.T.: 7.585 min
Delta R.T.: -0.012 min
Response: 1239461
Conc: 24.00 ng/ml

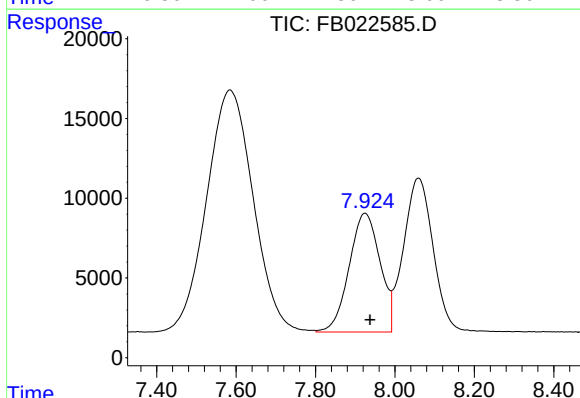


#3 n-Heptane

R.T.: 7.925 min
Delta R.T.: -0.012 min
Response: 402389
Conc: 7.99 ng/ml

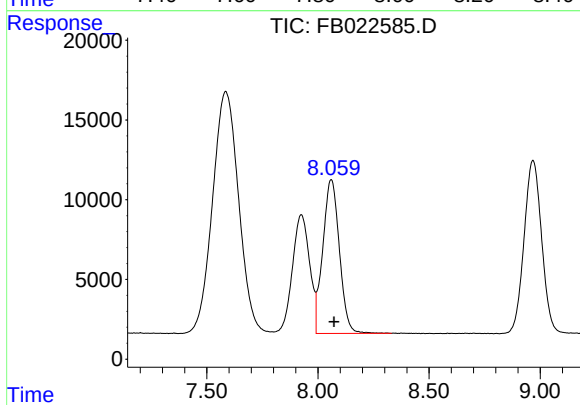


#4 Benzene

R.T.: 8.060 min
Delta R.T.: -0.012 min
Response: 500752
Conc: 8.44 ng/ml

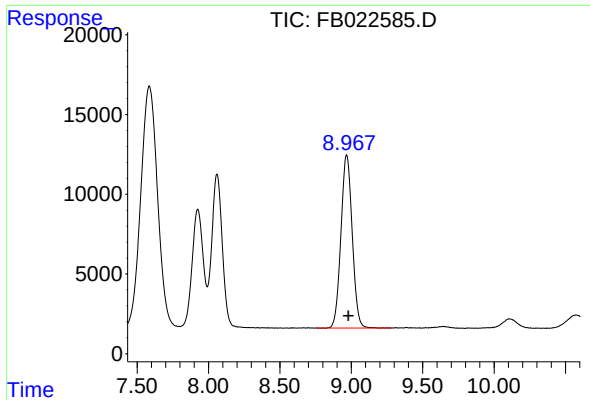


#5 AAA-TFT

R.T.: 8.968 min
Delta R.T.: -0.011 min
Response: 597773
Conc: 20.55 ng/ml

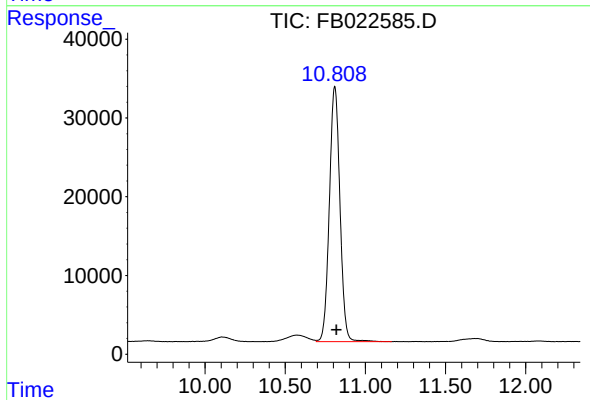


#6 Toluene

R.T.: 10.809 min
Delta R.T.: -0.010 min
Response: 1489344
Conc: 31.31 ng/ml

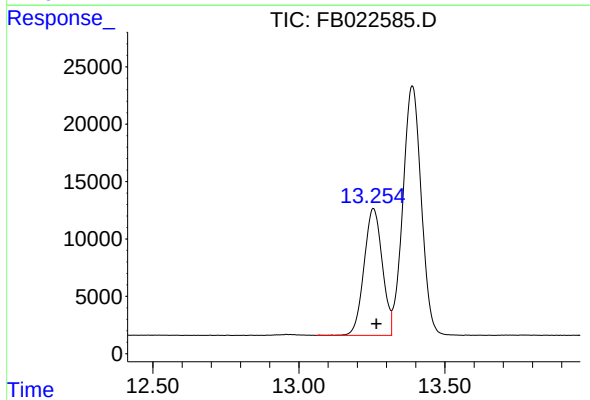


#7 Ethylbenzene

R.T.: 13.256 min
Delta R.T.: -0.010 min
Response: 480142
Conc: 16.02 ng/ml

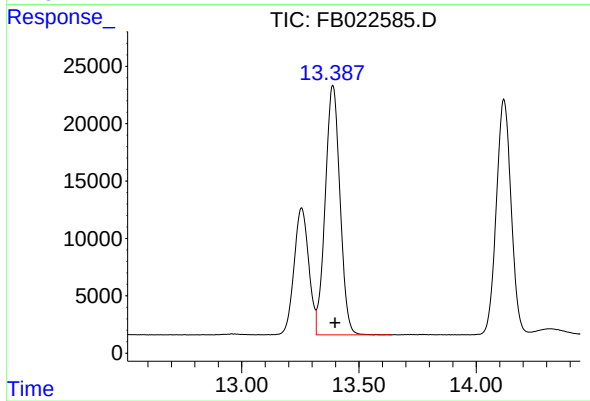

#8 m-Xylene

R.T.: 13.389 min
Delta R.T.: -0.009 min
Response: 952239
Conc: 35.84 ng/ml

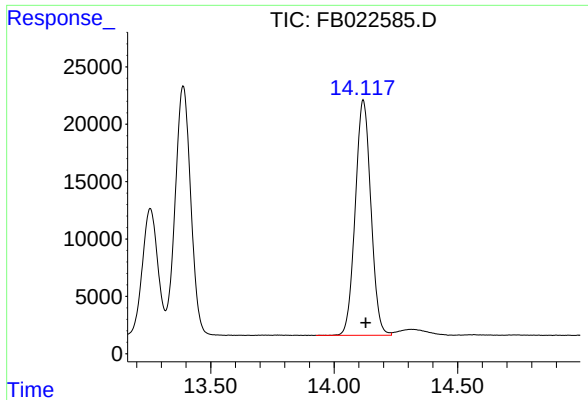


#9 O-Xylene

R.T.: 14.118 min

Delta R.T.: -0.010 min

Response: 901257

Conc: 37.15 ng/ml

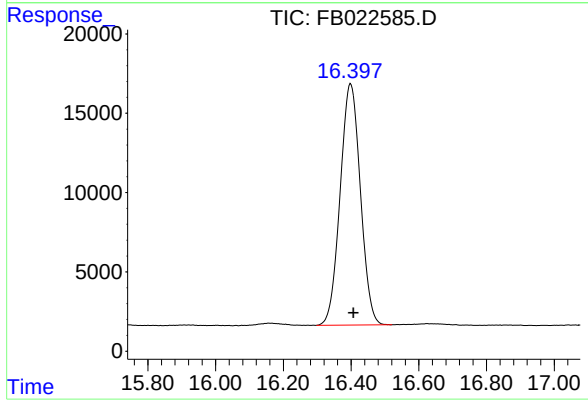

#10 1,2,4-Trimethylbenzene

R.T.: 16.399 min

Delta R.T.: -0.008 min

Response: 632077

Conc: 24.24 ng/ml