

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092419\
 Data File : FB022590.D
 Signal(s) : FID2B.CH
 Acq On : 24 Sep 2019 11:57
 Operator : DD/AJ
 Sample : K4668-13MSD
 Misc : 5.03g/5.00ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 24 12:49:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.968	587191	20.187 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.834	998046	20.313 ng/ml
2) t 2,2,4-Trimethylpentane	7.586	1119434	21.679 ng/ml
3) t n-Heptane	7.926	363527	7.223 ng/ml
4) t Benzene	8.061	471576	7.946 ng/ml
6) t Toluene	10.810	1392046	29.261 ng/ml
7) t Ethylbenzene	13.256	445362	14.856 ng/ml
8) t m-Xylene	13.389	880324	33.137 ng/ml
9) t O-Xylene	14.119	831919	34.292 ng/ml
10) t 1,2,4-Trimethylbenzene	16.400	568065	21.789 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092419\
Data File : FB022590.D
Signal(s) : FID2B.CH
Acq On : 24 Sep 2019 11:57
Operator : DD/AJ
Sample : K4668-13MSD
Misc : 5.03g/5.00ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 24 12:49:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

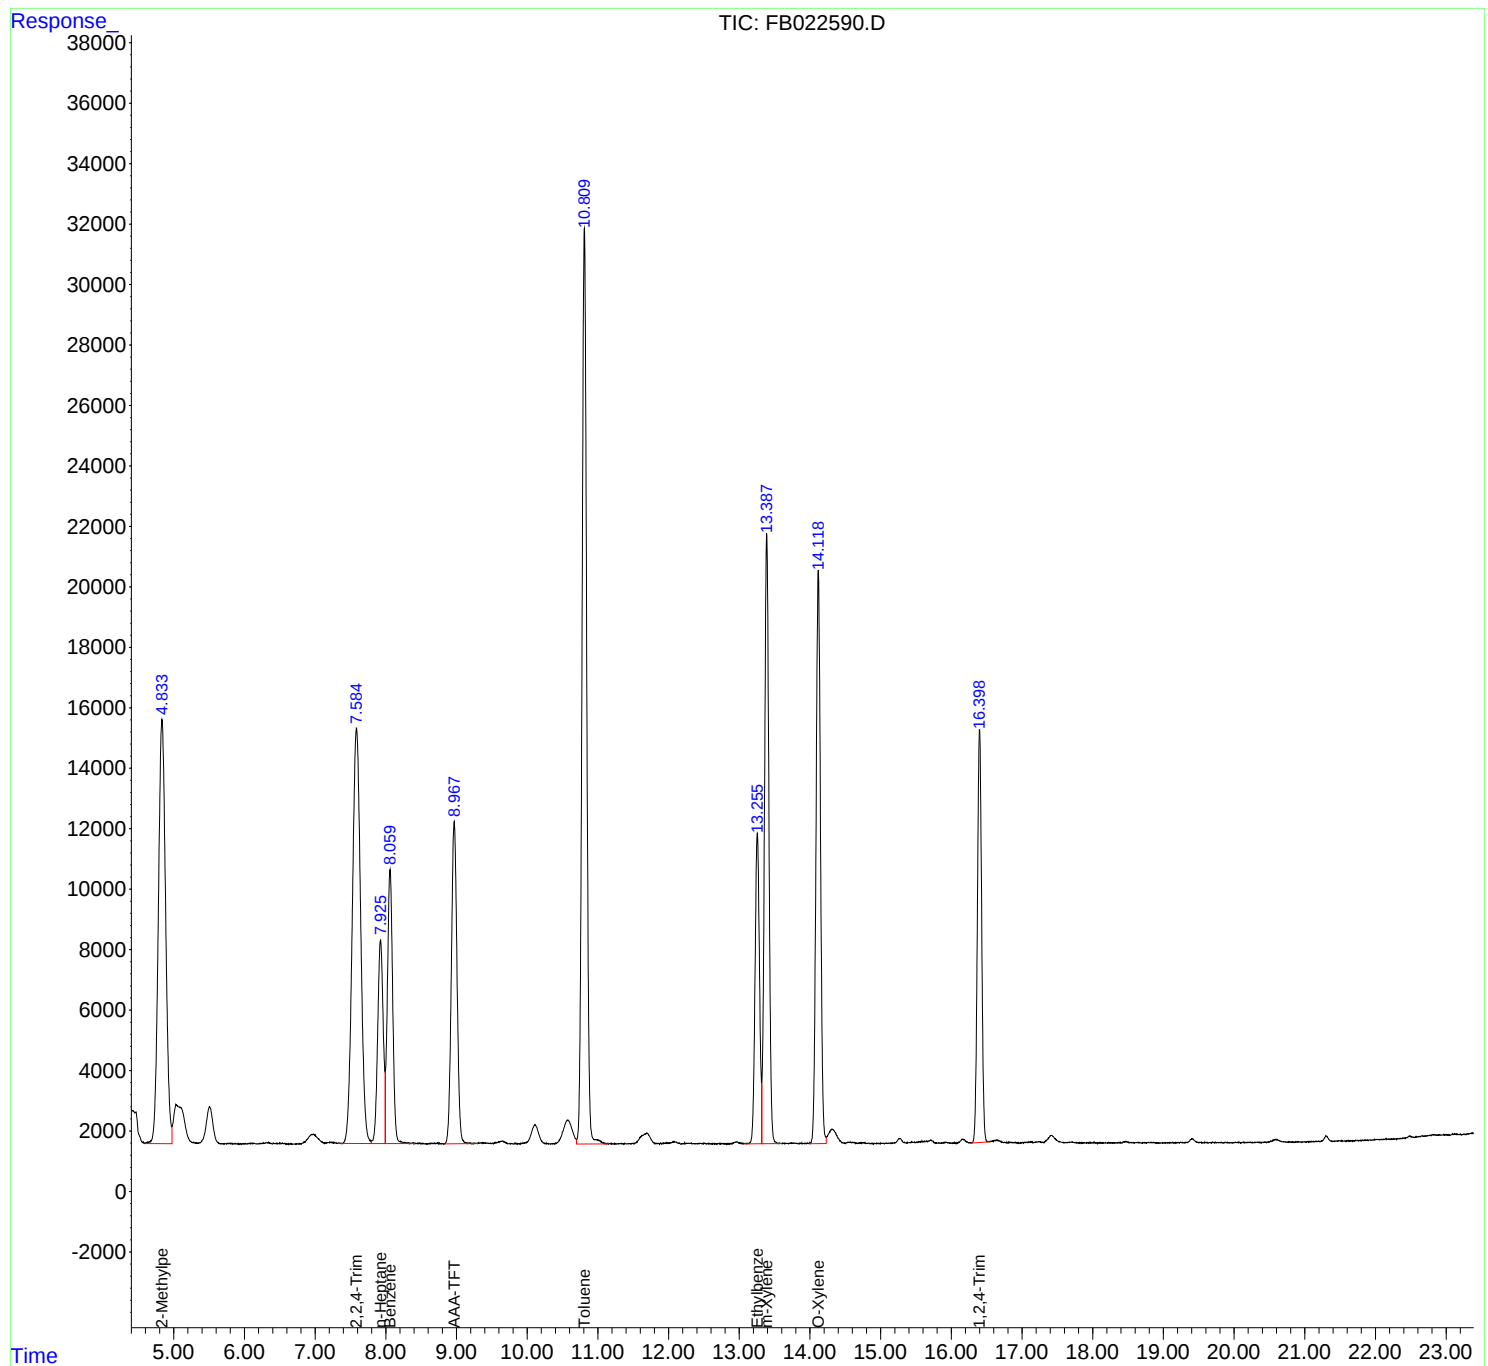

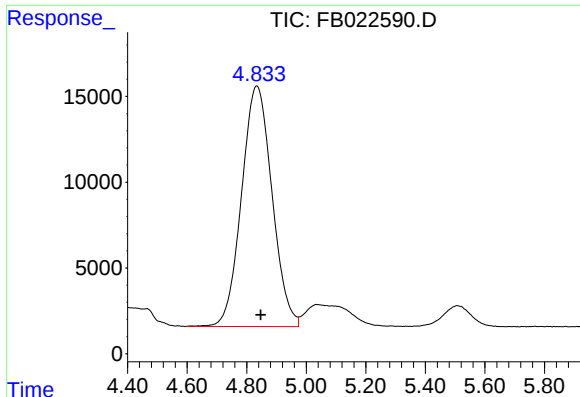


#1 2-Methylpentane

R.T.: 4.834 min
Delta R.T.: -0.013 min
Response: 998046
Conc: 20.31 ng/ml

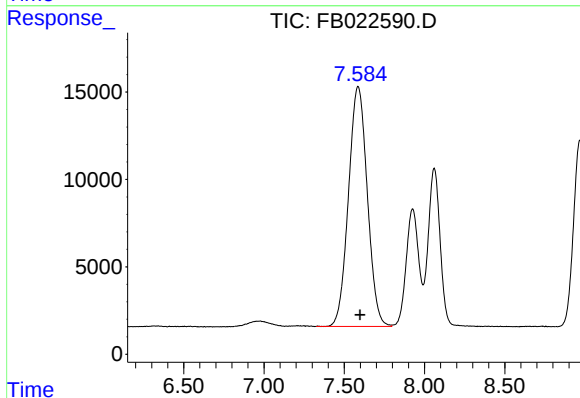


#2 2,2,4-Trimethylpentane

R.T.: 7.586 min
Delta R.T.: -0.012 min
Response: 1119434
Conc: 21.68 ng/ml

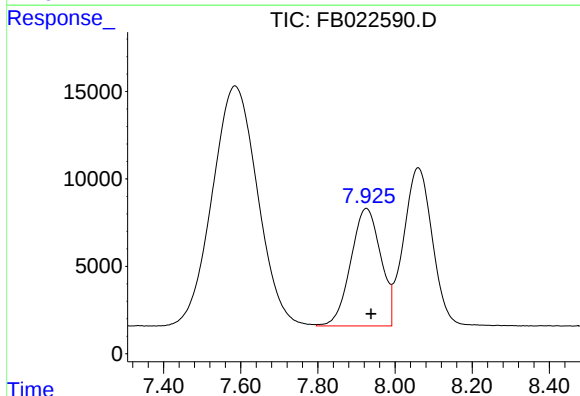


#3 n-Heptane

R.T.: 7.926 min
Delta R.T.: -0.012 min
Response: 363527
Conc: 7.22 ng/ml

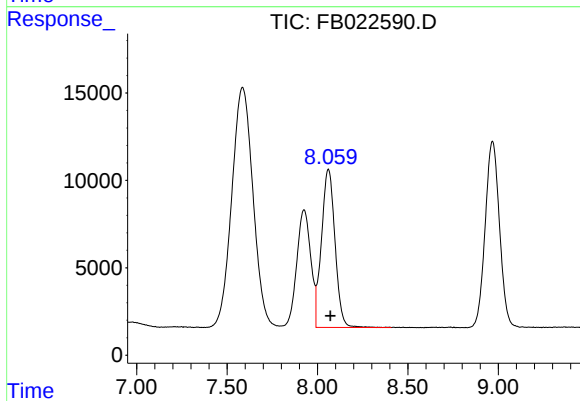


#4 Benzene

R.T.: 8.061 min
Delta R.T.: -0.012 min
Response: 471576
Conc: 7.95 ng/ml

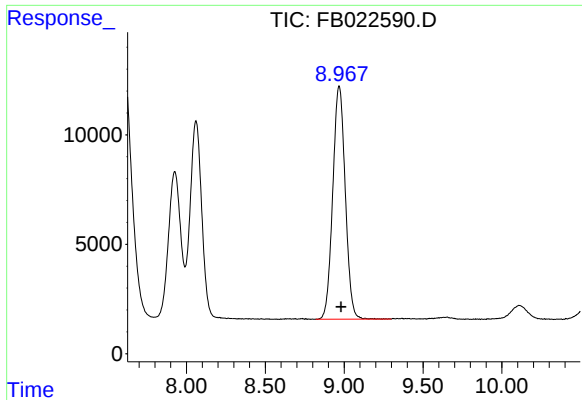


#5 AAA-TFT

R.T.: 8.968 min
Delta R.T.: -0.011 min
Response: 587191
Conc: 20.19 ng/ml

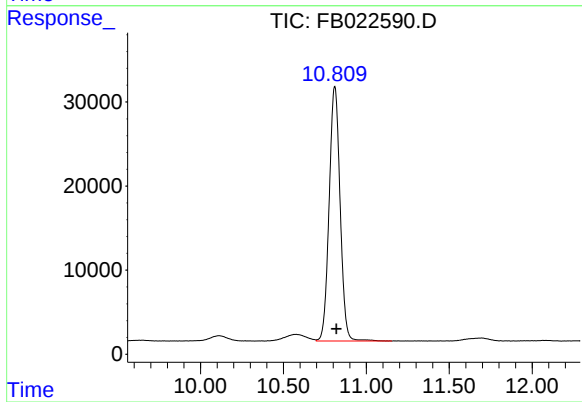


#6 Toluene

R.T.: 10.810 min
Delta R.T.: -0.010 min
Response: 1392046
Conc: 29.26 ng/ml

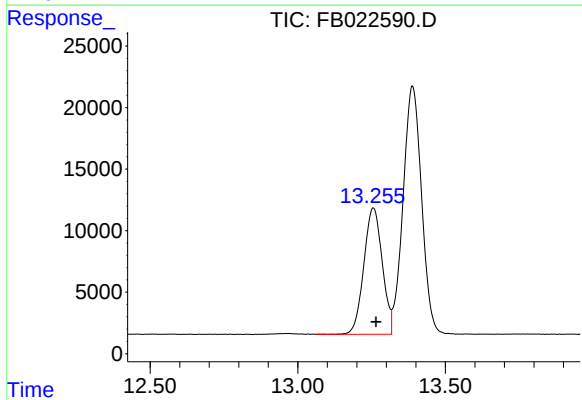


#7 Ethylbenzene

R.T.: 13.256 min
Delta R.T.: -0.009 min
Response: 445362
Conc: 14.86 ng/ml

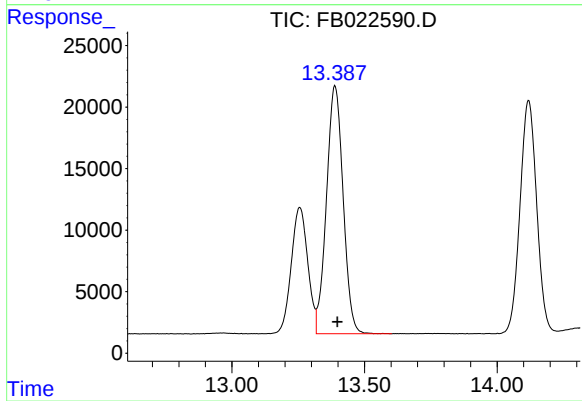


#8 m-Xylene

R.T.: 13.389 min
Delta R.T.: -0.009 min
Response: 880324
Conc: 33.14 ng/ml

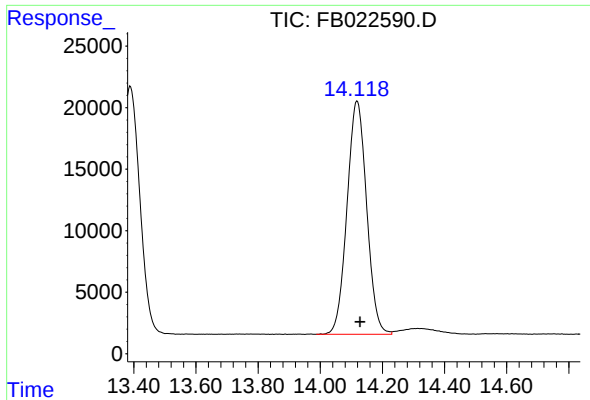

#9 O-Xylene

R.T.: 14.119 min
Delta R.T.: -0.009 min
Response: 831919
Conc: 34.29 ng/ml

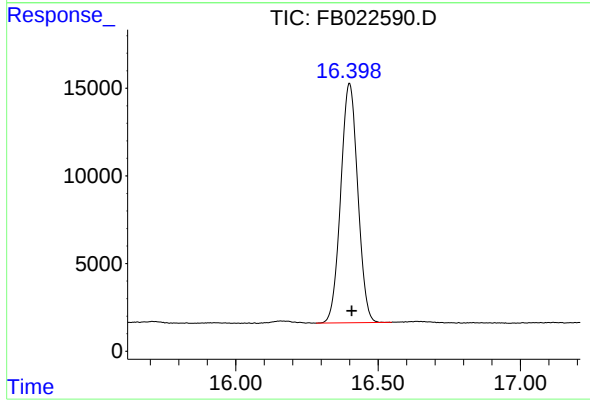

#10 1,2,4-Trimethylbenzene

R.T.: 16.400 min
Delta R.T.: -0.007 min
Response: 568065
Conc: 21.79 ng/ml