

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092420\
 Data File : FB024938.D
 Signal(s) : FID2B.CH
 Acq On : 24 Sep 2020 17:33
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 25 00:52:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	412169	19.633 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	903579	30.046 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	931797	30.487 ng/ml
3) t n-Heptane	7.761	310623	10.211 ng/ml
4) t Benzene	7.895	381196	10.233 ng/ml
6) t Toluene	10.633	1064759	30.500 ng/ml
7) t Ethylbenzene	13.073	325316	10.036 ng/ml
8) t m-Xylene	13.205	645063	20.307 ng/ml
9) t O-Xylene	13.933	620023	20.404 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	514382	20.281 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092420\
Data File : FB024938.D
Signal(s) : FID2B.CH
Acq On : 24 Sep 2020 17:33
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 25 00:52:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

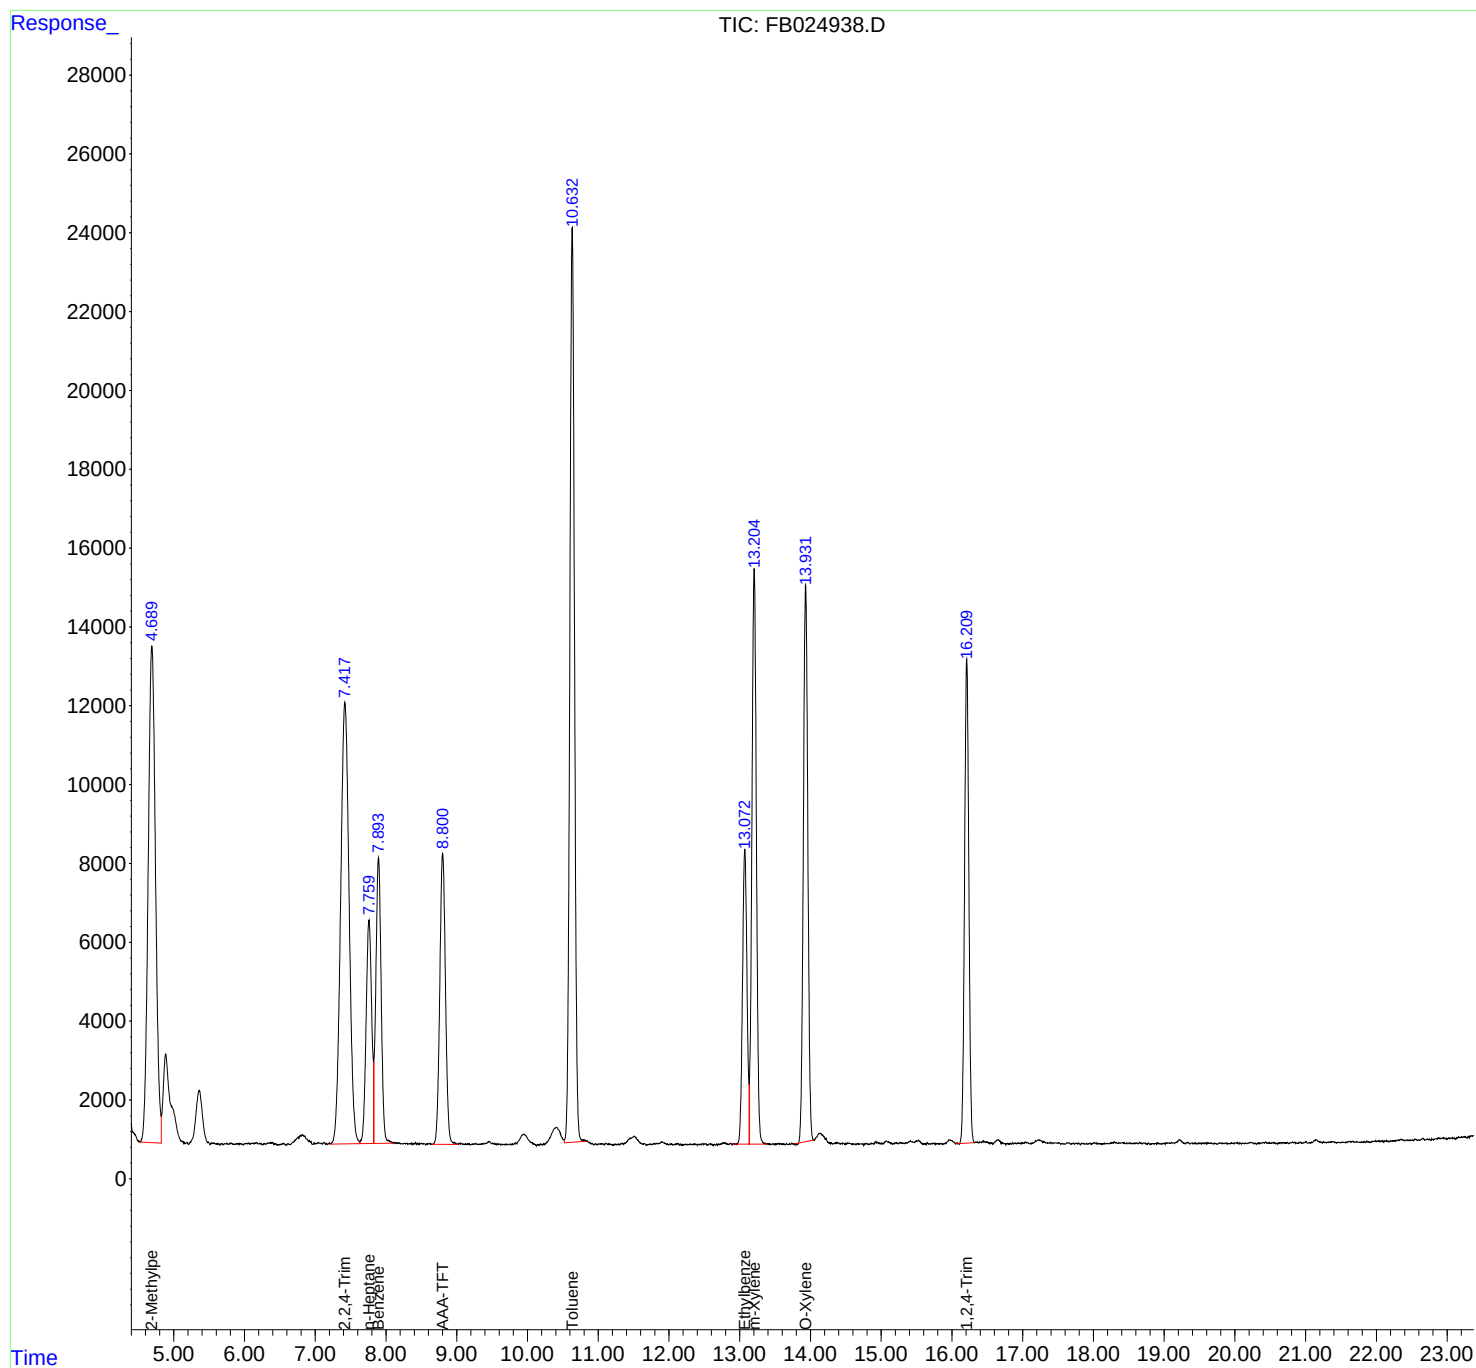

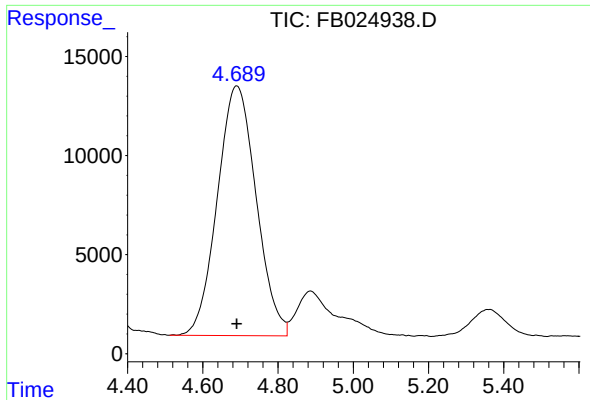


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 903579
Conc: 30.05 ng/ml

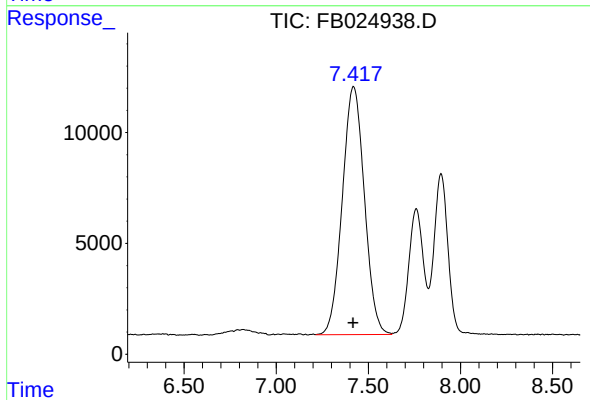


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 931797
Conc: 30.49 ng/ml

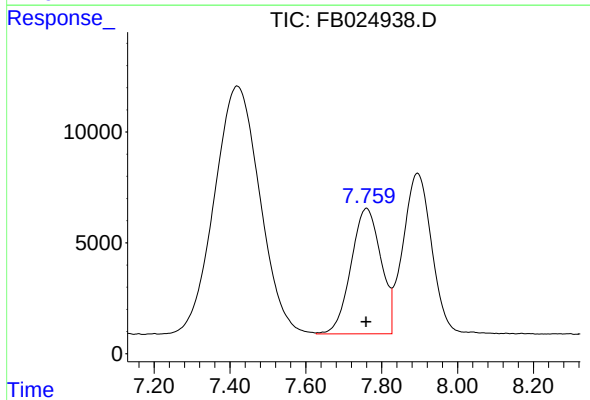


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.002 min
Response: 310623
Conc: 10.21 ng/ml

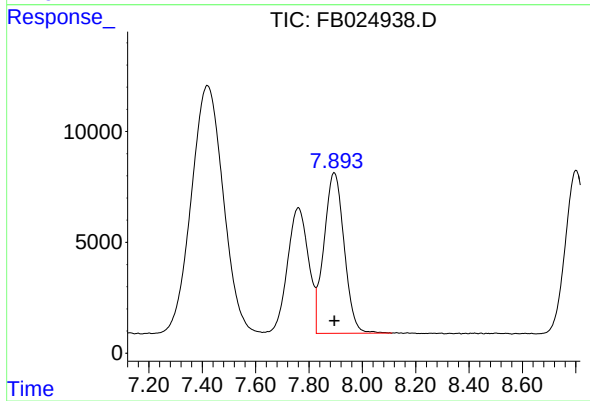


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 381196
Conc: 10.23 ng/ml

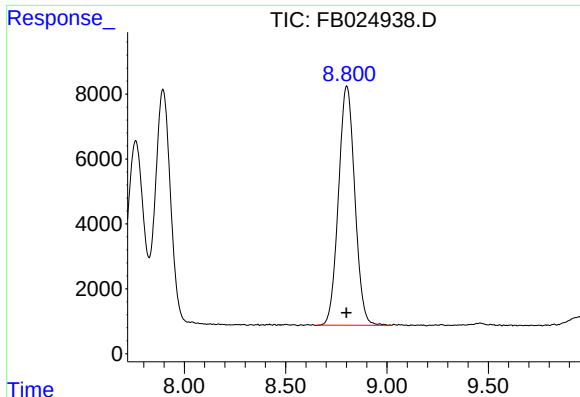


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.001 min
Response: 412169
Conc: 19.63 ng/ml

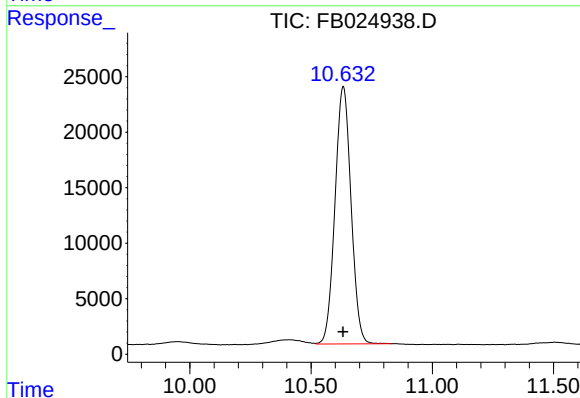


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.002 min
Response: 1064759
Conc: 30.50 ng/ml

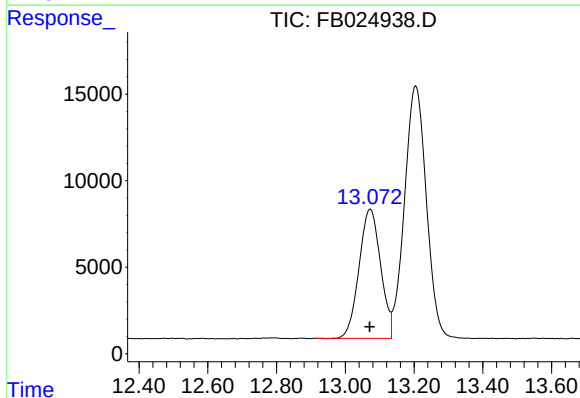


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.001 min
Response: 325316
Conc: 10.04 ng/ml

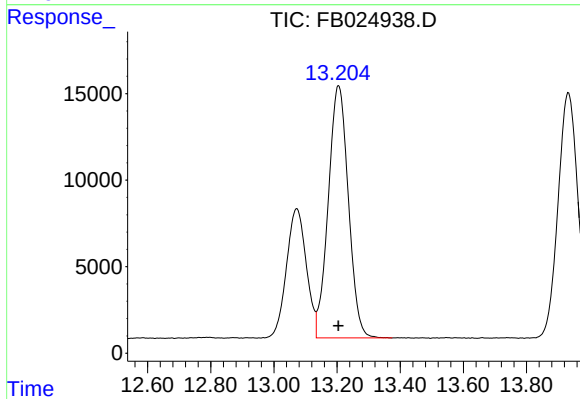


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.001 min
Response: 645063
Conc: 20.31 ng/ml

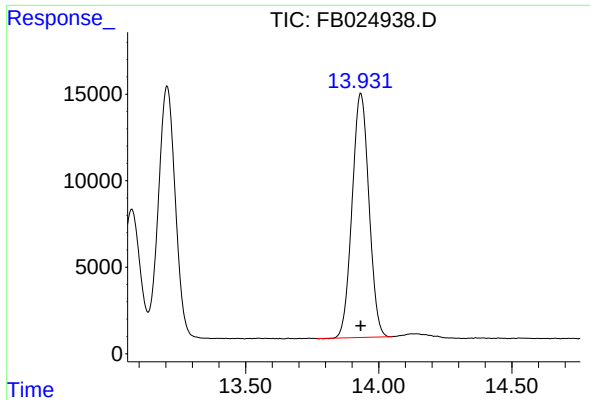

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 620023
Conc: 20.40 ng/ml

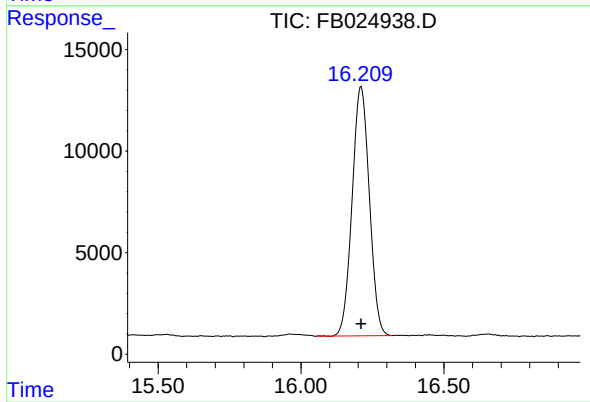

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 514382
Conc: 20.28 ng/ml