

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092518\
 Data File : FB017916.D
 Signal(s) : FID2B.CH
 Acq On : 25 Sep 2018 10:41 am
 Operator : MJ/SJ
 Sample : J5055-05MSD
 Misc : 5.03g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 26 07:58:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.098	77381	9.148 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.949	133883	8.407 ng/ml
2) t 2,2,4-Trimethylpentane	7.713	114583	7.200 ng/ml
3) t n-Heptane	8.054	38356	2.489 ng/ml
4) t Benzene	8.192	74052	3.890 ng/ml
6) t Toluene	10.953	198675	12.554 ng/ml
7) t Ethylbenzene	13.404	76491	4.681 ng/ml
8) t m-Xylene	13.536	153888	8.895 ng/ml
9) t O-Xylene	14.268	158608	8.728 ng/ml
10) t 1,2,4-Trimethylbenzene	16.550	154718	7.273 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092518\
Data File : FB017916.D
Signal(s) : FID2B.CH
Acq On : 25 Sep 2018 10:41 am
Operator : MJ/SJ
Sample : J5055-05MSD
Misc : 5.03g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 26 07:58:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

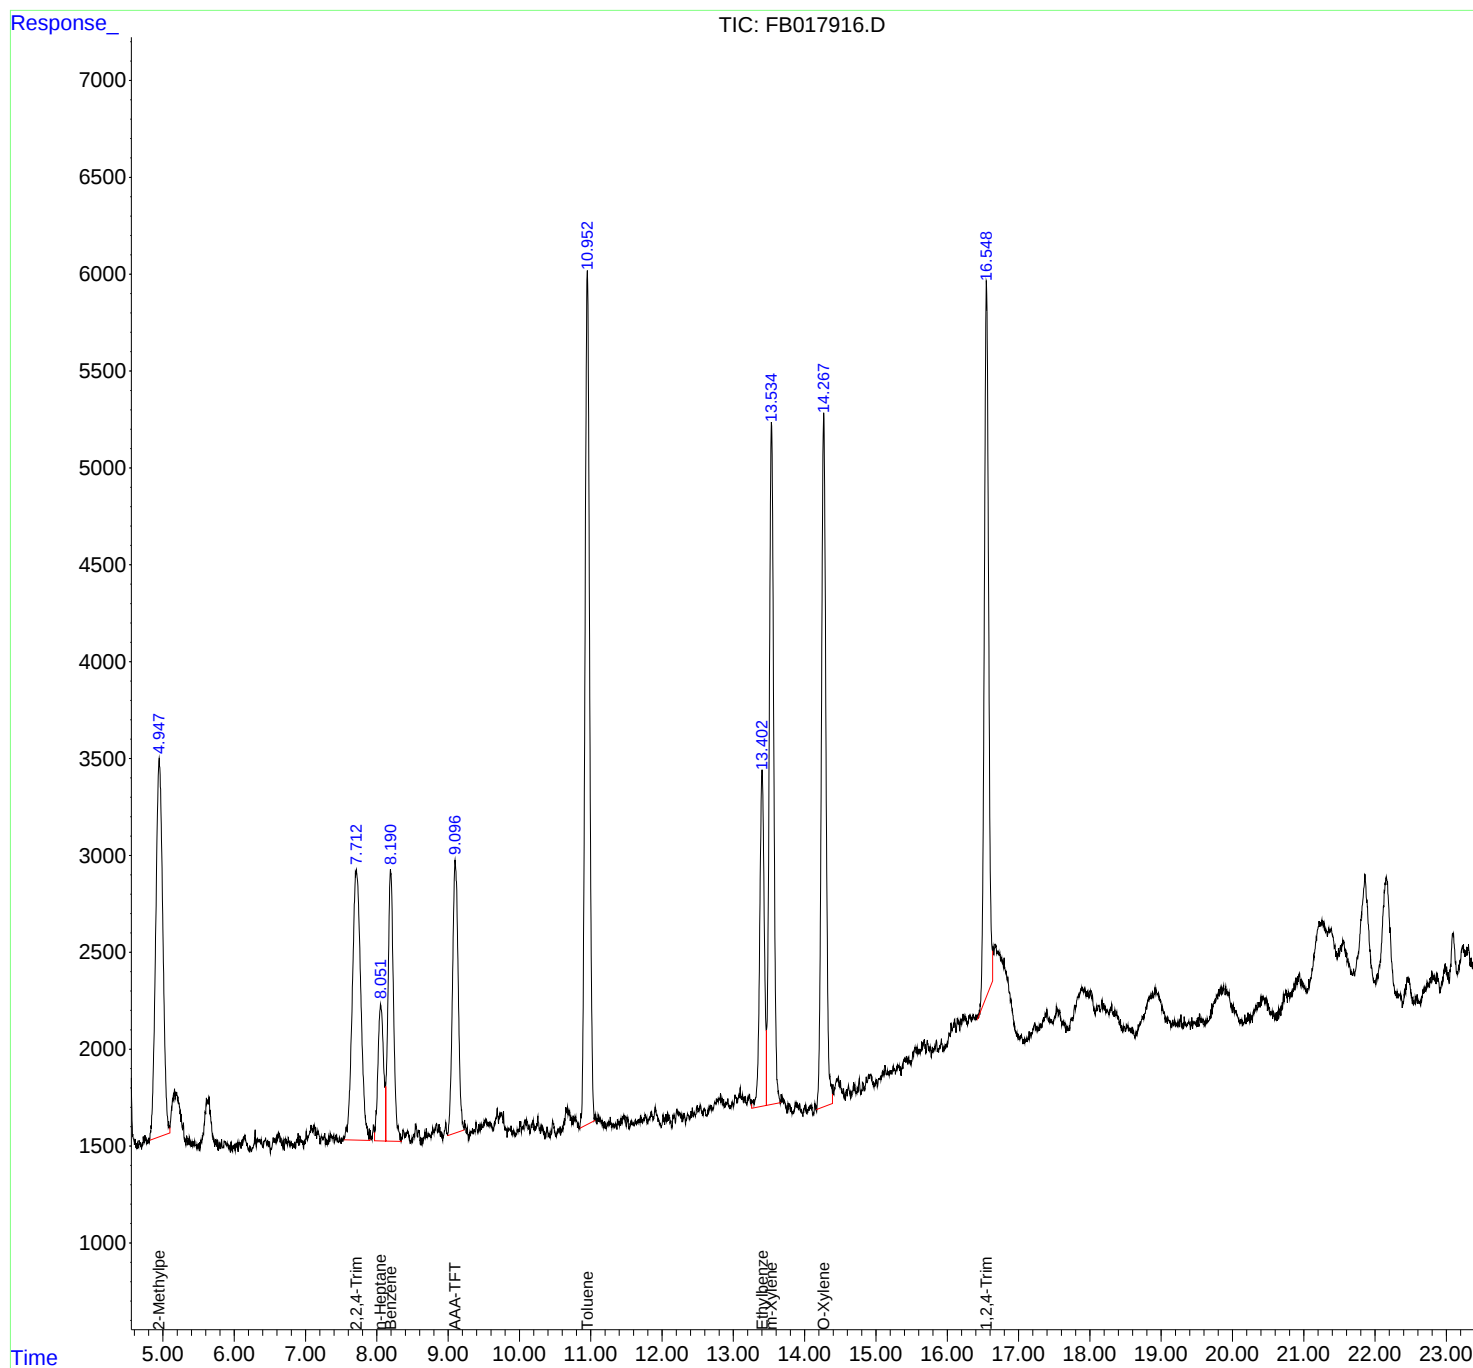

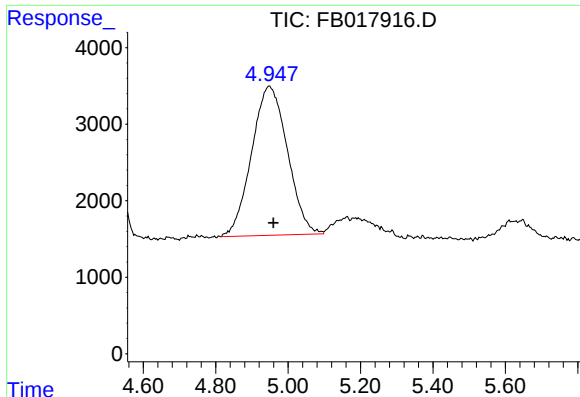


#1 2-Methylpentane

R.T.: 4.949 min
Delta R.T.: -0.011 min
Response: 133883
Conc: 8.41 ng/ml

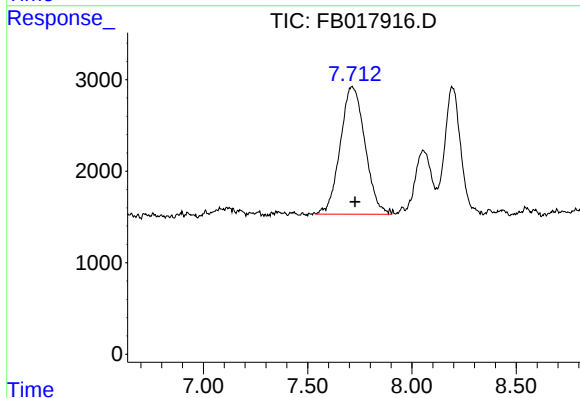


#2 2,2,4-Trimethylpentane

R.T.: 7.713 min
Delta R.T.: -0.014 min
Response: 114583
Conc: 7.20 ng/ml

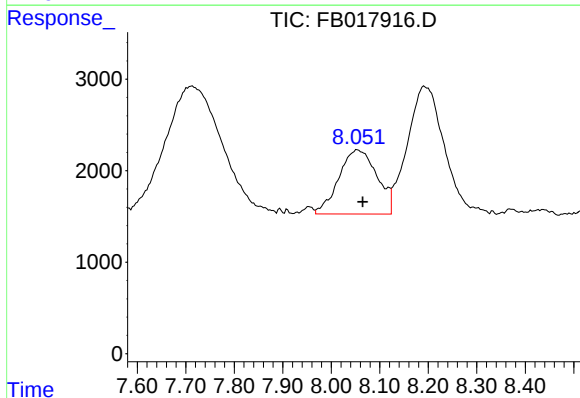


#3 n-Heptane

R.T.: 8.054 min
Delta R.T.: -0.011 min
Response: 38356
Conc: 2.49 ng/ml

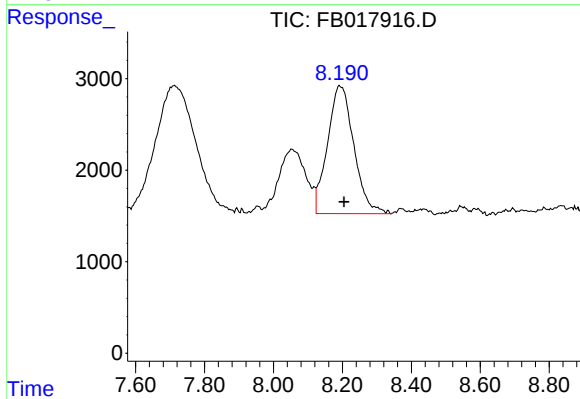


#4 Benzene

R.T.: 8.192 min
Delta R.T.: -0.012 min
Response: 74052
Conc: 3.89 ng/ml

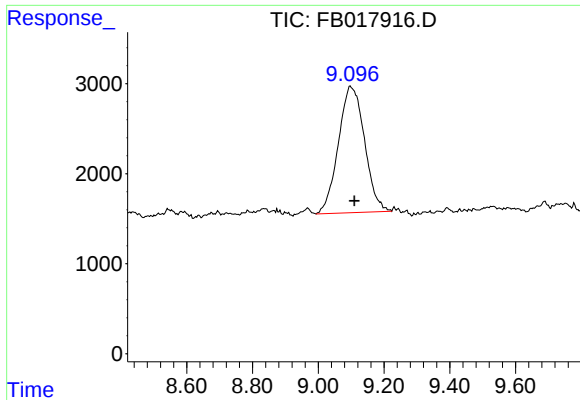


#5 AAA-TFT

R.T.: 9.098 min
Delta R.T.: -0.012 min
Response: 77381
Conc: 9.15 ng/ml

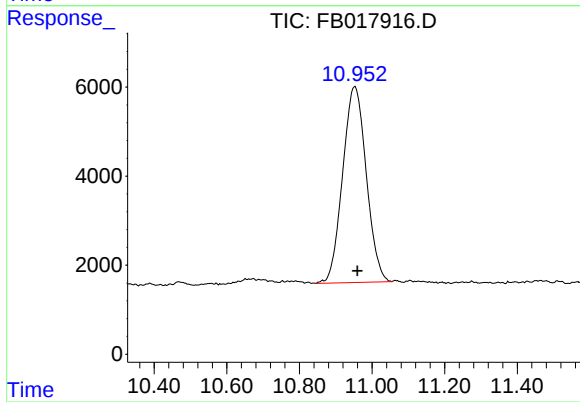


#6 Toluene

R.T.: 10.953 min
Delta R.T.: -0.006 min
Response: 198675
Conc: 12.55 ng/ml

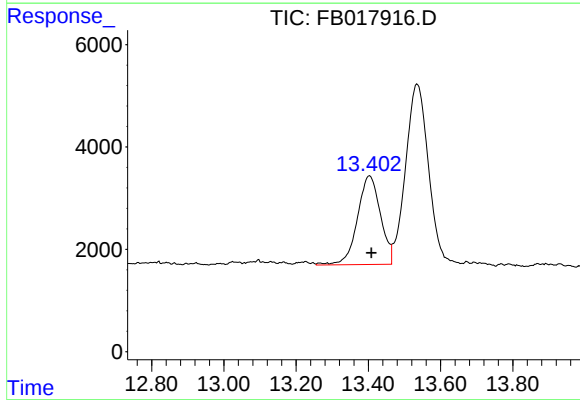


#7 Ethylbenzene

R.T.: 13.404 min
Delta R.T.: -0.005 min
Response: 76491
Conc: 4.68 ng/ml

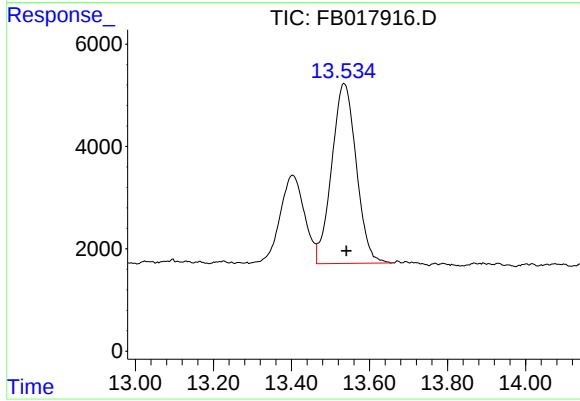


#8 m-Xylene

R.T.: 13.536 min
Delta R.T.: -0.006 min
Response: 153888
Conc: 8.90 ng/ml

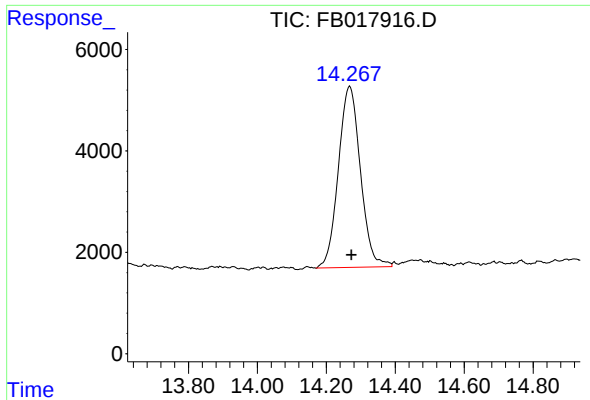

#9 O-Xylene

R.T.: 14.268 min
Delta R.T.: -0.005 min
Response: 158608
Conc: 8.73 ng/ml

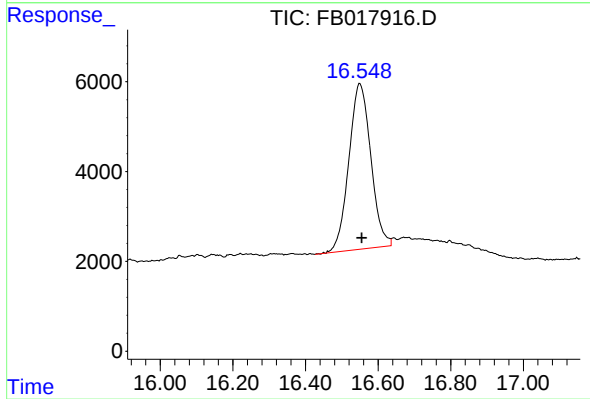

#10 1,2,4-Trimethylbenzene

R.T.: 16.550 min
Delta R.T.: -0.006 min
Response: 154718
Conc: 7.27 ng/ml