

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092518\
 Data File : FB017913.D
 Signal(s) : FID2B.CH
 Acq On : 25 Sep 2018 8:58
 Operator : MJ/SJ
 Sample : BSF0925S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 26 07:57:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.104	179851	21.262 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.956	450650	28.298 ng/ml
2) t 2,2,4-Trimethylpentane	7.720	468744	29.455 ng/ml
3) t n-Heptane	8.059	148944	9.665 ng/ml
4) t Benzene	8.199	187901	9.870 ng/ml
6) t Toluene	10.953	485663	30.687 ng/ml
7) t Ethylbenzene	13.403	170828	10.455 ng/ml
8) t m-Xylene	13.535	365199	21.110 ng/ml
9) t O-Xylene	14.267	383045	21.079 ng/ml
10) t 1,2,4-Trimethylbenzene	16.550	426467	20.049 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092518\
Data File : FB017913.D
Signal(s) : FID2B.CH
Acq On : 25 Sep 2018 8:58
Operator : MJ/SJ
Sample : BSF0925S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 26 07:57:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

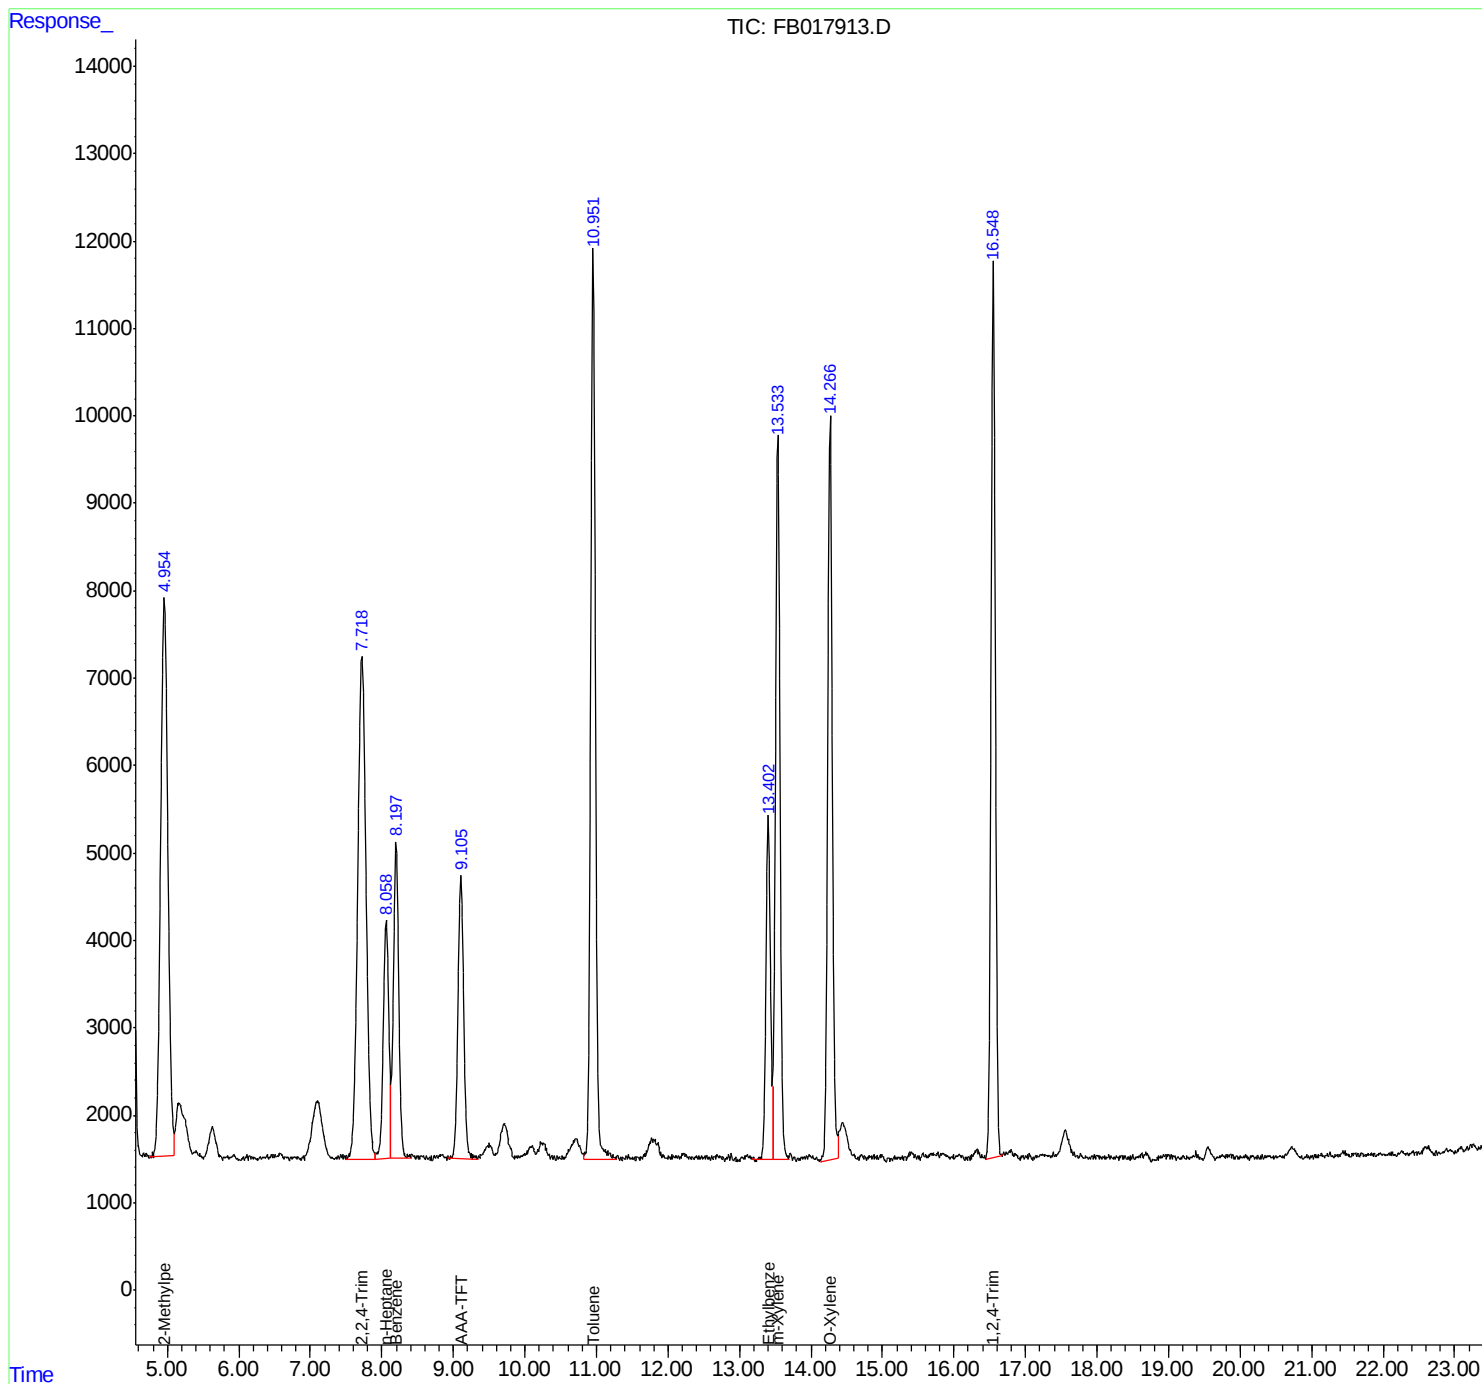

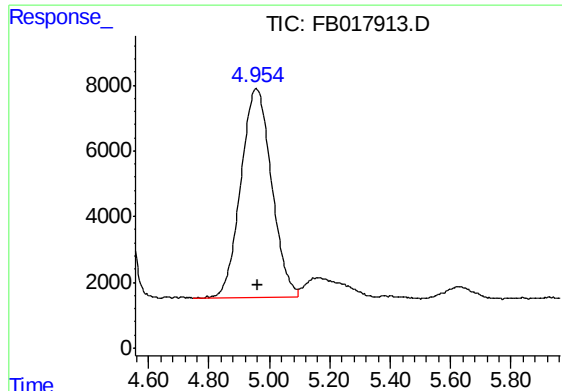


#1 2-Methylpentane

R.T.: 4.956 min
Delta R.T.: -0.004 min
Response: 450650
Conc: 28.30 ng/ml

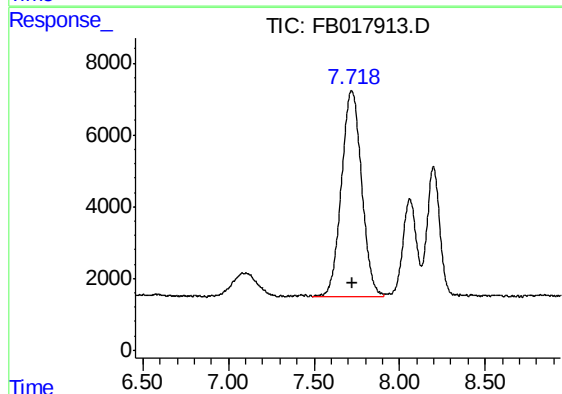


#2 2,2,4-Trimethylpentane

R.T.: 7.720 min
Delta R.T.: -0.007 min
Response: 468744
Conc: 29.46 ng/ml

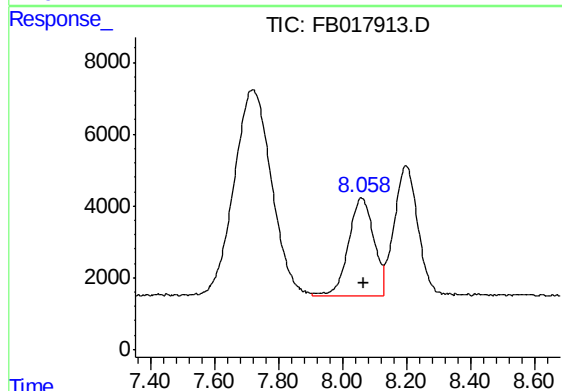


#3 n-Heptane

R.T.: 8.059 min
Delta R.T.: -0.006 min
Response: 148944
Conc: 9.67 ng/ml

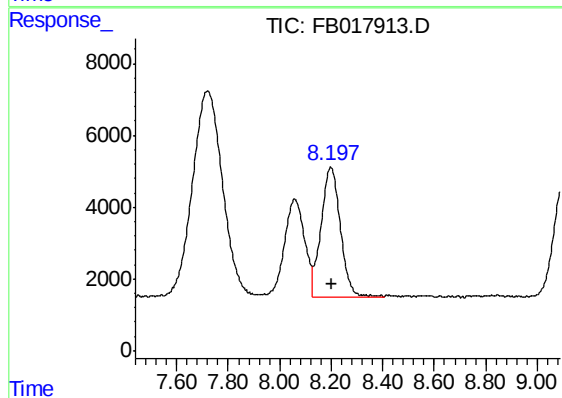


#4 Benzene

R.T.: 8.199 min
Delta R.T.: -0.005 min
Response: 187901
Conc: 9.87 ng/ml

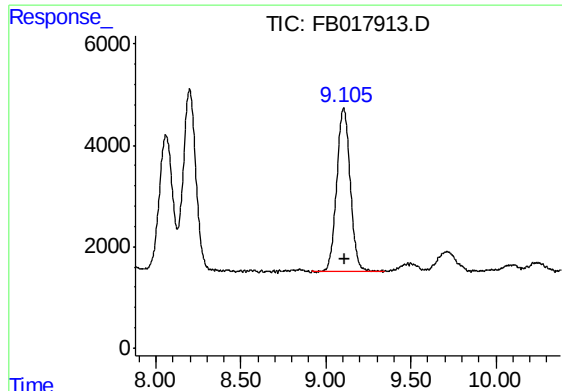


#5 AAA-TFT

R.T.: 9.104 min
Delta R.T.: -0.006 min
Response: 179851
Conc: 21.26 ng/ml

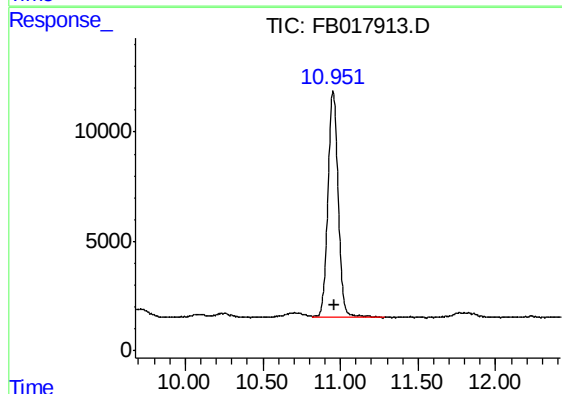


#6 Toluene

R.T.: 10.953 min
Delta R.T.: -0.007 min
Response: 485663
Conc: 30.69 ng/ml

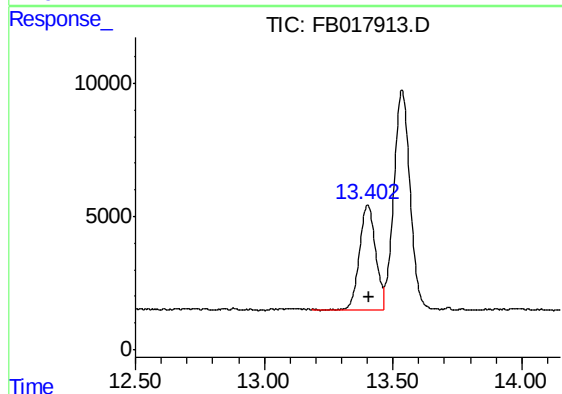


#7 Ethylbenzene

R.T.: 13.403 min
Delta R.T.: -0.006 min
Response: 170828
Conc: 10.45 ng/ml

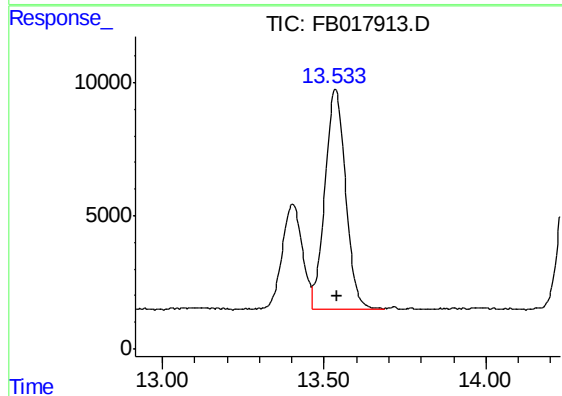


#8 m-Xylene

R.T.: 13.535 min
Delta R.T.: -0.006 min
Response: 365199
Conc: 21.11 ng/ml

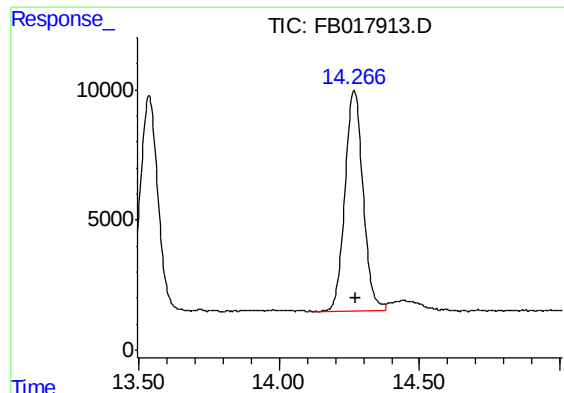

#9 O-Xylene

R.T.: 14.267 min
Delta R.T.: -0.006 min
Response: 383045
Conc: 21.08 ng/ml

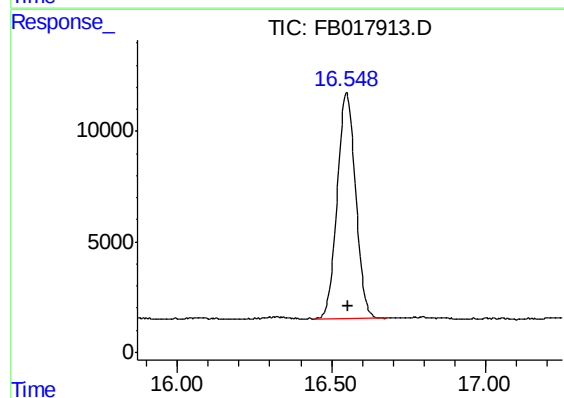

#10 1,2,4-Trimethylbenzene

R.T.: 16.550 min
Delta R.T.: -0.006 min
Response: 426467
Conc: 20.05 ng/ml