

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092520\
 Data File : FB024947.D
 Signal(s) : FID2B.CH
 Acq On : 25 Sep 2020 12:26
 Operator : DD/AJ
 Sample : BSF0925S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 26 00:06:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.799	415114	19.773 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	936690	31.147 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	978575	32.018 ng/ml
3) t	n-Heptane	7.757	323198	10.624 ng/ml
4) t	Benzene	7.892	382163	10.259 ng/ml
6) t	Toluene	10.630	1076912	30.849 ng/ml
7) t	Ethylbenzene	13.070	332992	10.273 ng/ml
8) t	m-Xylene	13.203	656476	20.666 ng/ml
9) t	O-Xylene	13.931	631533	20.783 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	531019	20.937 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092520\
Data File : FB024947.D
Signal(s) : FID2B.CH
Acq On : 25 Sep 2020 12:26
Operator : DD/AJ
Sample : BSF0925S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 26 00:06:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

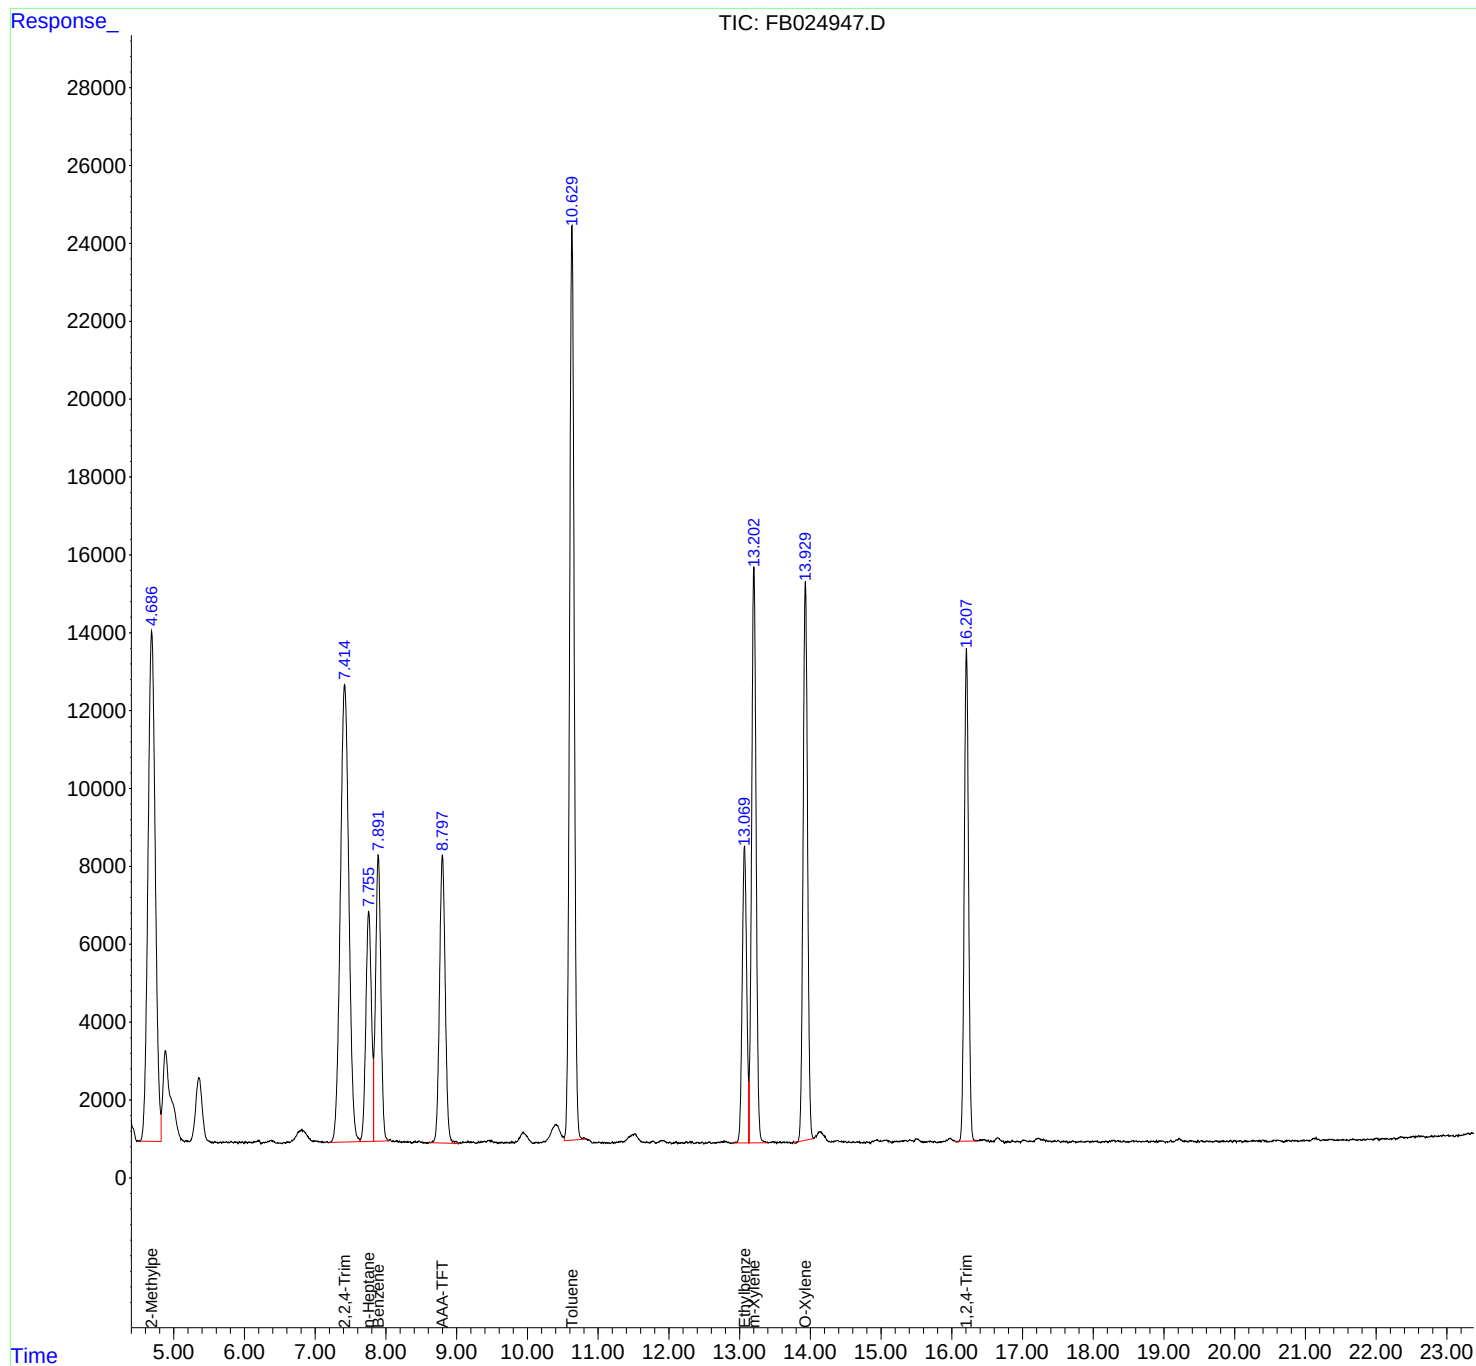

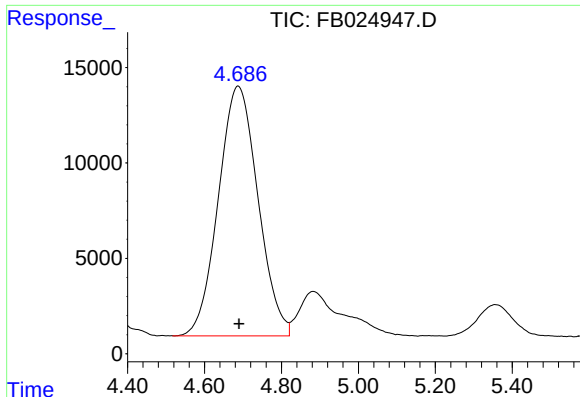


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 936690
Conc: 31.15 ng/ml

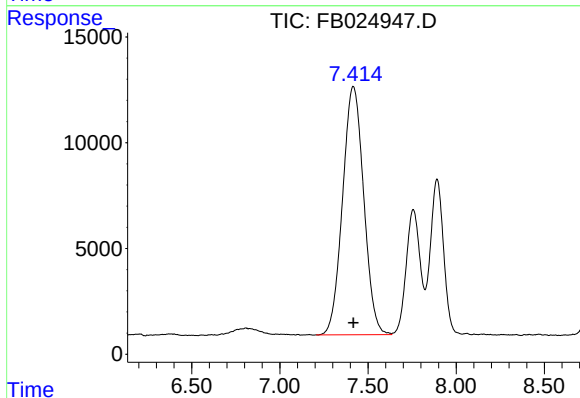


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.003 min
Response: 978575
Conc: 32.02 ng/ml

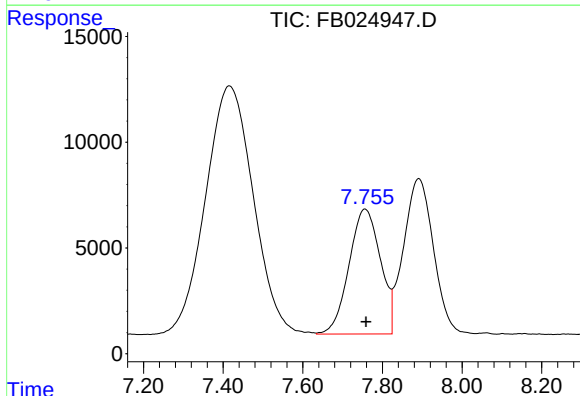


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 323198
Conc: 10.62 ng/ml

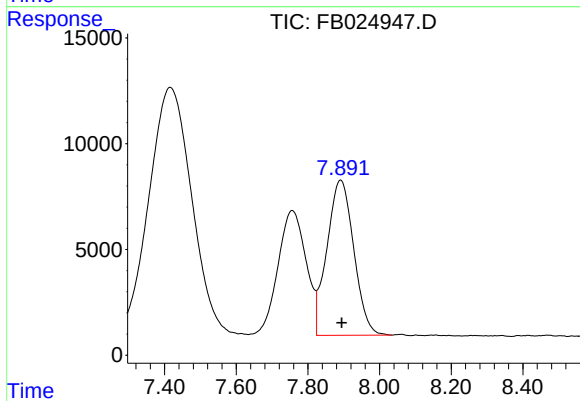


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 382163
Conc: 10.26 ng/ml

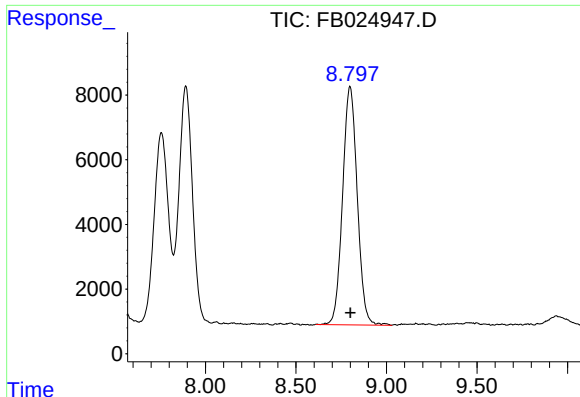


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.002 min
Response: 415114
Conc: 19.77 ng/ml

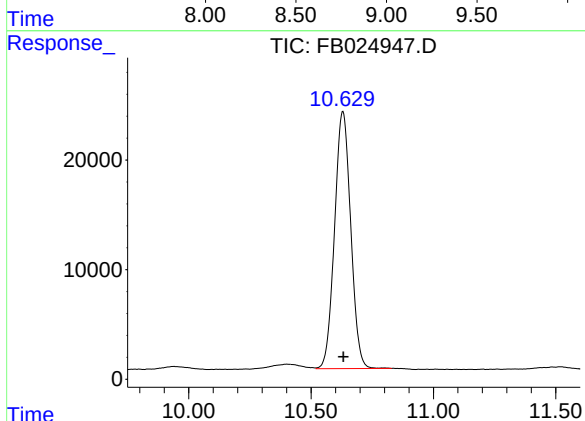


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.001 min
Response: 1076912
Conc: 30.85 ng/ml

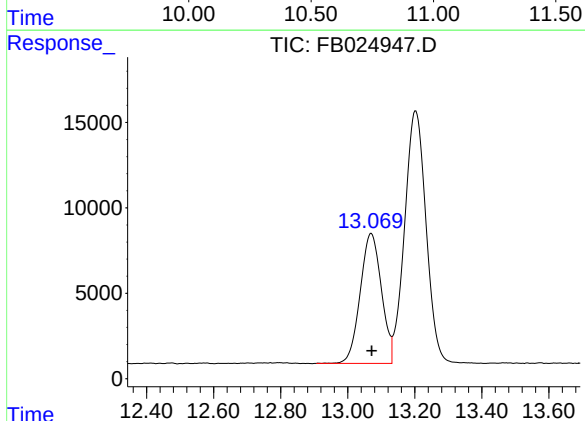


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.001 min
Response: 332992
Conc: 10.27 ng/ml

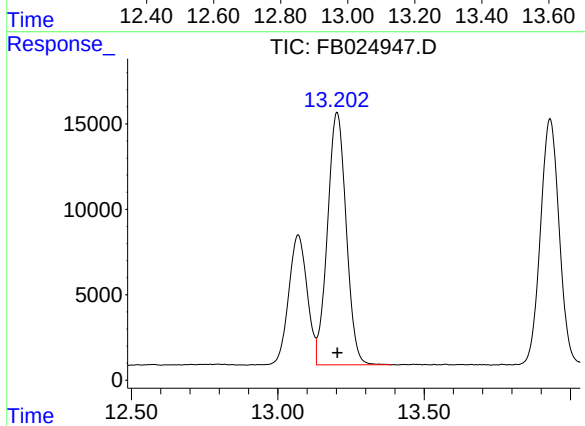


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: -0.001 min
Response: 656476
Conc: 20.67 ng/ml

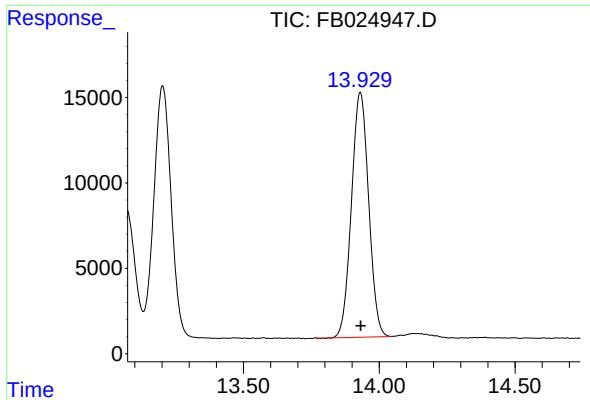

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.001 min
Response: 631533
Conc: 20.78 ng/ml

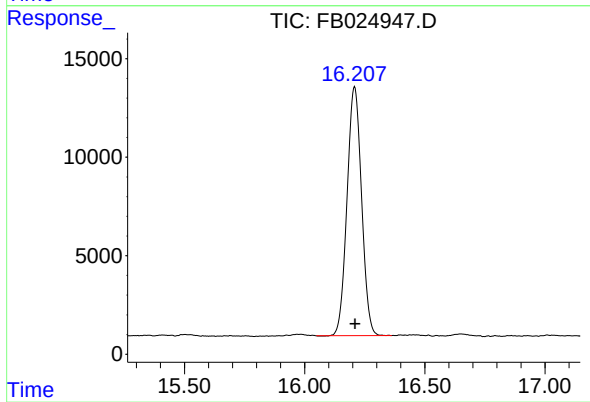

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 531019
Conc: 20.94 ng/ml