

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092619\
 Data File : FB022593.D
 Signal(s) : FID2B.CH
 Acq On : 26 Sep 2019 8:56
 Operator : DD/AJ
 Sample : VBF0926S1
 Misc : 5.00g/5.00ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF0926S1

Integration File: Calibration.e
 Quant Time: Sep 27 01:40:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.966	591560	20.337 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.825	29470	0.600 ng/ml
2) t 2,2,4-Trimethylpentane	7.603	6798	0.132 ng/ml
3) t n-Heptane	7.928	4629	0.092 ng/ml
6) t Toluene	10.819	14888	0.313 ng/ml
7) t Ethylbenzene	13.227	5297	0.177 ng/ml
8) t m-Xylene	13.379	5121	0.193 ng/ml
9) t O-Xylene	14.122	7641	0.315 ng/ml
10) t 1,2,4-Trimethylbenzene	16.408	9333	0.358 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092619\
Data File : FB022593.D
Signal(s) : FID2B.CH
Acq On : 26 Sep 2019 8:56
Operator : DD/AJ
Sample : VBF0926S1
Misc : 5.00g/5.00ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0926S1

Integration File: Calibration.e
Quant Time: Sep 27 01:40:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

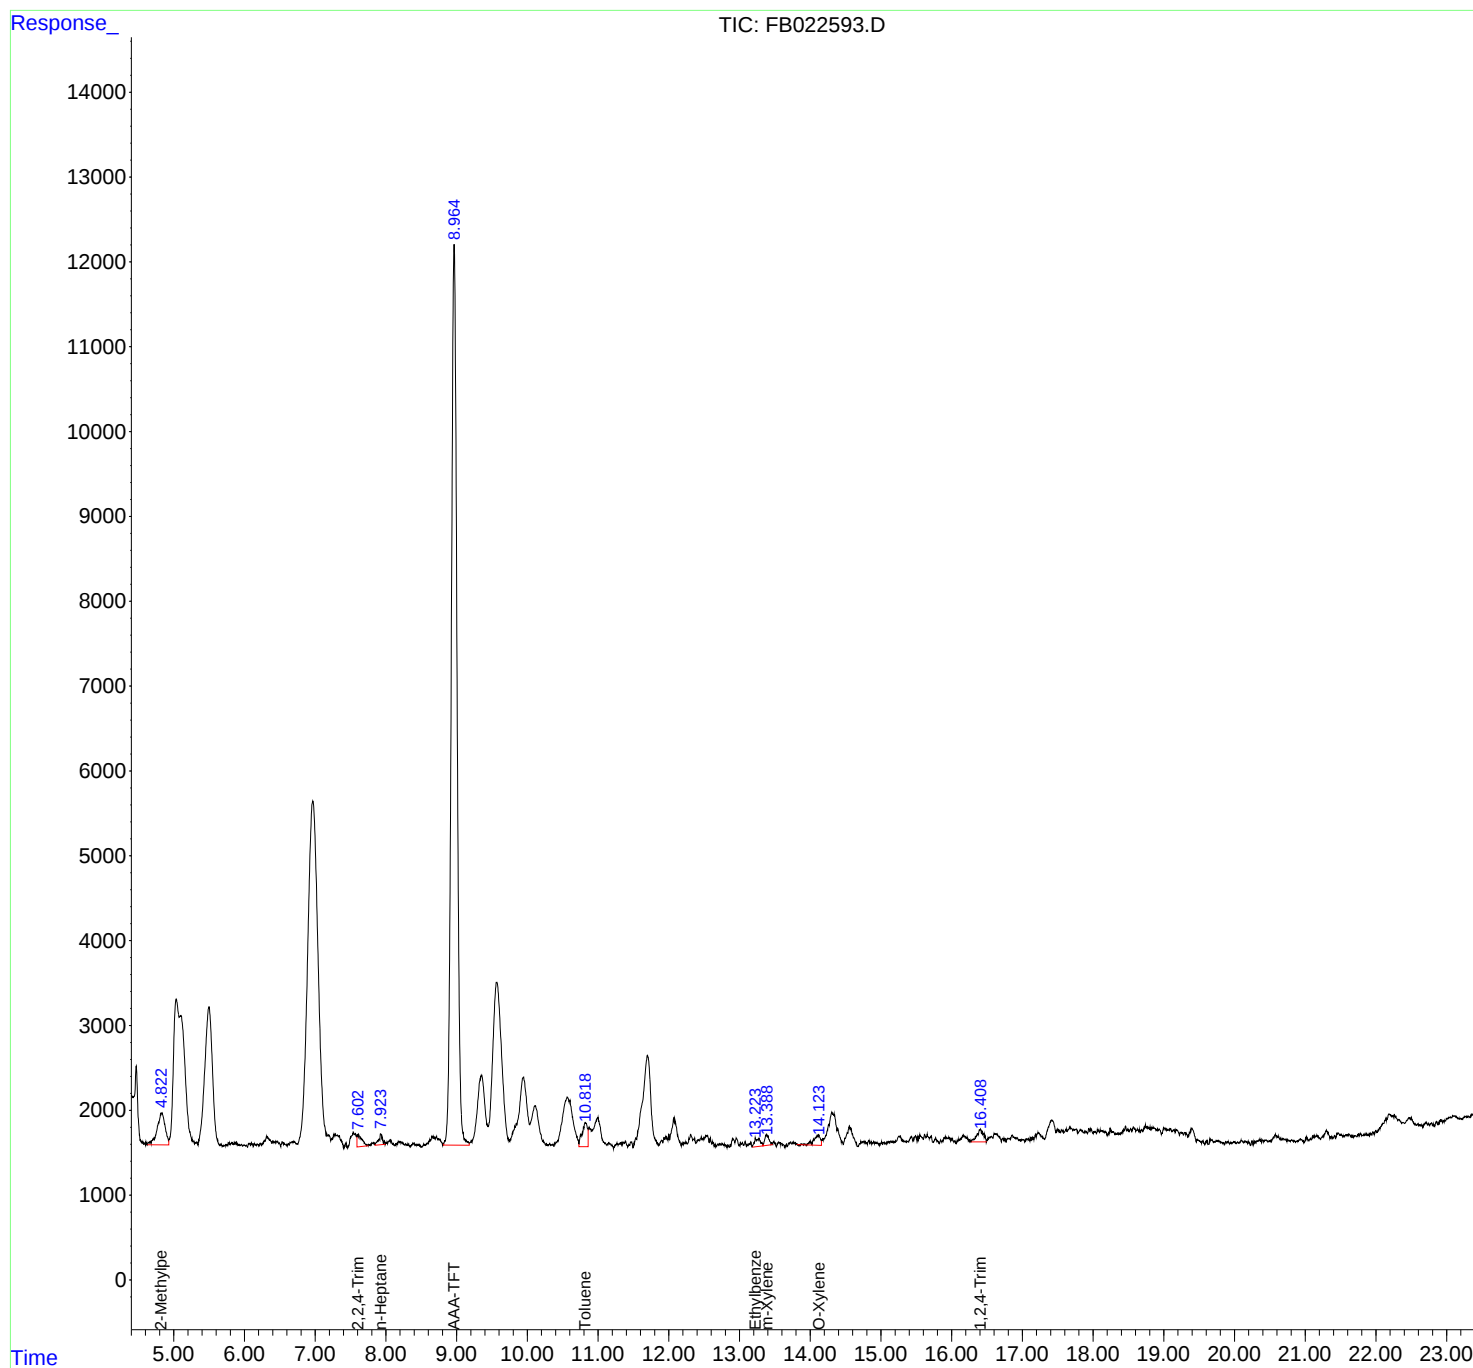


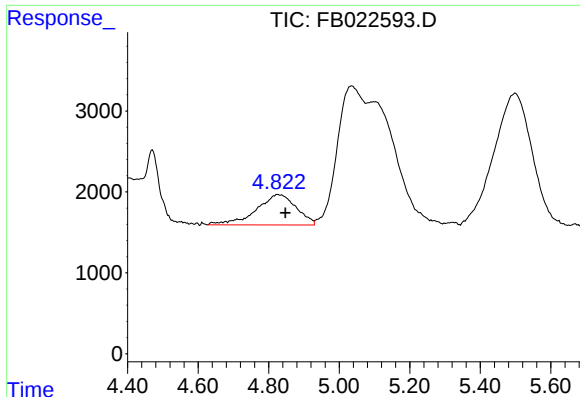

#1 2-Methylpentane


R.T.: 4.825 min
Delta R.T.: -0.022 min
Response: 29470
Conc: 0.60 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0926S1

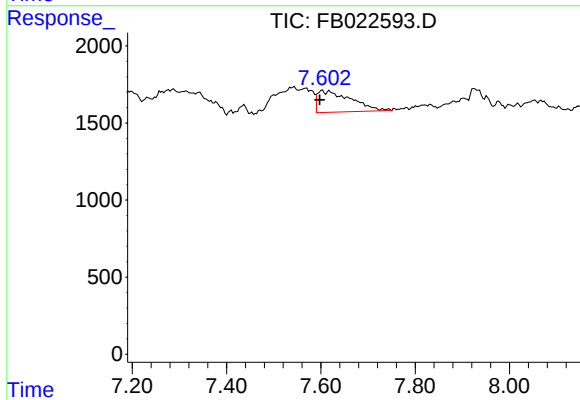


#2 2,2,4-Trimethylpentane

R.T.: 7.603 min
Delta R.T.: 0.005 min
Response: 6798
Conc: 0.13 ng/ml

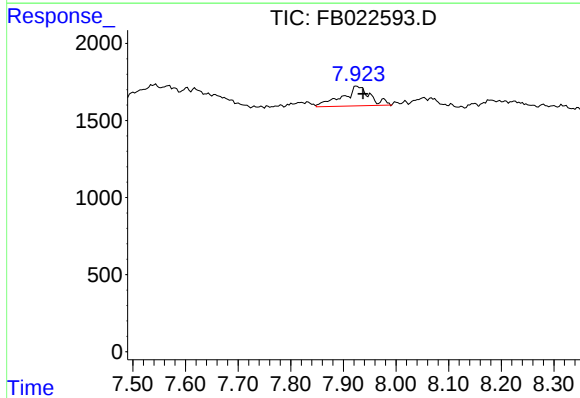


#3 n-Heptane

R.T.: 7.928 min
Delta R.T.: -0.009 min
Response: 4629
Conc: 0.09 ng/ml

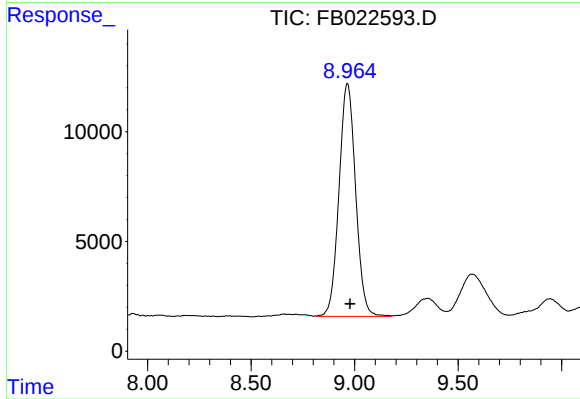

#5 AAA-TFT


R.T.: 8.966 min
Delta R.T.: -0.013 min
Response: 591560
Conc: 20.34 ng/ml

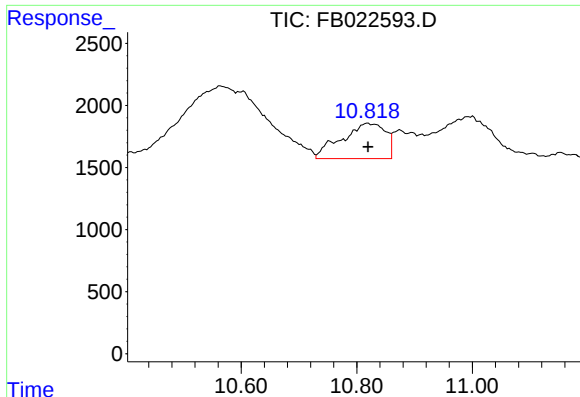

#6 Toluene


R.T.: 10.819 min
Delta R.T.: 0.000 min
Response: 14888
Conc: 0.31 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0926S1

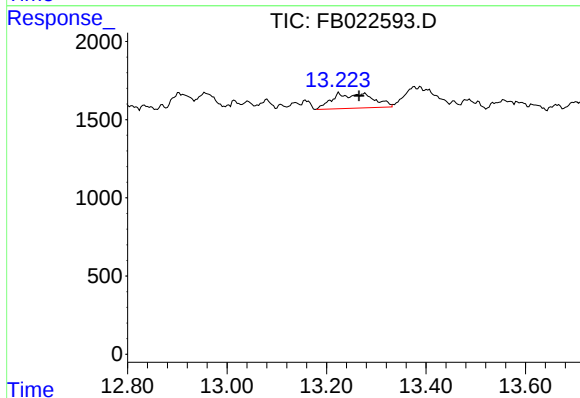


#7 Ethylbenzene

R.T.: 13.227 min
Delta R.T.: -0.038 min
Response: 5297
Conc: 0.18 ng/ml

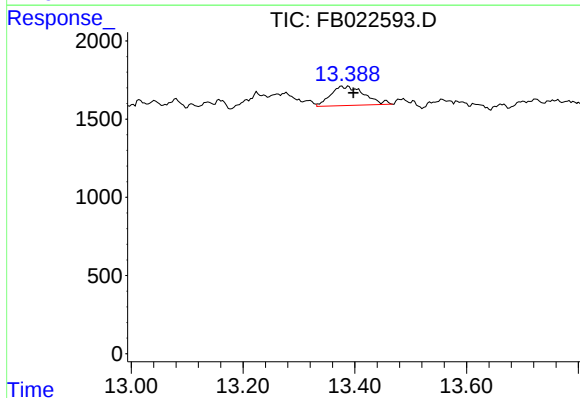


#8 m-Xylene

R.T.: 13.379 min
Delta R.T.: -0.018 min
Response: 5121
Conc: 0.19 ng/ml

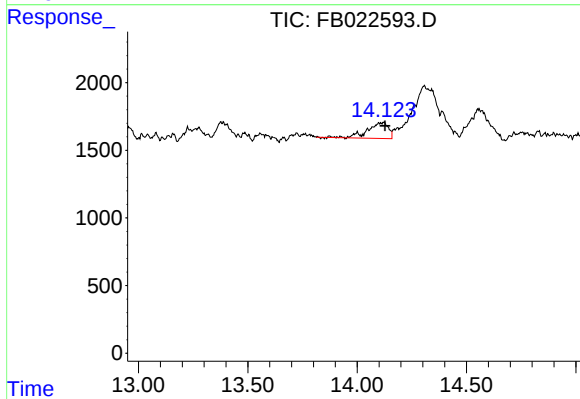

#9 O-Xylene

R.T.: 14.122 min
Delta R.T.: -0.006 min
Response: 7641
Conc: 0.31 ng/ml

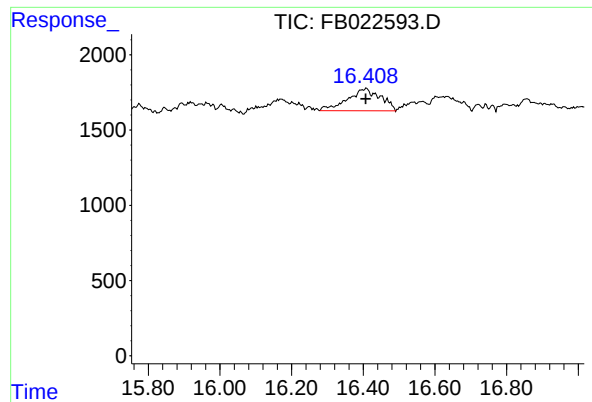

#10 1,2,4-Trimethylbenzene

R.T.: 16.408 min
Delta R.T.: 0.000 min
Response: 9333
Conc: 0.36 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0926S1