

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB092619\  
 Data File : FB022594.D  
 Signal(s) : FID2B.CH  
 Acq On : 26 Sep 2019 9:25  
 Operator : DD/AJ  
 Sample : BSF0926S1  
 Misc : 5.01g/5.00ML DI WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 BSF0926S1

Integration File: Calibration.e  
 Quant Time: Sep 27 01:40:46 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090419.M  
 Quant Title :  
 QLast Update : Wed Sep 04 17:01:40 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.966  | 588924   | 20.247 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.833  | 1057448  | 21.522 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.584  | 1223886  | 23.701 ng/ml |
| 3) t n-Heptane               | 7.924  | 396173   | 7.871 ng/ml  |
| 4) t Benzene                 | 8.059  | 489159   | 8.242 ng/ml  |
| 6) t Toluene                 | 10.807 | 1468881  | 30.876 ng/ml |
| 7) t Ethylbenzene            | 13.254 | 470671   | 15.700 ng/ml |
| 8) t m-Xylene                | 13.387 | 932174   | 35.089 ng/ml |
| 9) t O-Xylene                | 14.117 | 881337   | 36.329 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.397 | 612873   | 23.508 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB092619\  
Data File : FB022594.D  
Signal(s) : FID2B.CH  
Acq On : 26 Sep 2019 9:25  
Operator : DD/AJ  
Sample : BSF0926S1  
Misc : 5.01g/5.00ML DI WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
BSF0926S1

Integration File: Calibration.e  
Quant Time: Sep 27 01:40:46 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090419.M  
Quant Title :  
QLast Update : Wed Sep 04 17:01:40 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

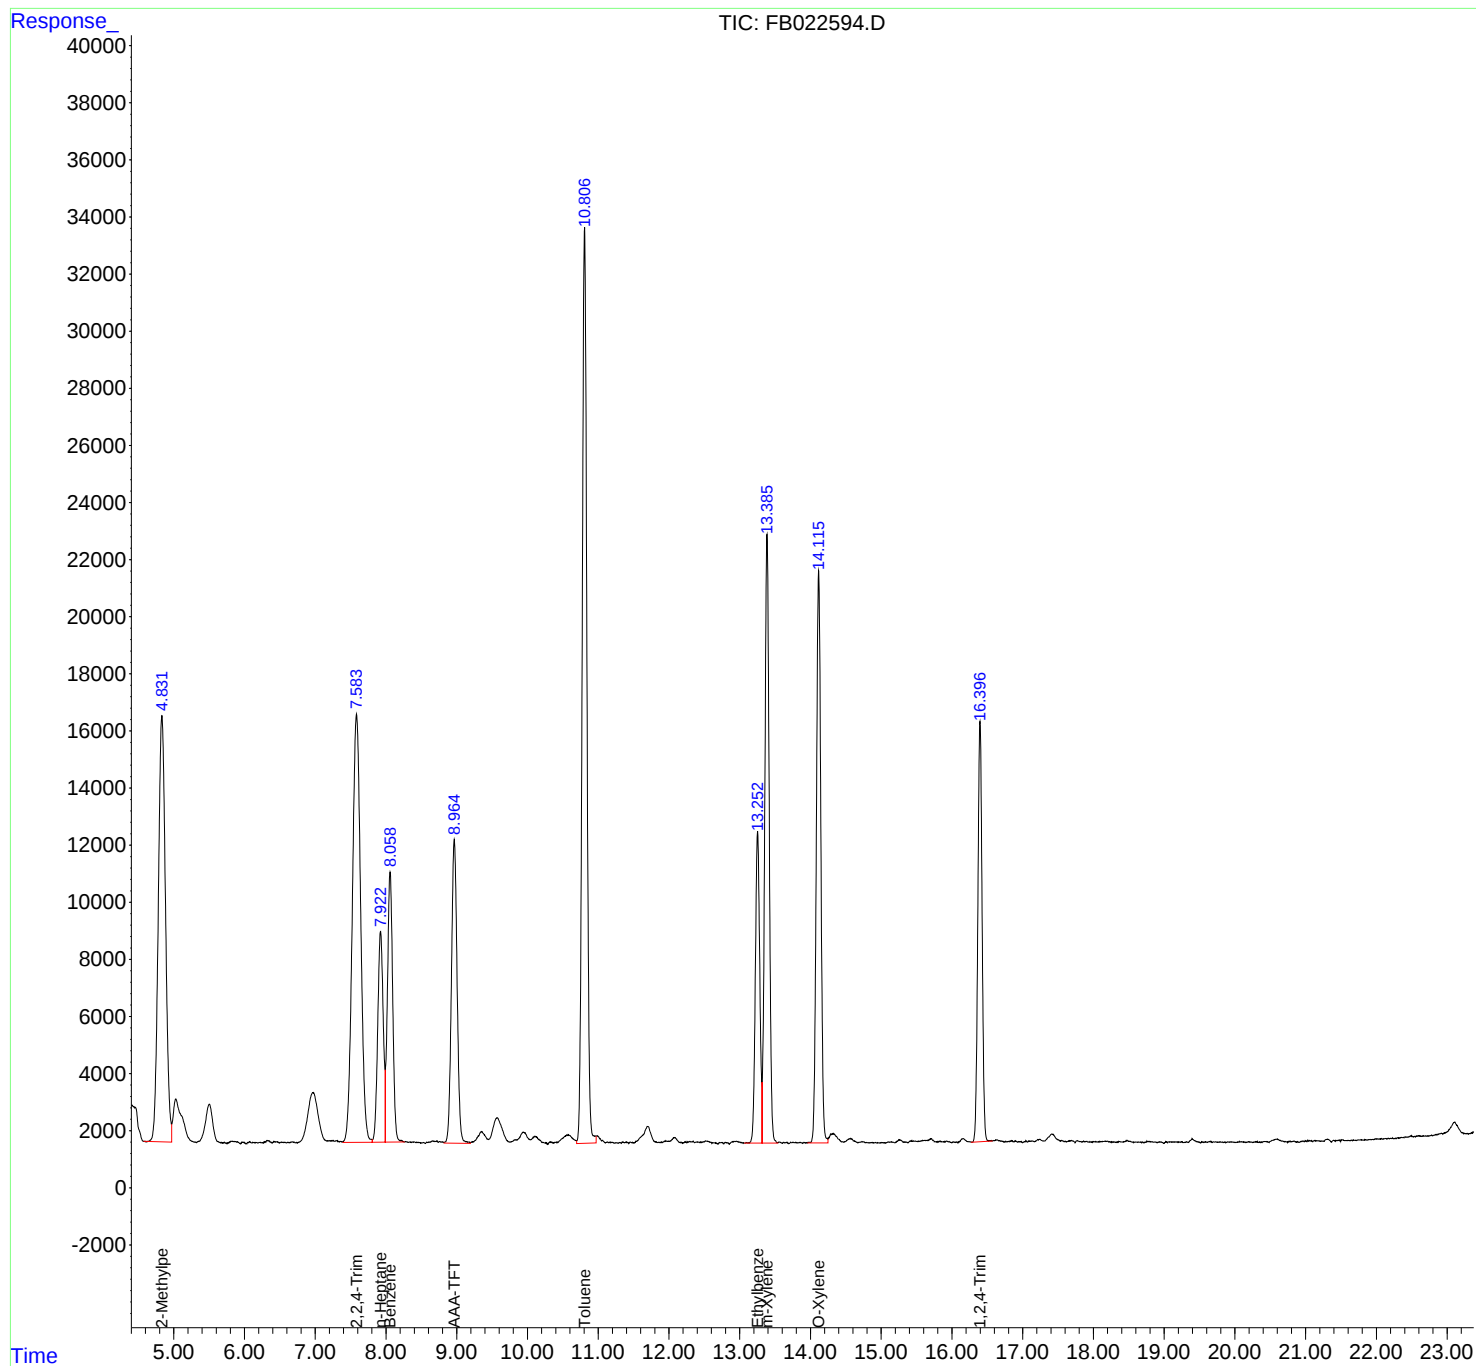


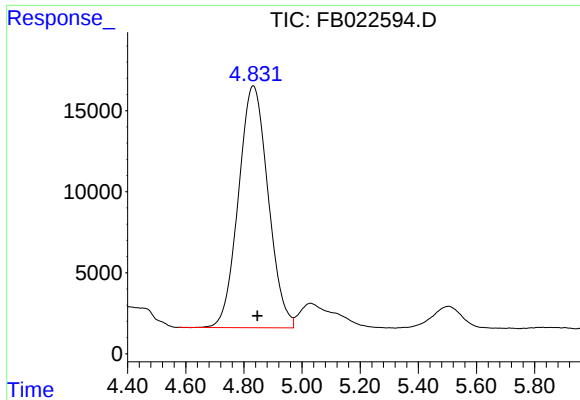

#1 2-Methylpentane


R.T.: 4.833 min  
Delta R.T.: -0.014 min  
Response: 1057448  
Conc: 21.52 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0926S1

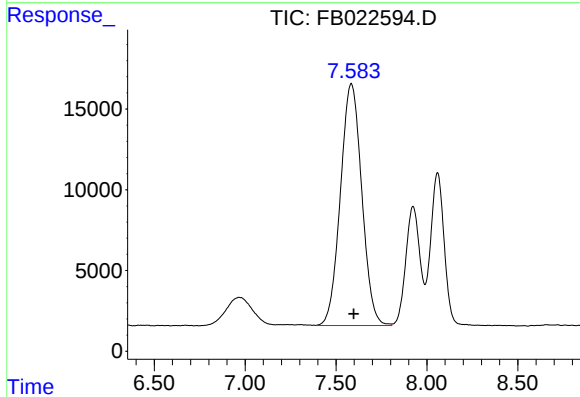


#2 2,2,4-Trimethylpentane

R.T.: 7.584 min  
Delta R.T.: -0.014 min  
Response: 1223886  
Conc: 23.70 ng/ml

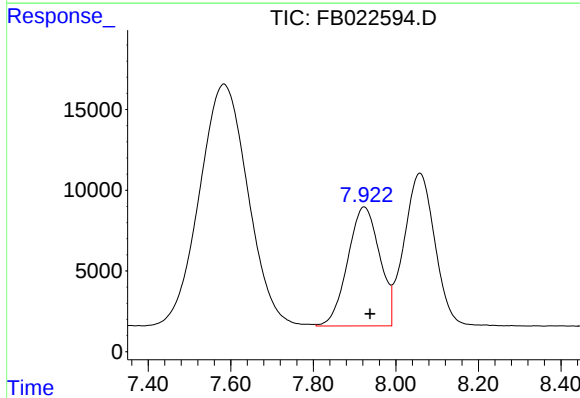


#3 n-Heptane

R.T.: 7.924 min  
Delta R.T.: -0.014 min  
Response: 396173  
Conc: 7.87 ng/ml

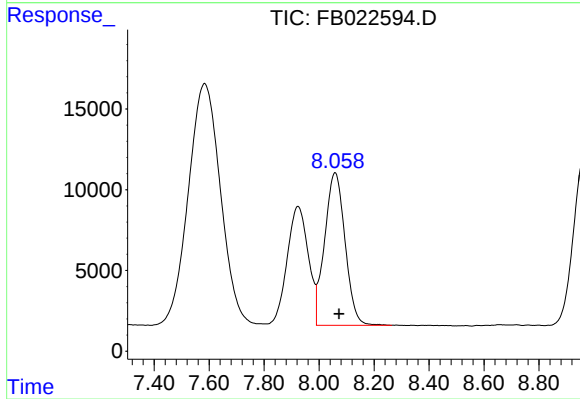

#4 Benzene


R.T.: 8.059 min  
Delta R.T.: -0.014 min  
Response: 489159  
Conc: 8.24 ng/ml

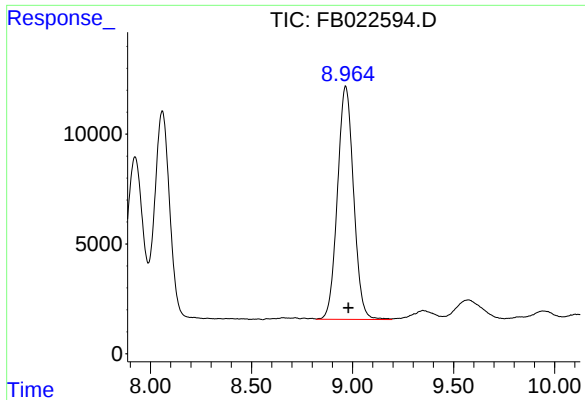

#5 AAA-TFT


R.T.: 8.966 min  
Delta R.T.: -0.013 min  
Response: 588924  
Conc: 20.25 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0926S1

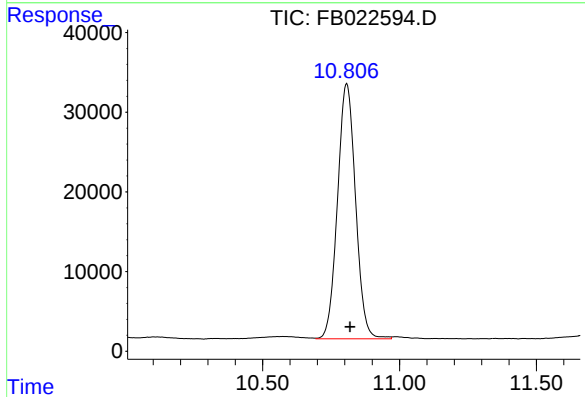


#6 Toluene

R.T.: 10.807 min  
Delta R.T.: -0.012 min  
Response: 1468881  
Conc: 30.88 ng/ml

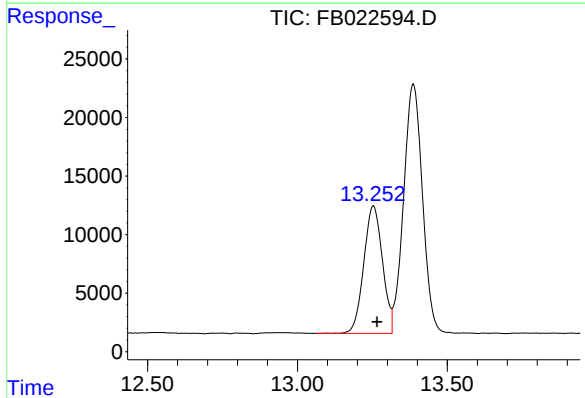


#7 Ethylbenzene

R.T.: 13.254 min  
Delta R.T.: -0.012 min  
Response: 470671  
Conc: 15.70 ng/ml

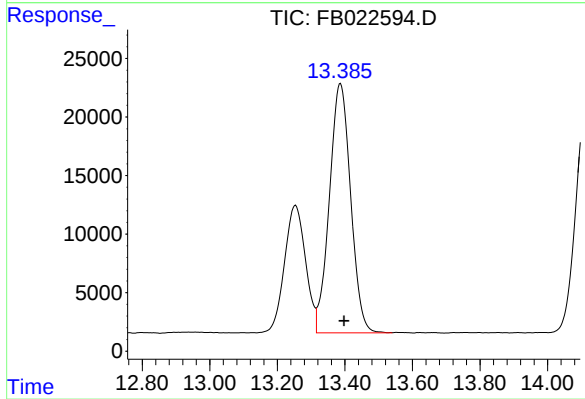

#8 m-Xylene

R.T.: 13.387 min  
Delta R.T.: -0.011 min  
Response: 932174  
Conc: 35.09 ng/ml

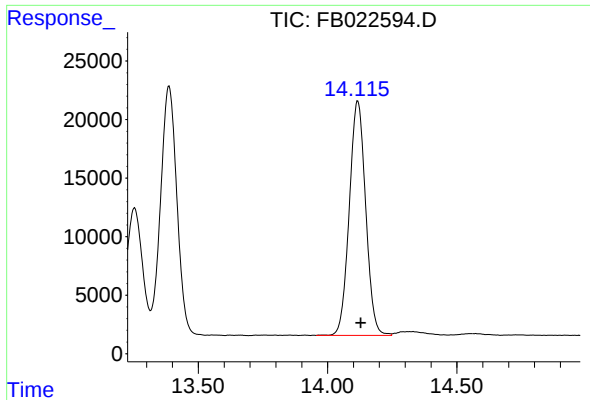

#9 O-Xylene


R.T.: 14.117 min

Delta R.T.: -0.011 min

Response: 881337

Conc: 36.33 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0926S1

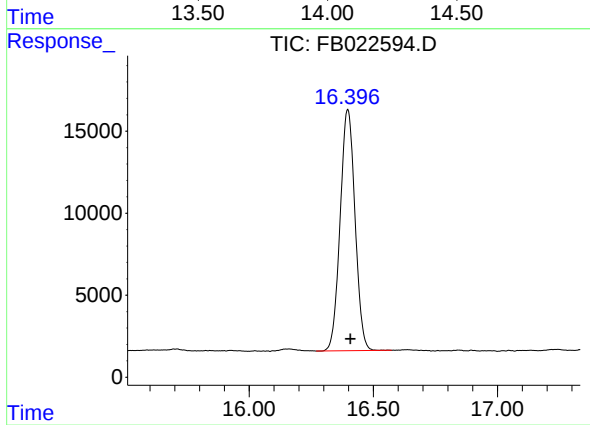

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min

Delta R.T.: -0.010 min

Response: 612873

Conc: 23.51 ng/ml