

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092619\
Data File : FB022598.D
Signal(s) : FID2B.CH
Acq On : 26 Sep 2019 11:34
Operator : DD/AJ
Sample : K5020-01
Misc : 4.98g/5.00ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RT-3860

Integration File: Calibration.e
Quant Time: Sep 27 01:41:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.969	543112	18.672 ng/ml
Target Compounds			
6) t Toluene	10.818	4078	0.086 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092619\
Data File : FB022598.D
Signal(s) : FID2B.CH
Acq On : 26 Sep 2019 11:34
Operator : DD/AJ
Sample : K5020-01
Misc : 4.98g/5.00ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RT-3860

Integration File: Calibration.e
Quant Time: Sep 27 01:41:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

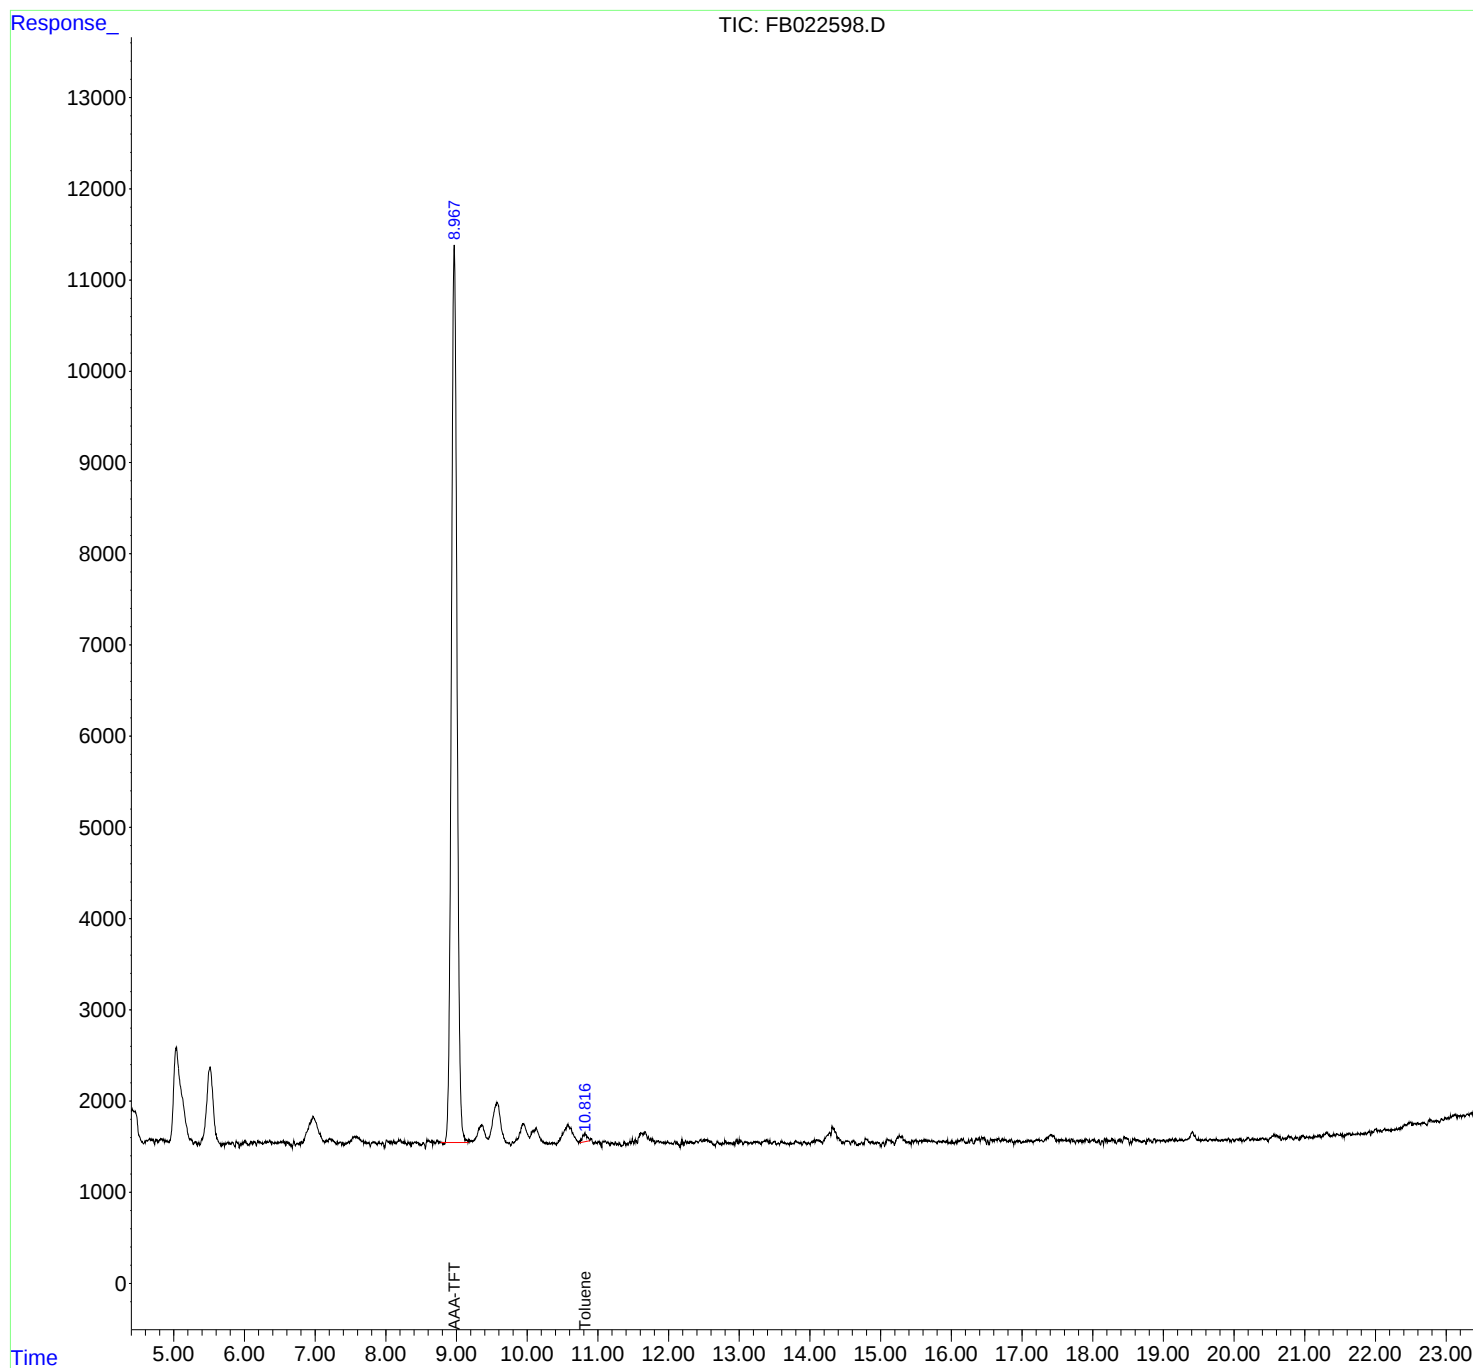


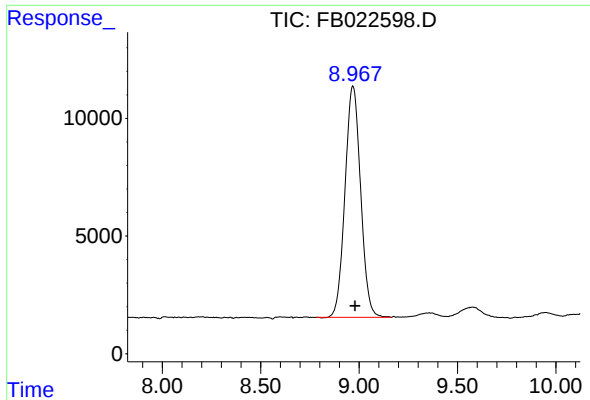

#5 AAA-TFT

R.T.: 8.969 min
Delta R.T.: -0.011 min
Response: 543112
Conc: 18.67 ng/ml

Instrument :
FID_B
ClientSampleId :
RT-3860

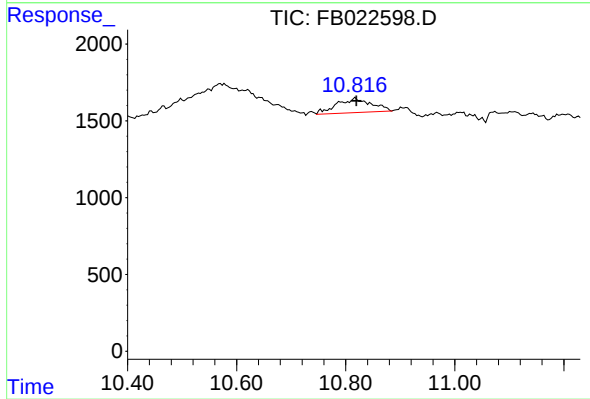

#6 Toluene

R.T.: 10.818 min
Delta R.T.: -0.002 min
Response: 4078
Conc: 0.09 ng/ml