

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092719\
Data File : FB022622.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2019 11:43
Operator : DD/AJ
Sample : K5067-04
Misc : 5.05g/5.00ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 27 23:07:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.966	440526	15.145 ng/ml
Target Compounds			
6) t Toluene	10.809	5524	0.116 ng/ml
7) t Ethylbenzene	13.229	95480	3.185 ng/ml
9) t O-Xylene	14.138	24914	1.027 ng/ml
10) t 1,2,4-Trimethylbenzene	16.433	16486	0.632 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092719\
Data File : FB022622.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2019 11:43
Operator : DD/AJ
Sample : K5067-04
Misc : 5.05g/5.00ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 27 23:07:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

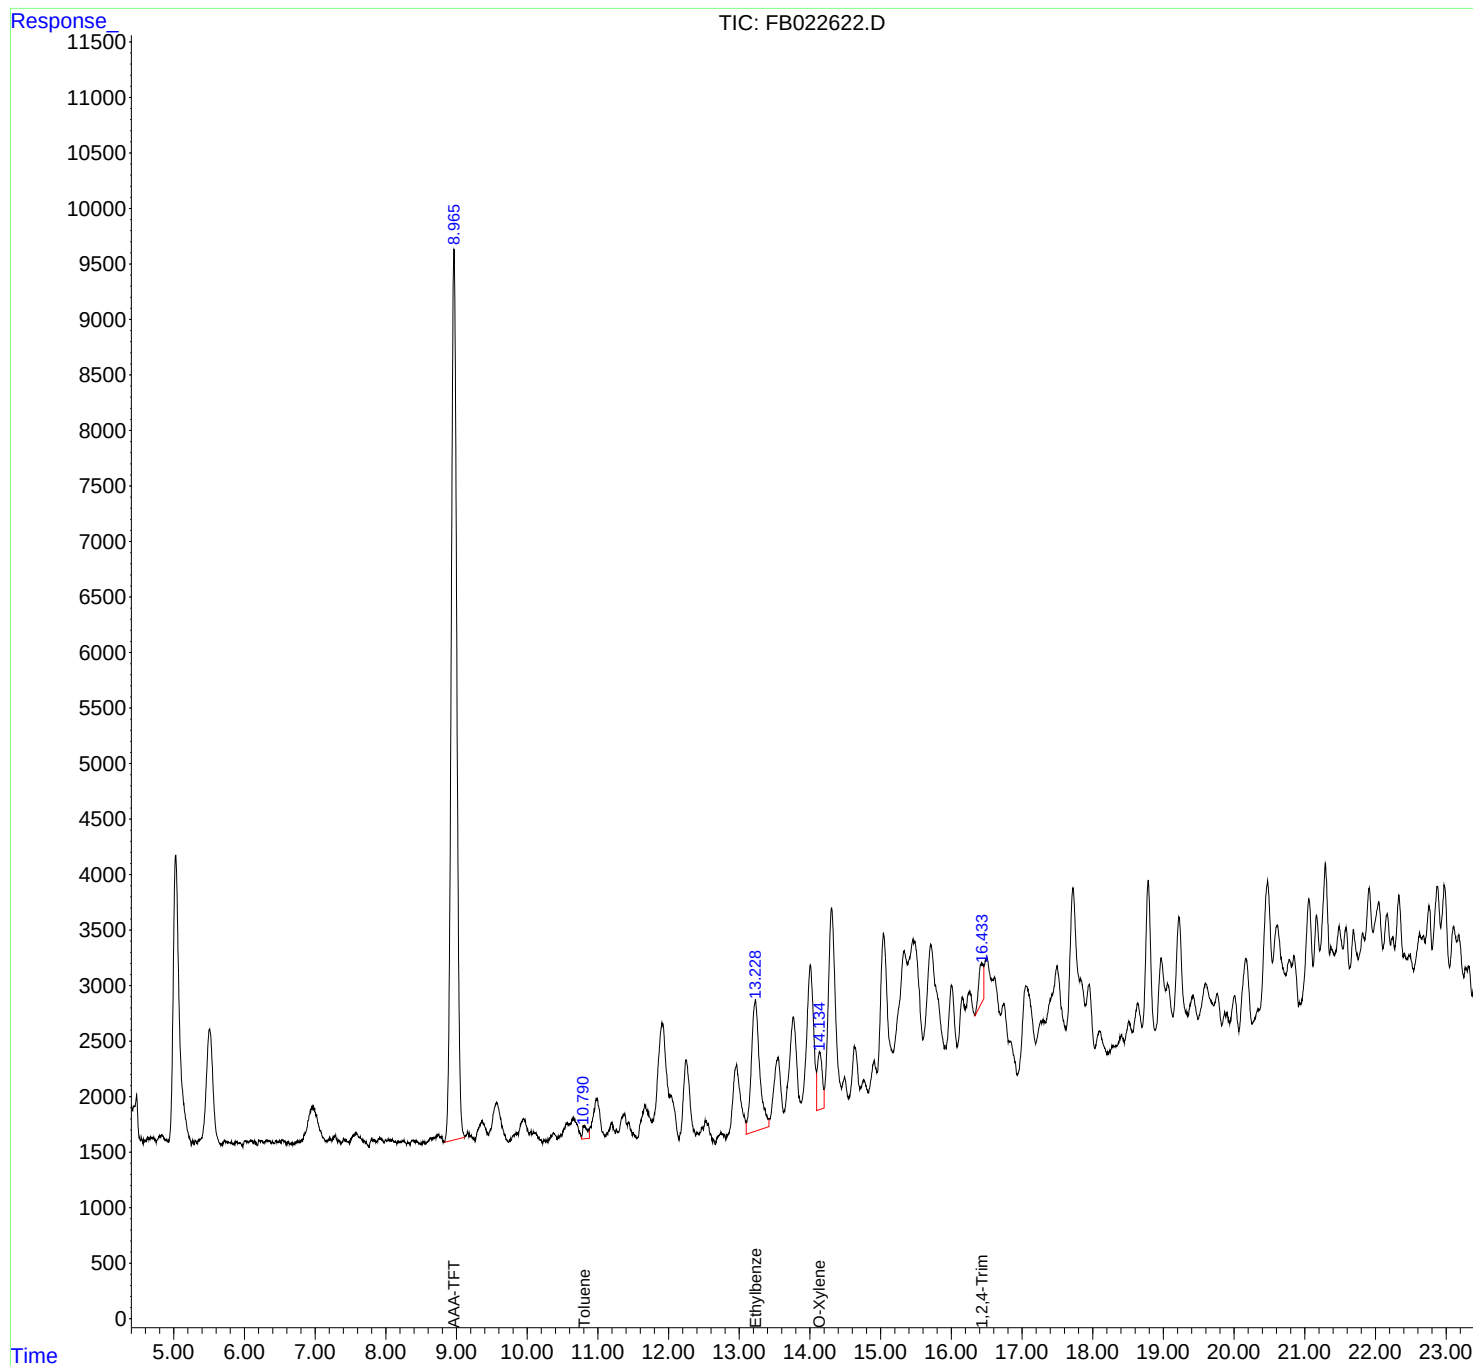


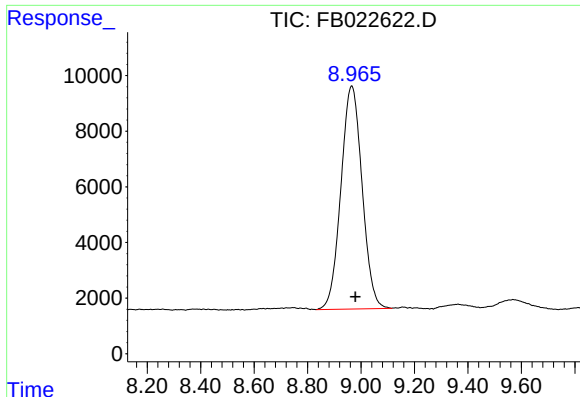

#5 AAA-TFT


R.T.: 8.966 min
Delta R.T.: -0.013 min
Response: 440526
Conc: 15.14 ng/ml

Instrument :
FID_B
ClientSampleId :

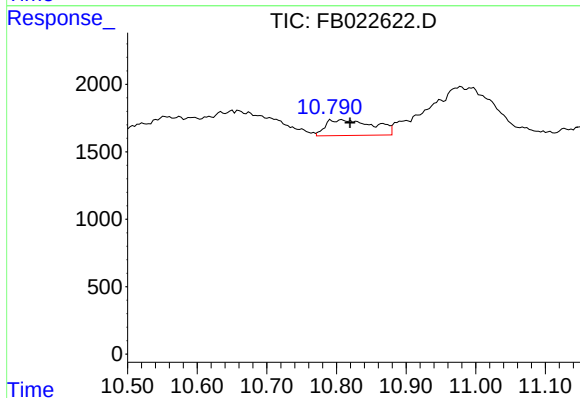


#6 Toluene

R.T.: 10.809 min
Delta R.T.: -0.011 min
Response: 5524
Conc: 0.12 ng/ml

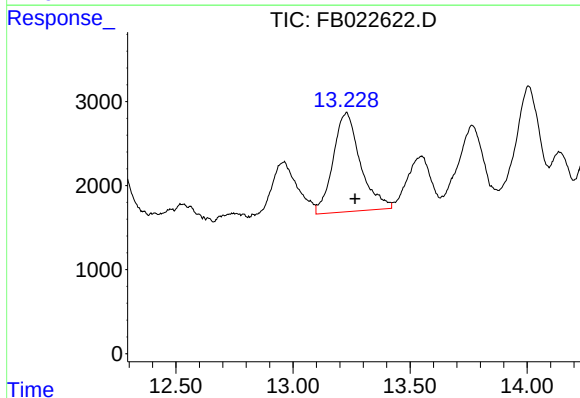


#7 Ethylbenzene

R.T.: 13.229 min
Delta R.T.: -0.036 min
Response: 95480
Conc: 3.18 ng/ml

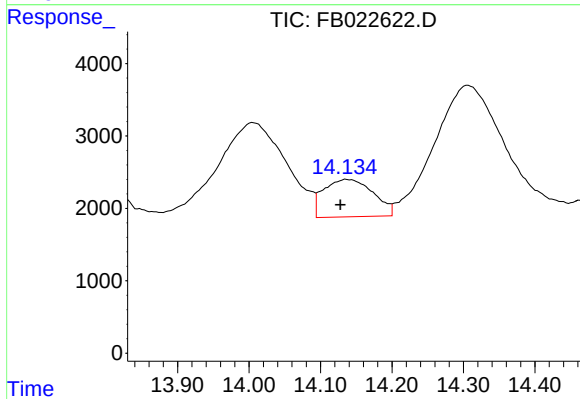

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: 0.010 min
Response: 24914
Conc: 1.03 ng/ml

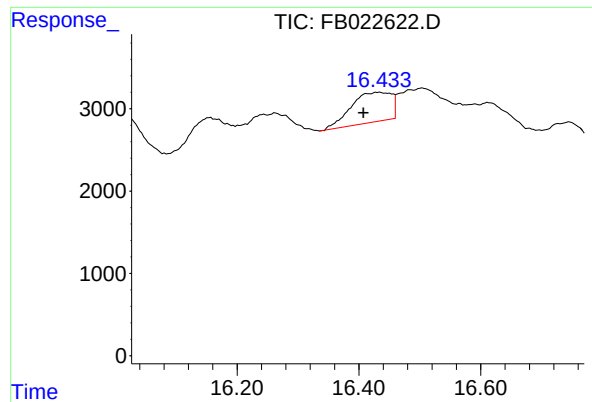

#10 1,2,4-Trimethylbenzene

R.T.: 16.433 min
Delta R.T.: 0.026 min
Response: 16486
Conc: 0.63 ng/ml

Instrument :
FID_B
ClientSampleId :