

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092719\
 Data File : FB022624.D
 Signal(s) : FID2B.CH
 Acq On : 27 Sep 2019 12:43
 Operator : DD/AJ
 Sample : K5064-01MSD
 Misc : 5.03g/5.00ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 27 23:07:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.965	569565	19.581 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.832	1042484	21.218 ng/ml
2) t 2,2,4-Trimethylpentane	7.583	1212144	23.474 ng/ml
3) t n-Heptane	7.924	382395	7.598 ng/ml
4) t Benzene	8.058	481990	8.121 ng/ml
6) t Toluene	10.807	1398243	29.391 ng/ml
7) t Ethylbenzene	13.253	448794	14.970 ng/ml
8) t m-Xylene	13.386	877042	33.013 ng/ml
9) t O-Xylene	14.116	834066	34.380 ng/ml
10) t 1,2,4-Trimethylbenzene	16.396	571167	21.908 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092719\
Data File : FB022624.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2019 12:43
Operator : DD/AJ
Sample : K5064-01MSD
Misc : 5.03g/5.00ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 27 23:07:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

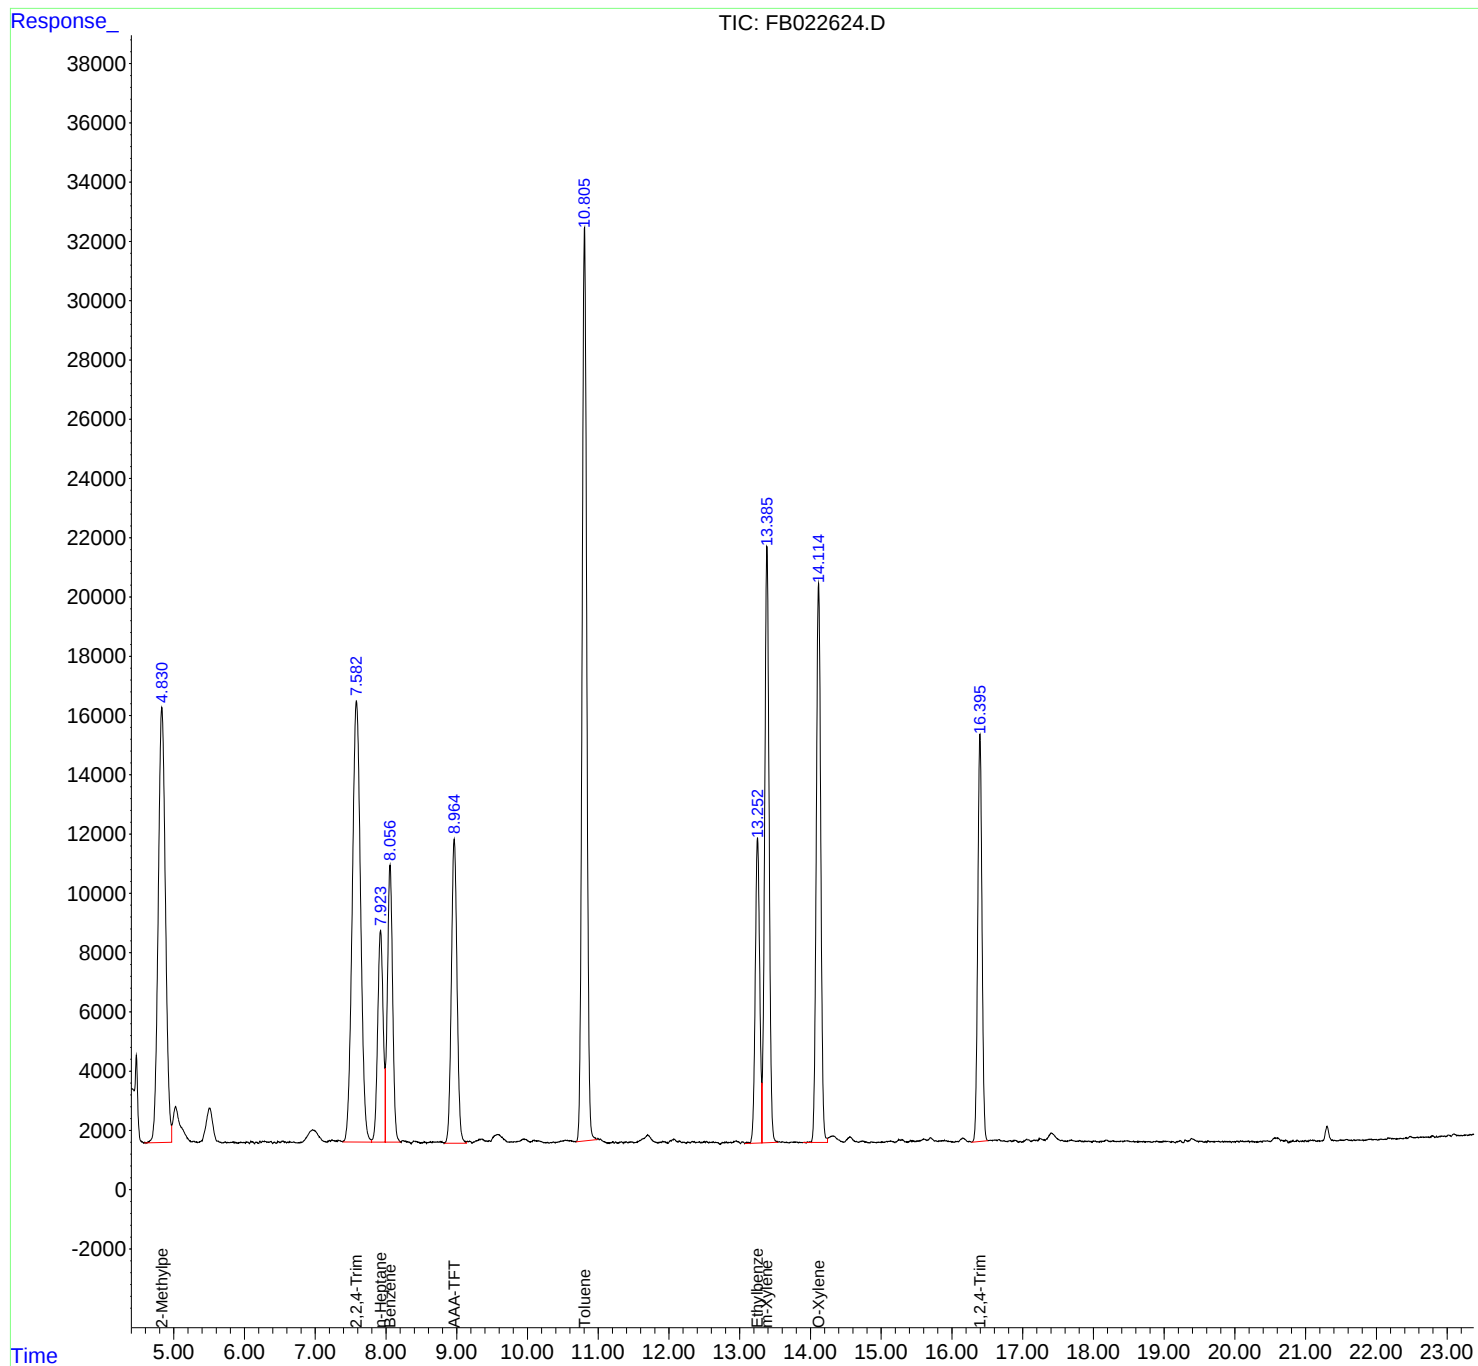


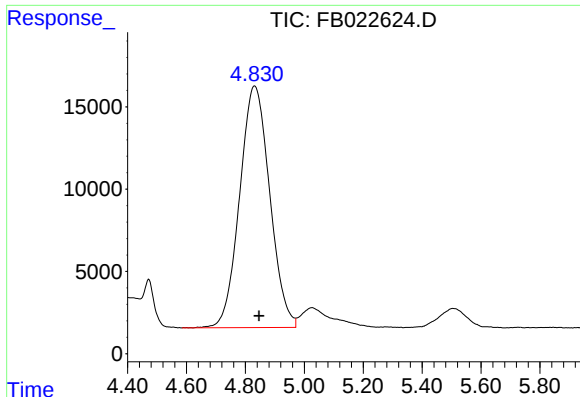

#1 2-Methylpentane


R.T.: 4.832 min
Delta R.T.: -0.015 min
Response: 1042484
Conc: 21.22 ng/ml

Instrument :
FID_B
ClientSampleId :

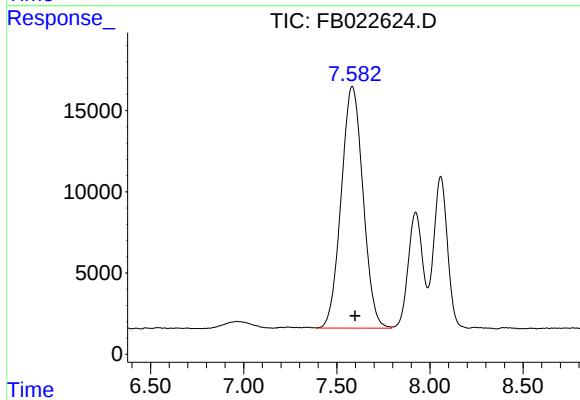


#2 2,2,4-Trimethylpentane

R.T.: 7.583 min
Delta R.T.: -0.015 min
Response: 1212144
Conc: 23.47 ng/ml

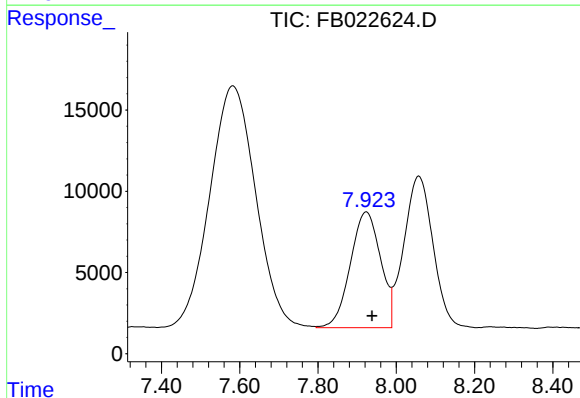


#3 n-Heptane

R.T.: 7.924 min
Delta R.T.: -0.014 min
Response: 382395
Conc: 7.60 ng/ml

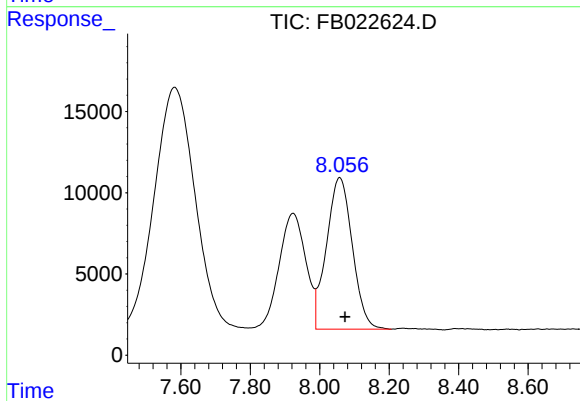

#4 Benzene


R.T.: 8.058 min
Delta R.T.: -0.014 min
Response: 481990
Conc: 8.12 ng/ml

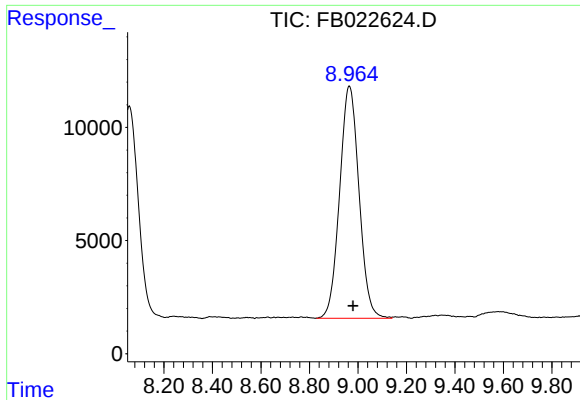

#5 AAA-TFT


R.T.: 8.965 min
Delta R.T.: -0.014 min
Response: 569565
Conc: 19.58 ng/ml

Instrument :
FID_B
ClientSampleId :

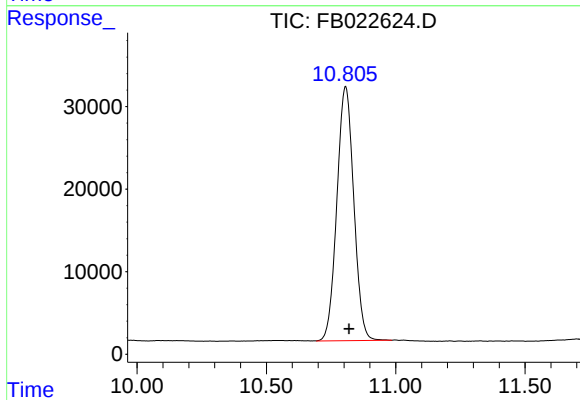


#6 Toluene

R.T.: 10.807 min
Delta R.T.: -0.013 min
Response: 1398243
Conc: 29.39 ng/ml

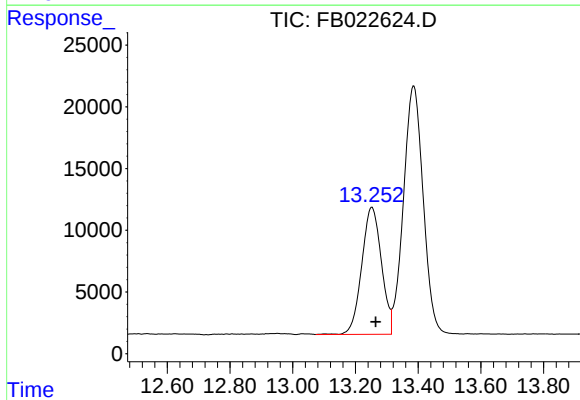


#7 Ethylbenzene

R.T.: 13.253 min
Delta R.T.: -0.013 min
Response: 448794
Conc: 14.97 ng/ml

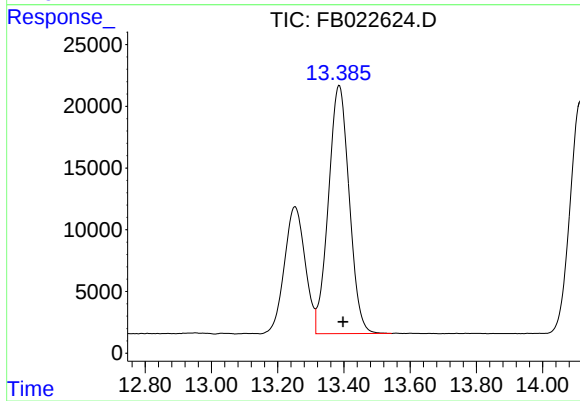

#8 m-Xylene


R.T.: 13.386 min
Delta R.T.: -0.012 min
Response: 877042
Conc: 33.01 ng/ml

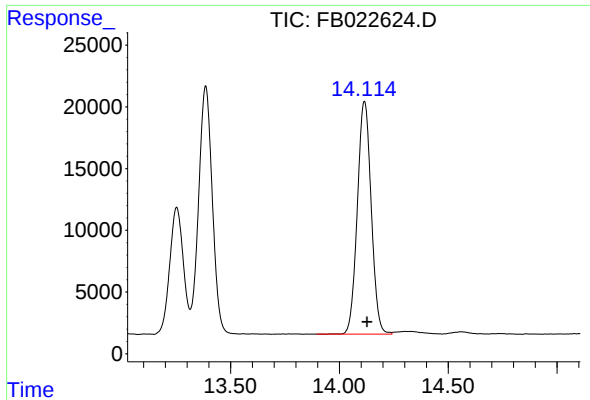

#9 O-Xylene

R.T.: 14.116 min
Delta R.T.: -0.012 min
Response: 834066
Conc: 34.38 ng/ml

Instrument :
FID_B
ClientSampleId :

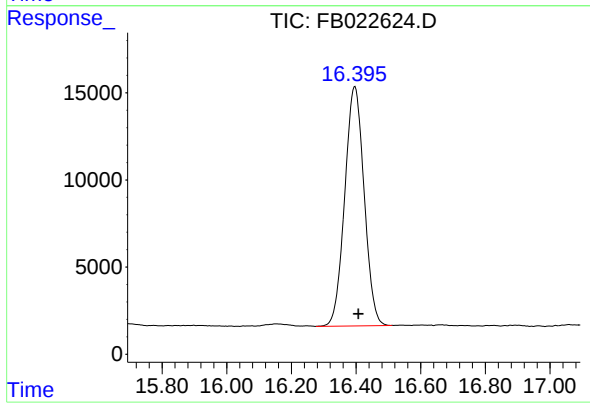

#10 1,2,4-Trimethylbenzene

R.T.: 16.396 min
Delta R.T.: -0.011 min
Response: 571167
Conc: 21.91 ng/ml