

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092719\
 Data File : FB022631.D
 Signal(s) : FID2B.CH
 Acq On : 27 Sep 2019 16:10
 Operator : DD/AJ
 Sample : K5019-03 20X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 27 23:08:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.966	551909	18.974 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.850	3689	0.075 ng/ml
2) t 2,2,4-Trimethylpentane	7.537	23172	0.449 ng/ml
4) t Benzene	8.059	8943618	150.694 ng/ml
6) t Toluene	10.807	1500475	31.540 ng/ml
7) t Ethylbenzene	13.253	2134550	71.201 ng/ml
8) t m-Xylene	13.382	3135599	118.029 ng/ml
9) t O-Xylene	14.116	2188679	90.218 ng/ml
10) t 1,2,4-Trimethylbenzene	16.396	536221	20.567 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092719\
Data File : FB022631.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2019 16:10
Operator : DD/AJ
Sample : K5019-03 20X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 27 23:08:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

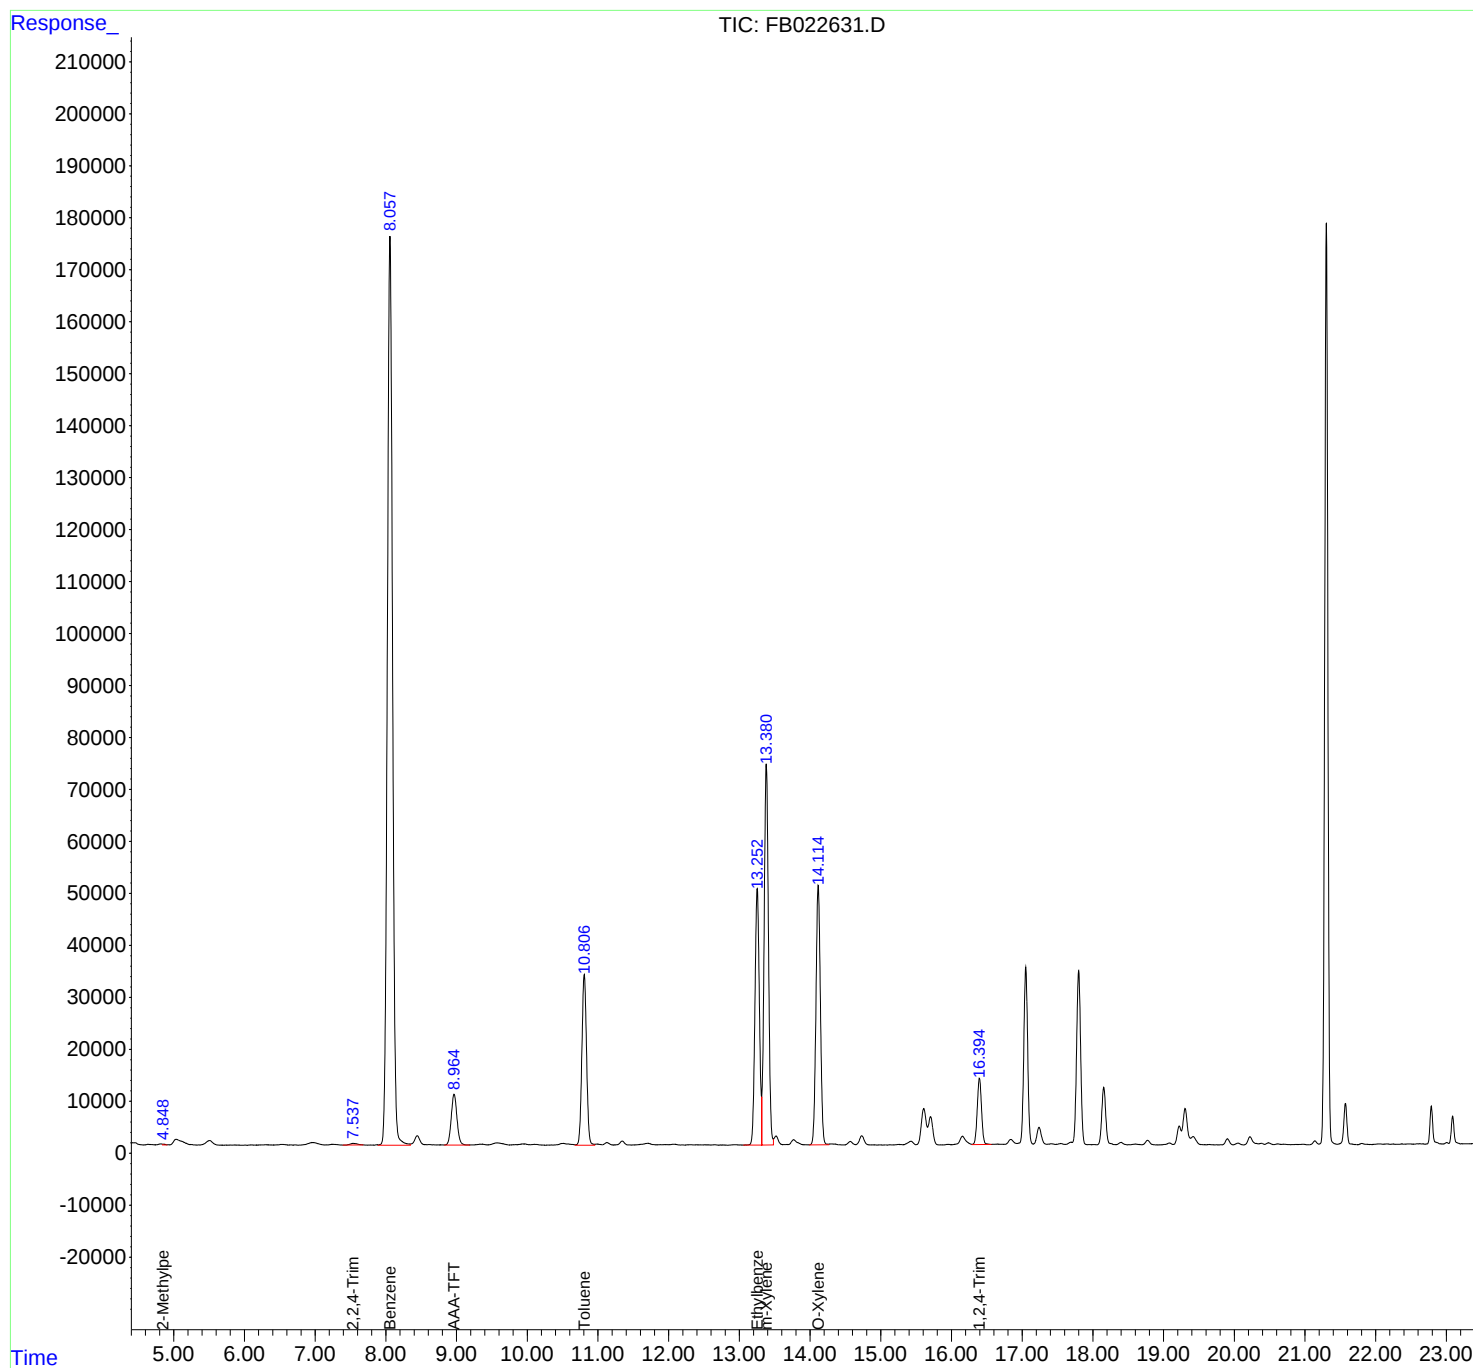


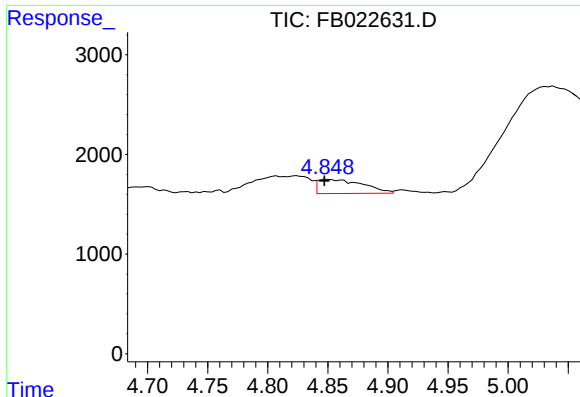

#1 2-Methylpentane


R.T.: 4.850 min
Delta R.T.: 0.003 min
Response: 3689
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :

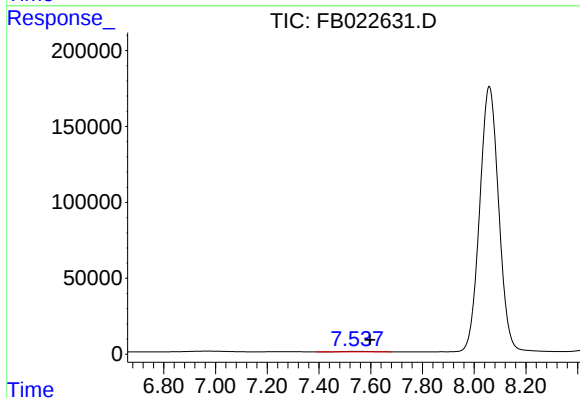


#2 2,2,4-Trimethylpentane

R.T.: 7.537 min
Delta R.T.: -0.060 min
Response: 23172
Conc: 0.45 ng/ml

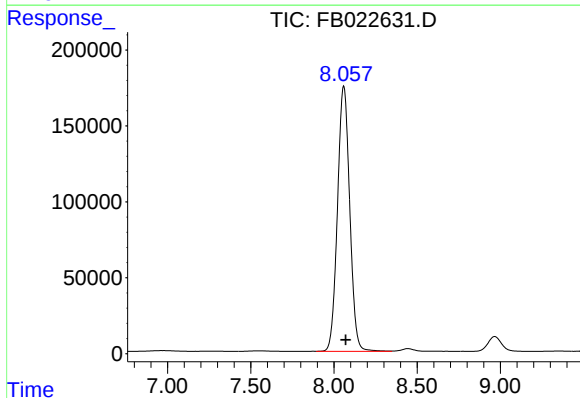


#4 Benzene

R.T.: 8.059 min
Delta R.T.: -0.014 min
Response: 8943618
Conc: 150.69 ng/ml

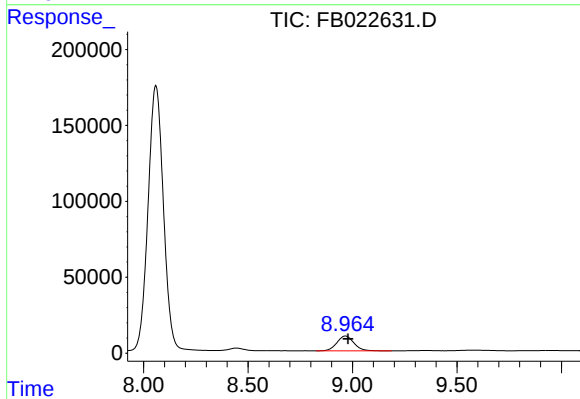

#5 AAA-TFT


R.T.: 8.966 min
Delta R.T.: -0.013 min
Response: 551909
Conc: 18.97 ng/ml

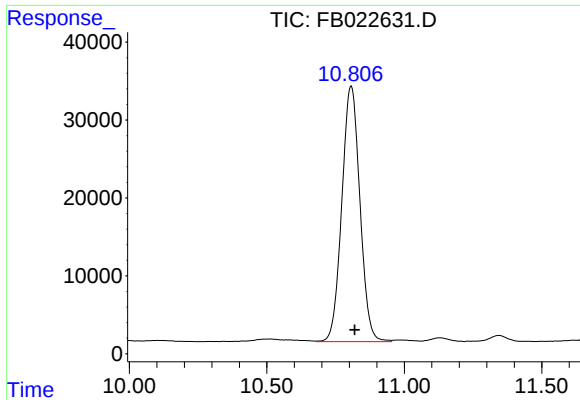

#6 Toluene


R.T.: 10.807 min
Delta R.T.: -0.013 min
Response: 1500475
Conc: 31.54 ng/ml

Instrument :
FID_B
ClientSampleId :

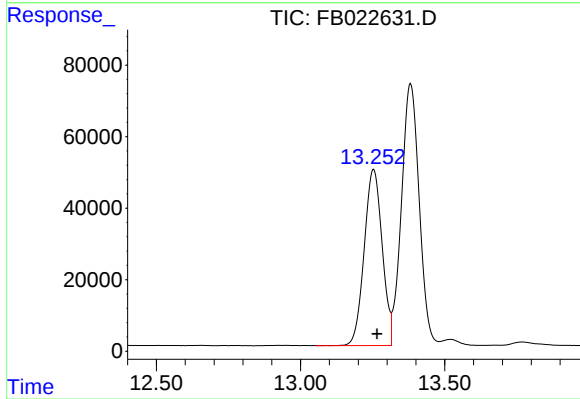


#7 Ethylbenzene

R.T.: 13.253 min
Delta R.T.: -0.012 min
Response: 2134550
Conc: 71.20 ng/ml

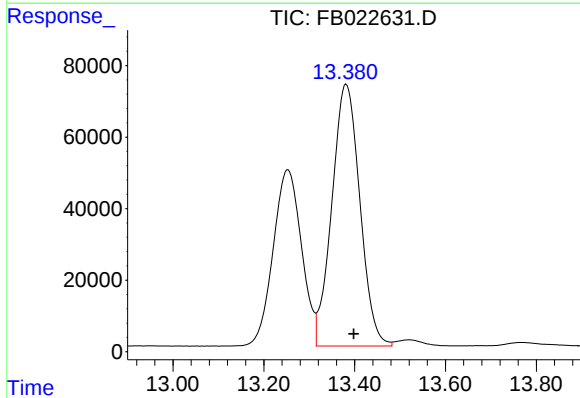


#8 m-Xylene

R.T.: 13.382 min
Delta R.T.: -0.016 min
Response: 3135599
Conc: 118.03 ng/ml

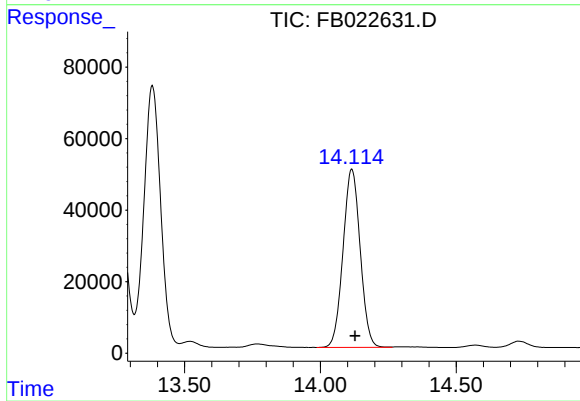

#9 O-Xylene

R.T.: 14.116 min
Delta R.T.: -0.012 min
Response: 2188679
Conc: 90.22 ng/ml

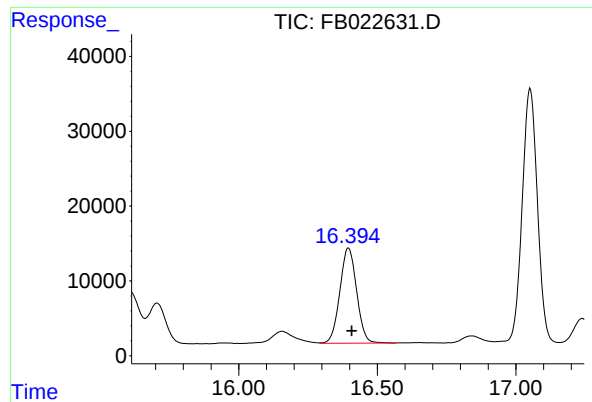

#10 1,2,4-Trimethylbenzene

R.T.: 16.396 min
Delta R.T.: -0.011 min
Response: 536221
Conc: 20.57 ng/ml

Instrument :
FID_B
ClientSampleId :