

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092719\
 Data File : FB022616.D
 Signal(s) : FID2B.CH
 Acq On : 27 Sep 2019 8:45
 Operator : DD/AJ
 Sample : BSF0927S1
 Misc : 5.02g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0927S1

Integration File: autoint1.e
 Quant Time: Sep 27 23:06:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.963	565196	19.431 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.831	1002209	20.398 ng/ml
2) t 2,2,4-Trimethylpentane	7.581	1169971	22.657 ng/ml
3) t n-Heptane	7.922	380695	7.564 ng/ml
4) t Benzene	8.056	474939	8.002 ng/ml
6) t Toluene	10.805	1414043	29.724 ng/ml
7) t Ethylbenzene	13.251	455774	15.203 ng/ml
8) t m-Xylene	13.384	907520	34.161 ng/ml
9) t O-Xylene	14.114	857620	35.351 ng/ml
10) t 1,2,4-Trimethylbenzene	16.395	591359	22.682 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092719\
Data File : FB022616.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2019 8:45
Operator : DD/AJ
Sample : BSF0927S1
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0927S1

Integration File: autoint1.e
Quant Time: Sep 27 23:06:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

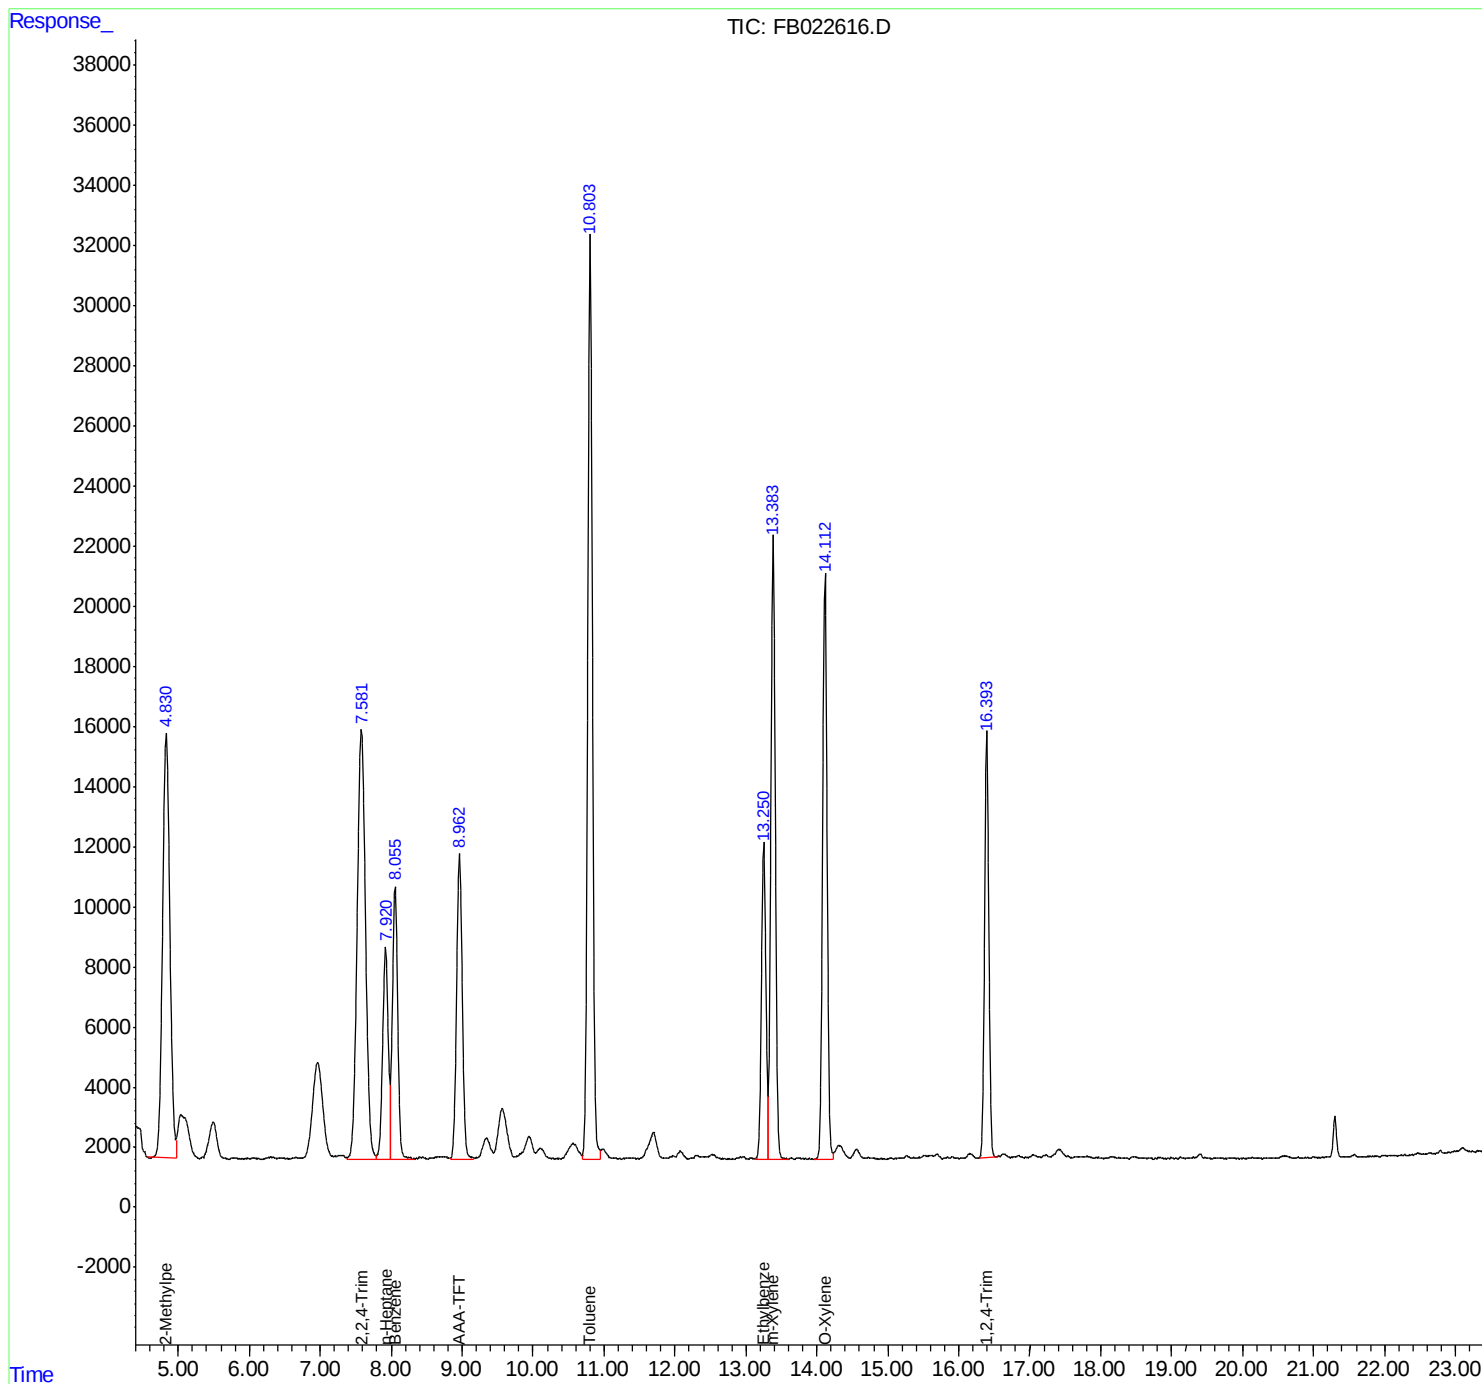


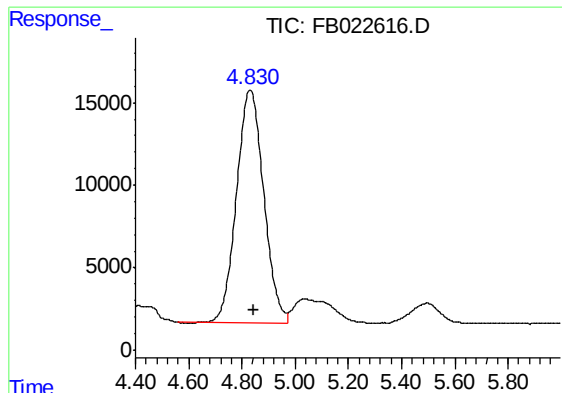

#1 2-Methylpentane


R.T.: 4.831 min
Delta R.T.: -0.016 min
Response: 1002209
Conc: 20.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0927S1

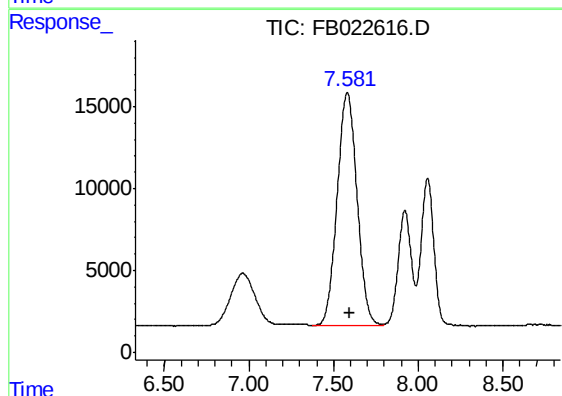


#2 2,2,4-Trimethylpentane

R.T.: 7.581 min
Delta R.T.: -0.016 min
Response: 1169971
Conc: 22.66 ng/ml

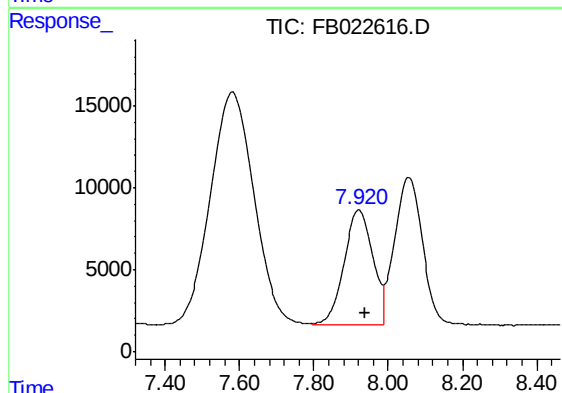


#3 n-Heptane

R.T.: 7.922 min
Delta R.T.: -0.016 min
Response: 380695
Conc: 7.56 ng/ml

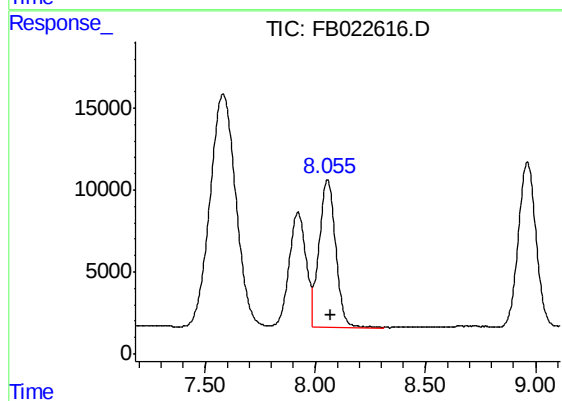

#4 Benzene


R.T.: 8.056 min
Delta R.T.: -0.017 min
Response: 474939
Conc: 8.00 ng/ml

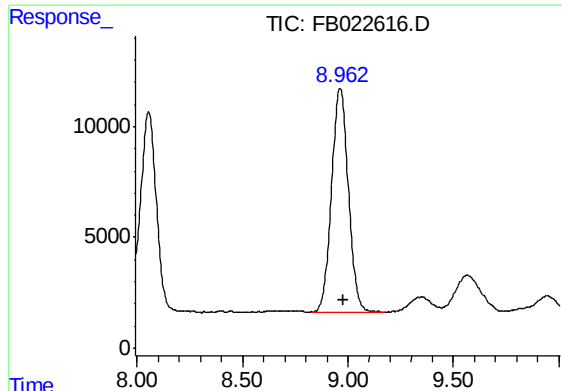

#5 AAA-TFT


R.T.: 8.963 min
Delta R.T.: -0.016 min
Response: 565196
Conc: 19.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0927S1

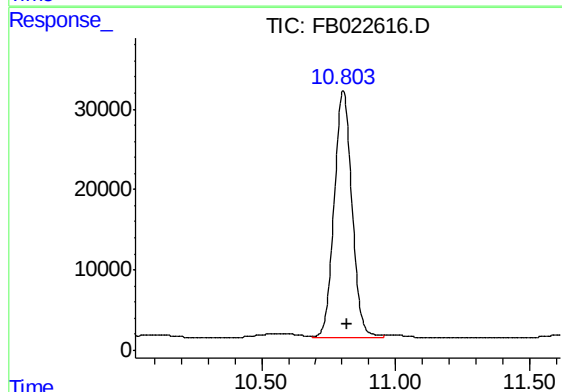


#6 Toluene

R.T.: 10.805 min
Delta R.T.: -0.015 min
Response: 1414043
Conc: 29.72 ng/ml

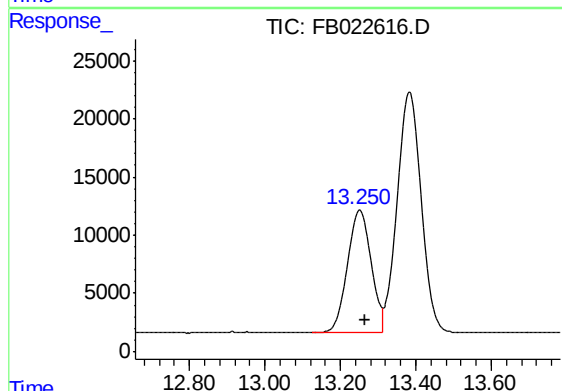


#7 Ethylbenzene

R.T.: 13.251 min
Delta R.T.: -0.014 min
Response: 455774
Conc: 15.20 ng/ml

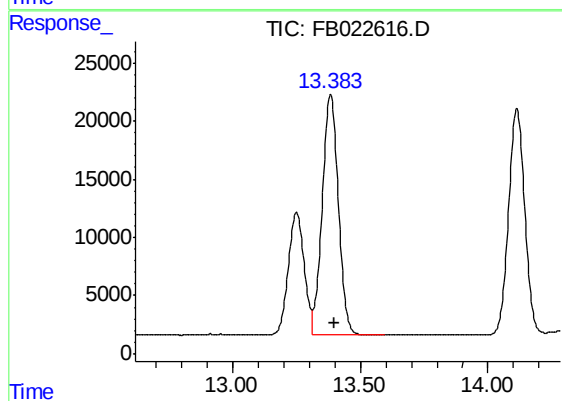

#8 m-Xylene


R.T.: 13.384 min
Delta R.T.: -0.014 min
Response: 907520
Conc: 34.16 ng/ml

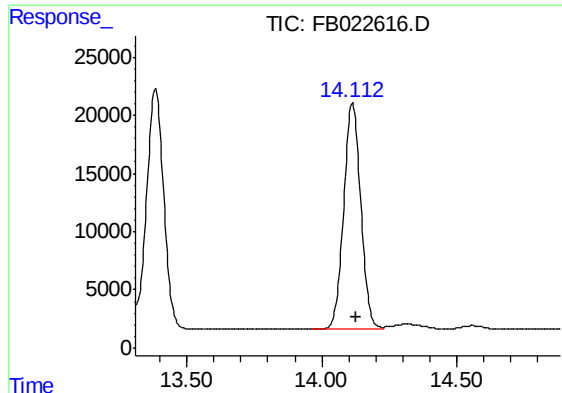

#9 O-Xylene

R.T.: 14.114 min
Delta R.T.: -0.014 min
Response: 857620
Conc: 35.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0927S1

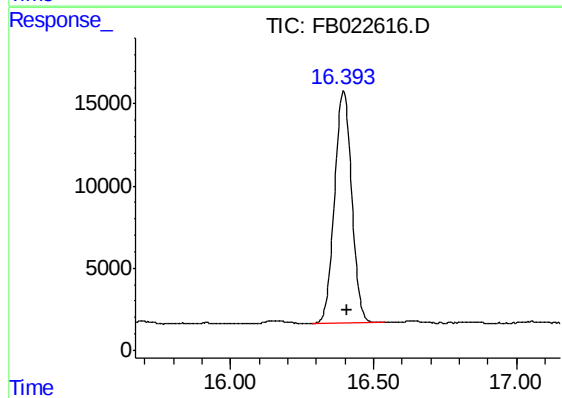

#10 1,2,4-Trimethylbenzene

R.T.: 16.395 min
Delta R.T.: -0.013 min
Response: 591359
Conc: 22.68 ng/ml