

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092722\
 Data File : FB028456.D
 Signal(s) : FID2B.CH
 Acq On : 27 Sep 2022 11:24
 Operator : AJ/MA
 Sample : BSF0927S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0927S1

Integration File: Calibration.e
 Quant Time: Sep 28 03:32:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	241495	20.177 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	587620	29.023 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	628713	29.887 ng/ml
3) t n-Heptane	7.753	203377	9.461 ng/ml
4) t Benzene	7.890	243794	9.910 ng/ml
6) t Toluene	10.623	701760	30.142 ng/ml
7) t Ethylbenzene	13.060	219455	9.868 ng/ml
8) t m-Xylene	13.193	434563	19.913 ng/ml
9) t O-Xylene	13.920	423643	20.220 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	408727	20.327 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092722\
Data File : FB028456.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2022 11:24
Operator : AJ/MA
Sample : BSF0927S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0927S1

Integration File: Calibration.e
Quant Time: Sep 28 03:32:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

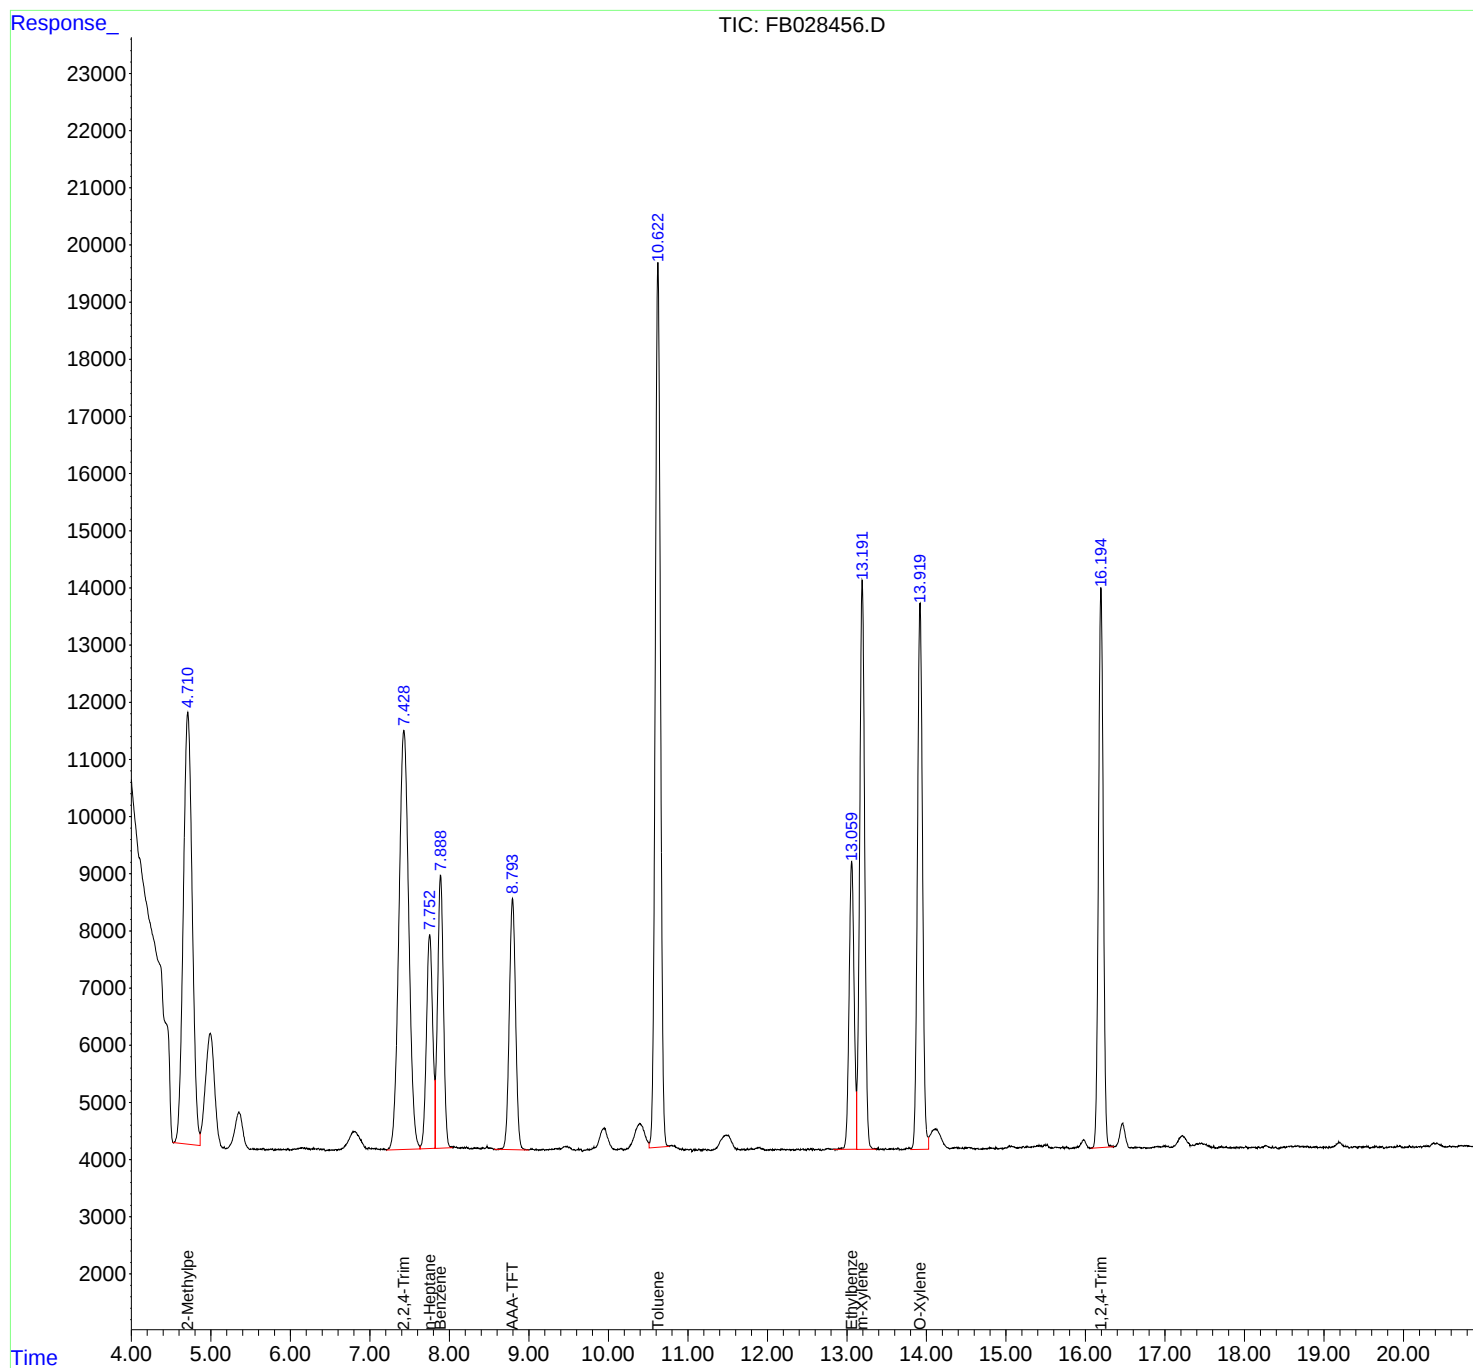


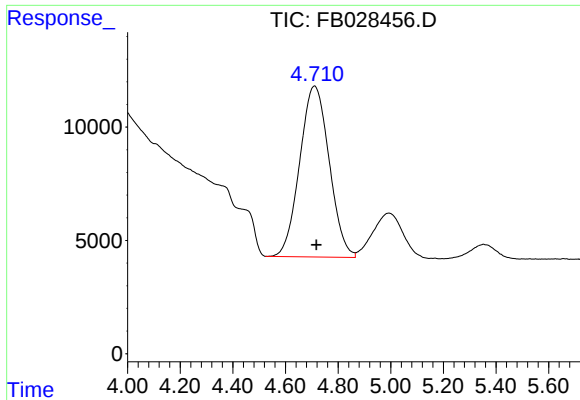

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: -0.006 min
Response: 587620
Conc: 29.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0927S1

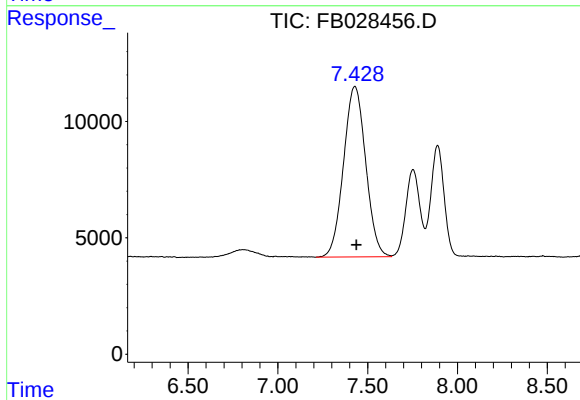


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: -0.008 min
Response: 628713
Conc: 29.89 ng/ml

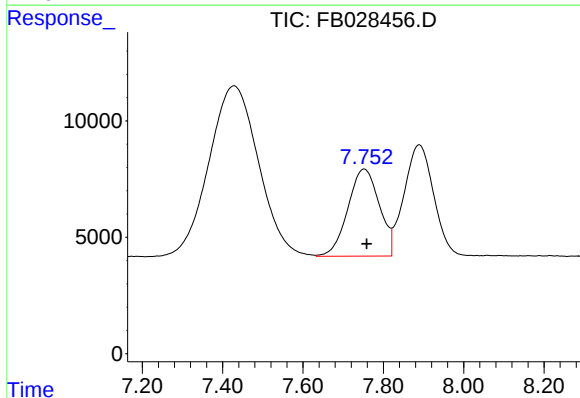


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 203377
Conc: 9.46 ng/ml

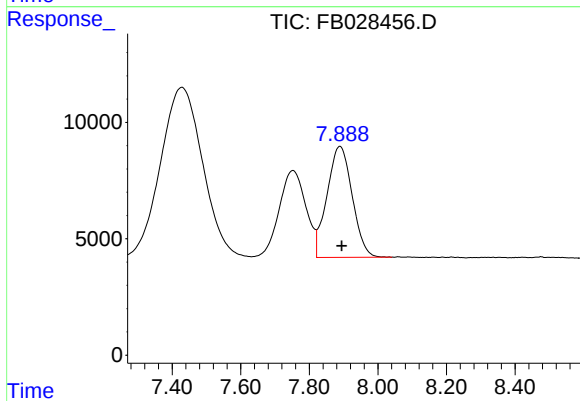

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.005 min
Response: 243794
Conc: 9.91 ng/ml

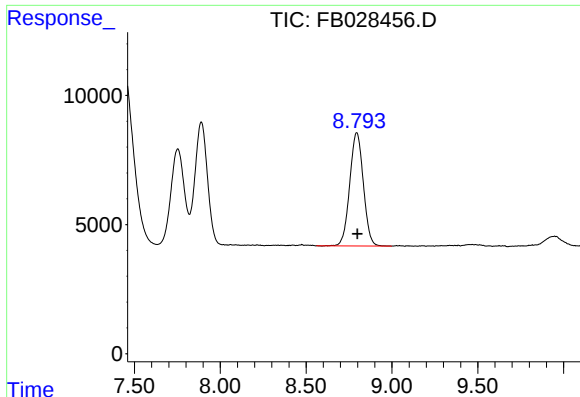

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 241495
Conc: 20.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0927S1

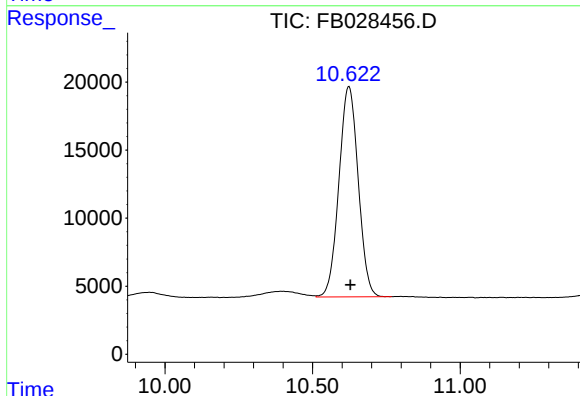


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.005 min
Response: 701760
Conc: 30.14 ng/ml

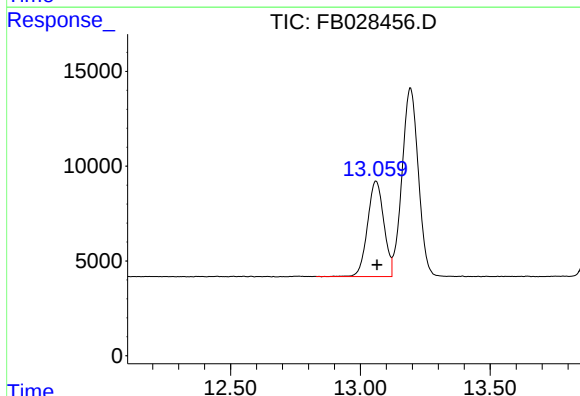


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.004 min
Response: 219455
Conc: 9.87 ng/ml

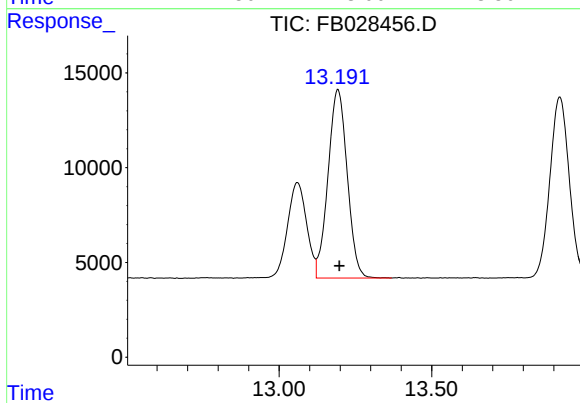

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.004 min
Response: 434563
Conc: 19.91 ng/ml

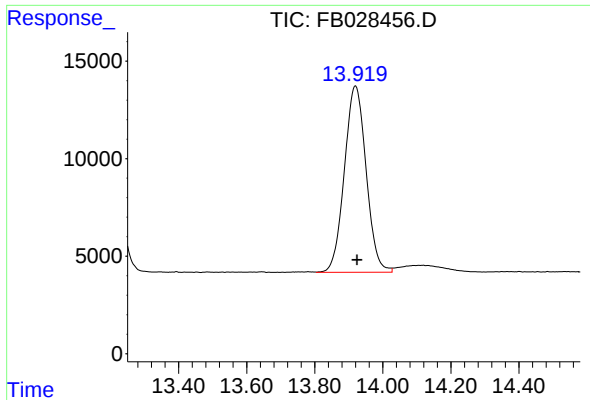

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 423643
Conc: 20.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0927S1

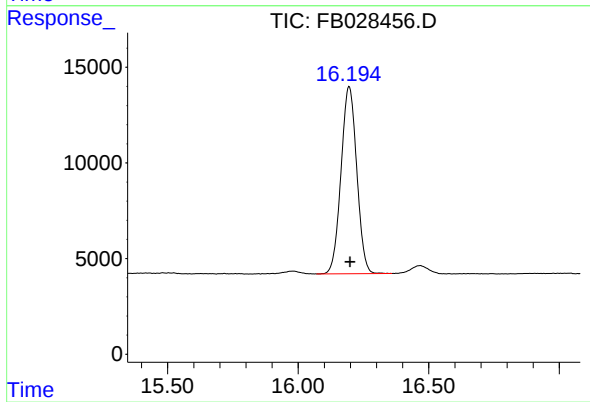

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.004 min
Response: 408727
Conc: 20.33 ng/ml