

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092722\
 Data File : FB028458.D
 Signal(s) : FID2B.CH
 Acq On : 27 Sep 2022 12:43
 Operator : AJ/MA
 Sample : N4782-01MS 50X
 Misc : 5.03G/5.00 ML MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-T-1-(0-6)MS

Integration File: Calibration.e
 Quant Time: Sep 28 03:33:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	243255	20.324 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.700	472906	23.357 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	590453	28.069 ng/ml
3) t n-Heptane	7.749	202349	9.413 ng/ml
4) t Benzene	7.888	286427	11.643 ng/ml
6) t Toluene	10.624	755033	32.431 ng/ml
7) t Ethylbenzene	13.061	225553	10.142 ng/ml
8) t m-Xylene	13.194	445654	20.422 ng/ml
9) t O-Xylene	13.921	440138	21.007 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	381177	18.957 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092722\
Data File : FB028458.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2022 12:43
Operator : AJ/MA
Sample : N4782-01MS 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(0-6)MS

Integration File: Calibration.e
Quant Time: Sep 28 03:33:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

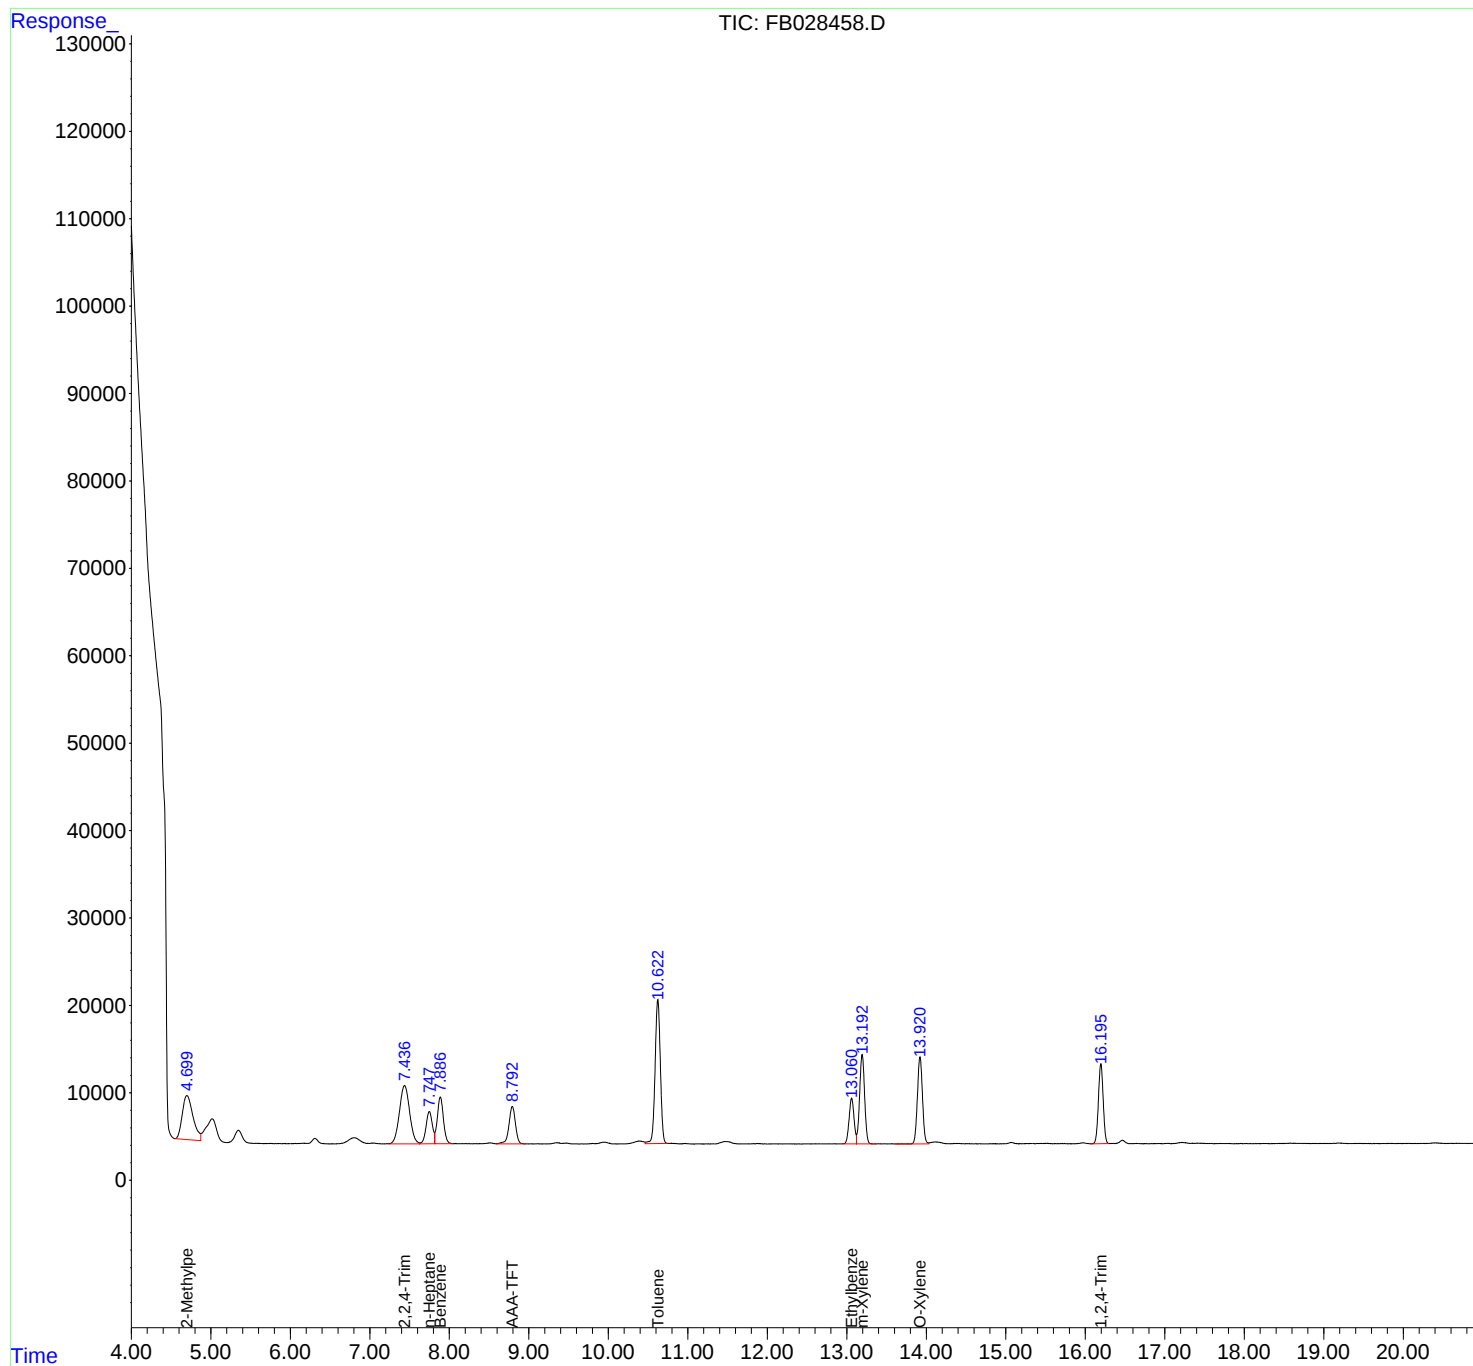


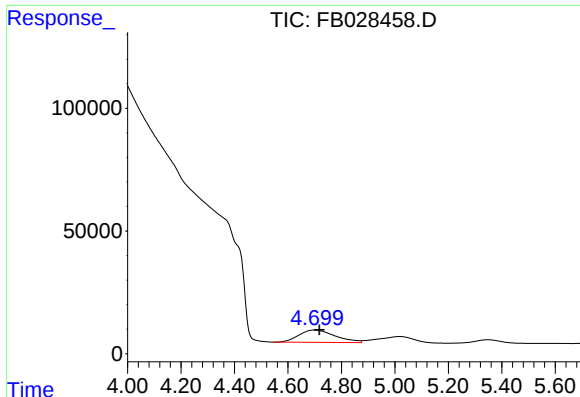

#1 2-Methylpentane


R.T.: 4.700 min
Delta R.T.: -0.018 min
Response: 472906
Conc: 23.36 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(0-6)MS

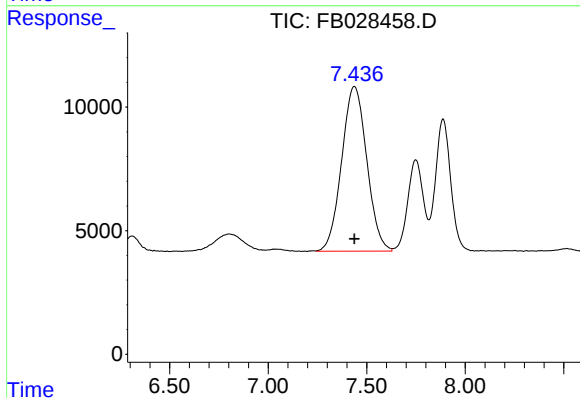


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.000 min
Response: 590453
Conc: 28.07 ng/ml

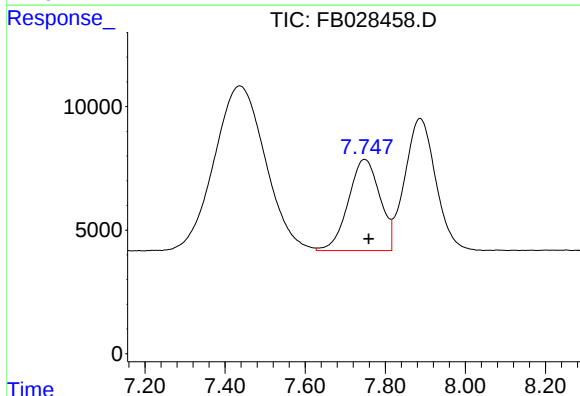


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.009 min
Response: 202349
Conc: 9.41 ng/ml

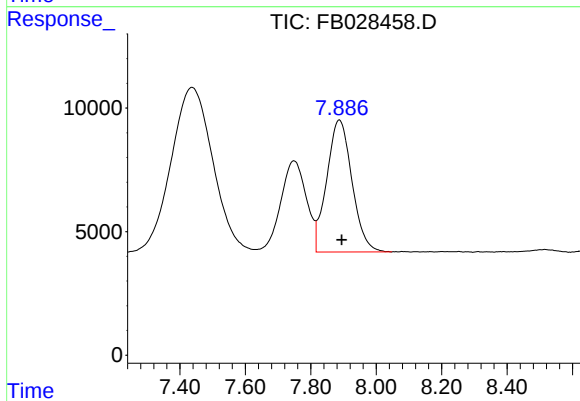

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.007 min
Response: 286427
Conc: 11.64 ng/ml

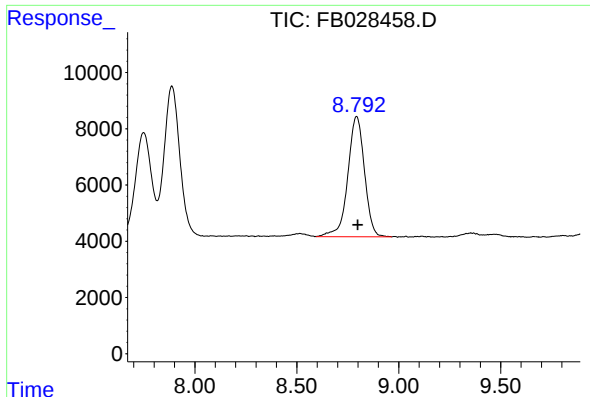

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.007 min
Response: 243255
Conc: 20.32 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(0-6)MS

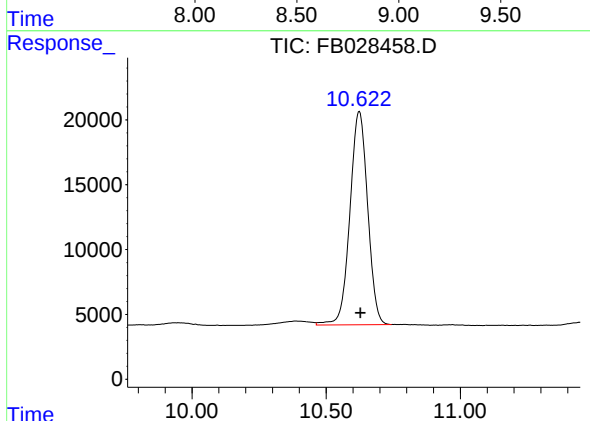


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.004 min
Response: 755033
Conc: 32.43 ng/ml

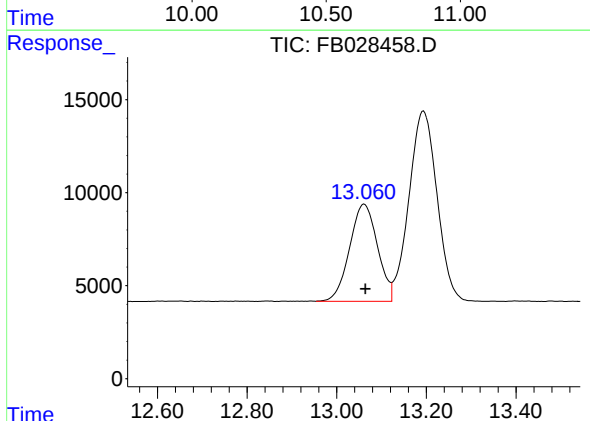


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.003 min
Response: 225553
Conc: 10.14 ng/ml

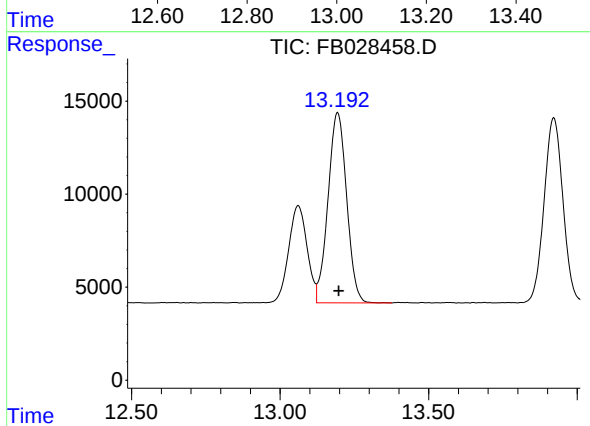

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.003 min
Response: 445654
Conc: 20.42 ng/ml

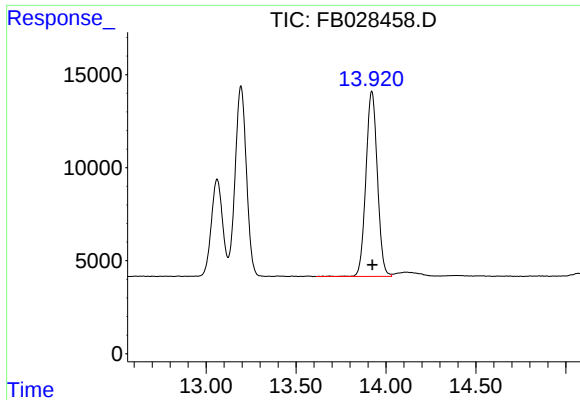

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.003 min
Response: 440138
Conc: 21.01 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(0-6)MS

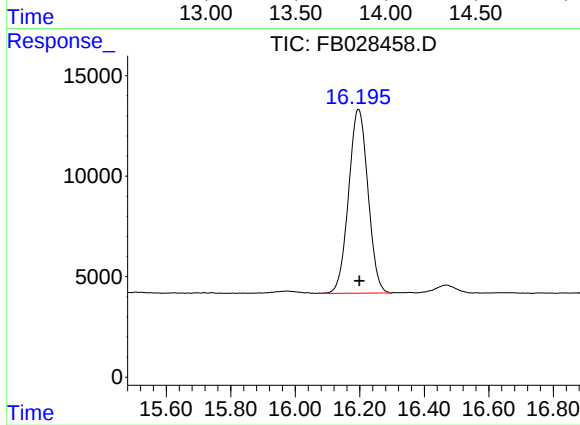

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.002 min
Response: 381177
Conc: 18.96 ng/ml