

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092722\
 Data File : FB028459.D
 Signal(s) : FID2B.CH
 Acq On : 27 Sep 2022 13:22
 Operator : AJ/MA
 Sample : N4782-01MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-T-1-(0-6)MSD

Integration File: Calibration.e
 Quant Time: Sep 28 03:33:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	236453	19.756 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	463058	22.870 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	570344	27.113 ng/ml
3) t n-Heptane	7.752	195655	9.102 ng/ml
4) t Benzene	7.889	266136	10.818 ng/ml
6) t Toluene	10.625	733321	31.498 ng/ml
7) t Ethylbenzene	13.063	223388	10.045 ng/ml
8) t m-Xylene	13.196	435682	19.965 ng/ml
9) t O-Xylene	13.923	419310	20.013 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	358314	17.820 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092722\
Data File : FB028459.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2022 13:22
Operator : AJ/MA
Sample : N4782-01MSD 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(0-6)MSD

Integration File: Calibration.e
Quant Time: Sep 28 03:33:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

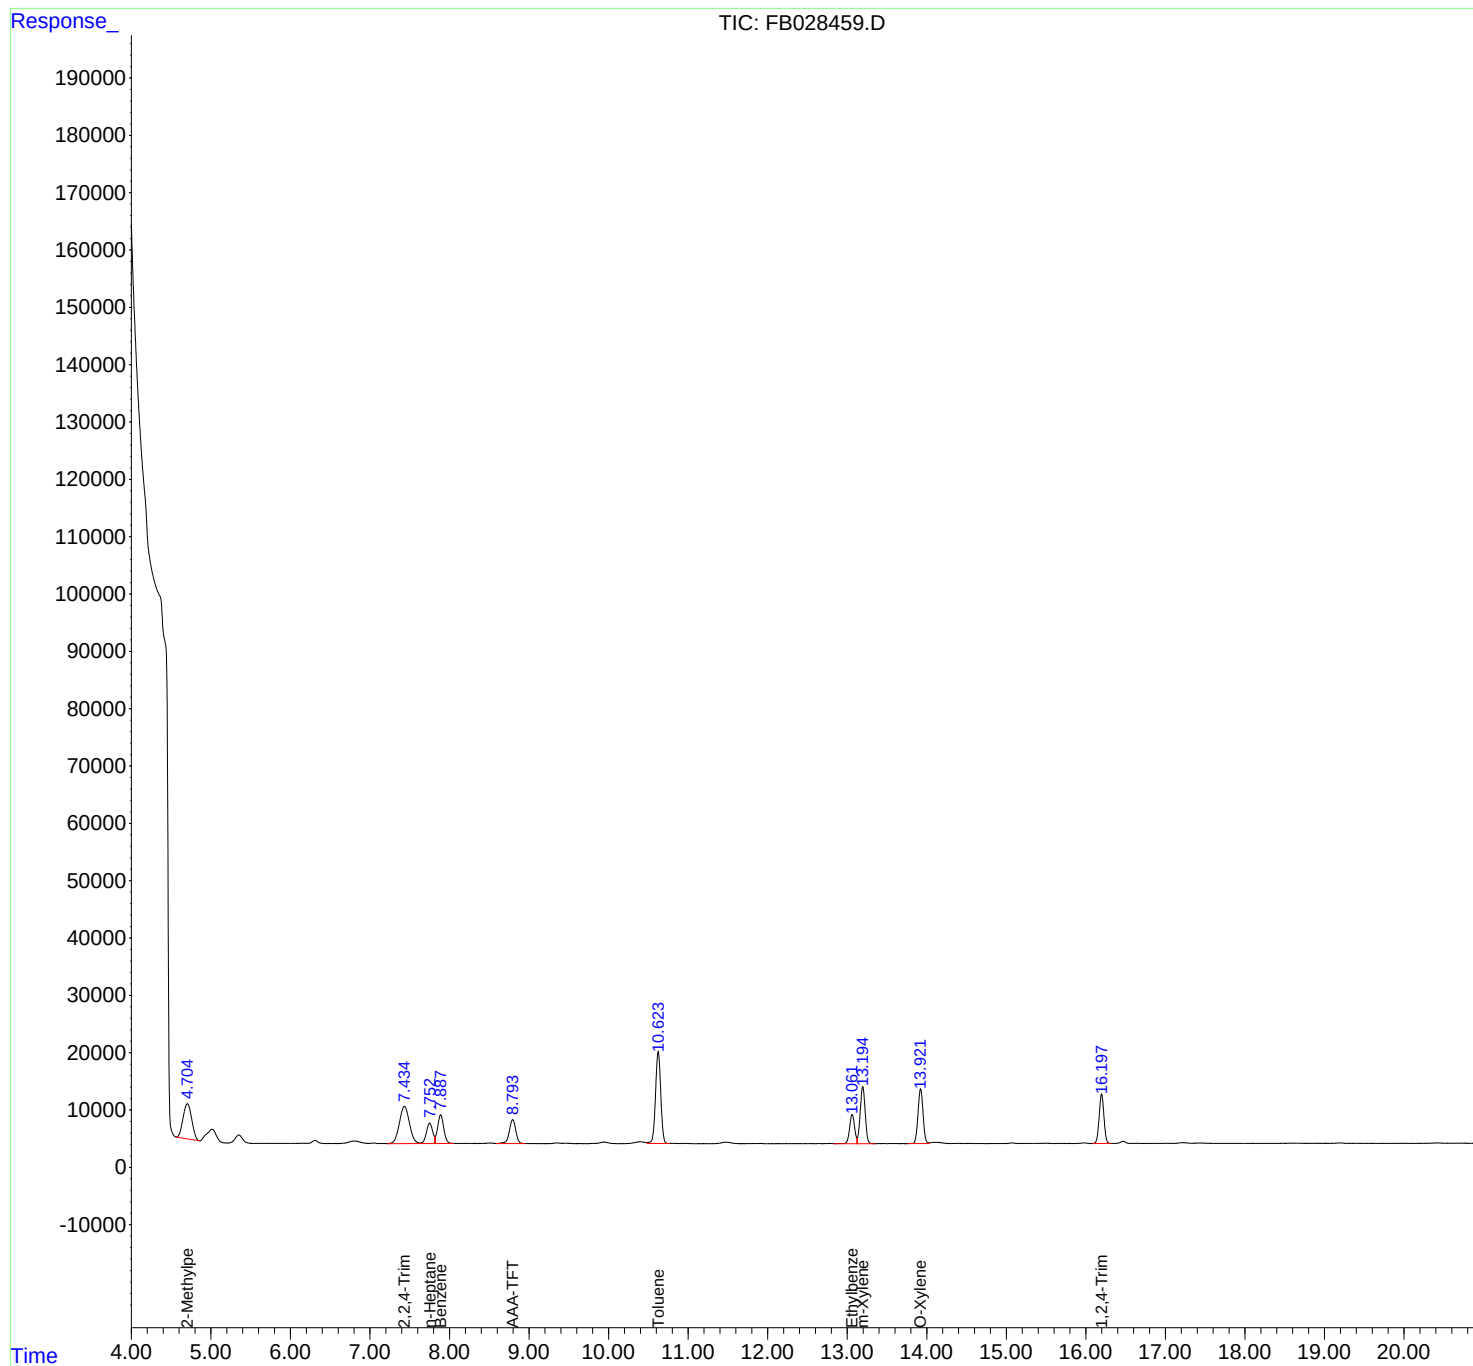


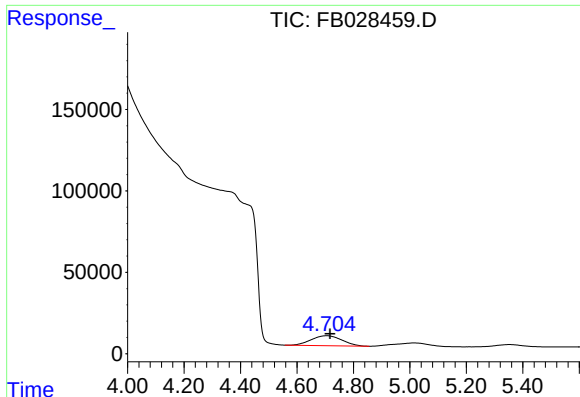

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.013 min
Response: 463058
Conc: 22.87 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(0-6)MSD

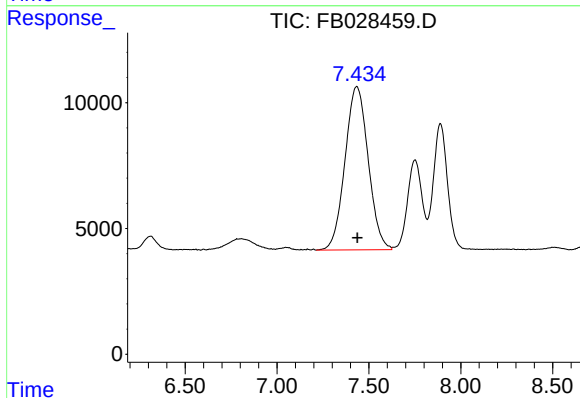


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: -0.002 min
Response: 570344
Conc: 27.11 ng/ml

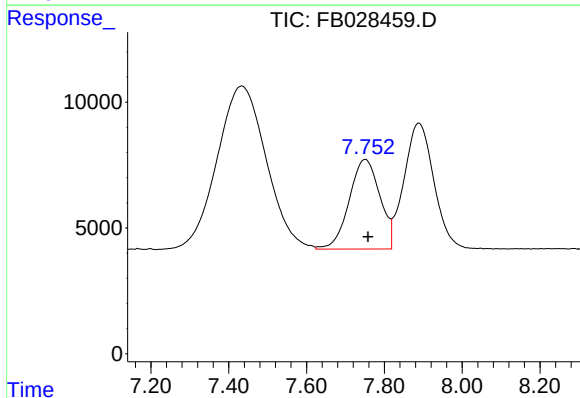


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 195655
Conc: 9.10 ng/ml

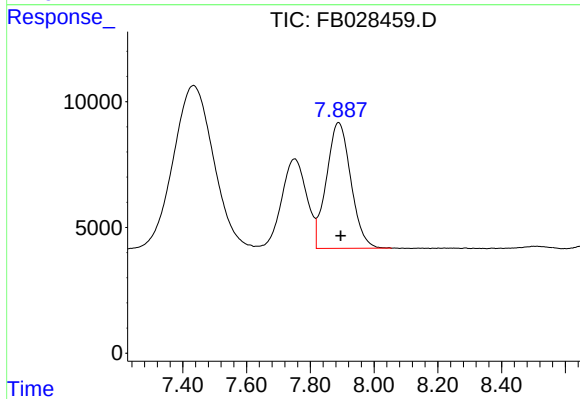

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.006 min
Response: 266136
Conc: 10.82 ng/ml

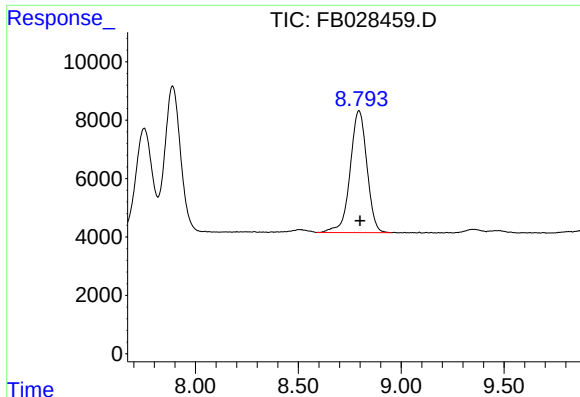

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.005 min
Response: 236453
Conc: 19.76 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(0-6)MSD

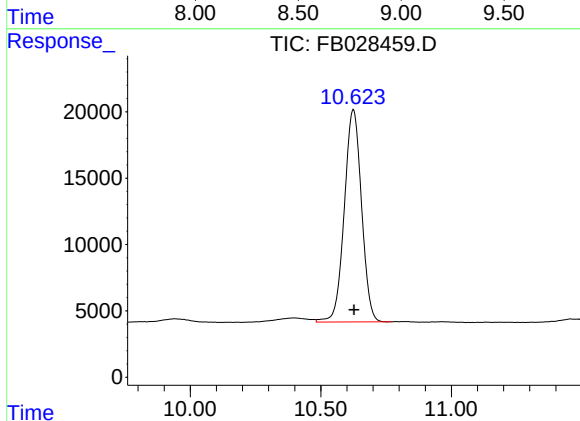


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 733321
Conc: 31.50 ng/ml

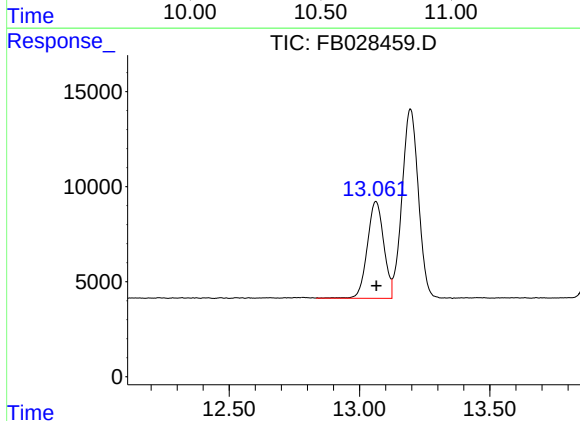


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.002 min
Response: 223388
Conc: 10.05 ng/ml

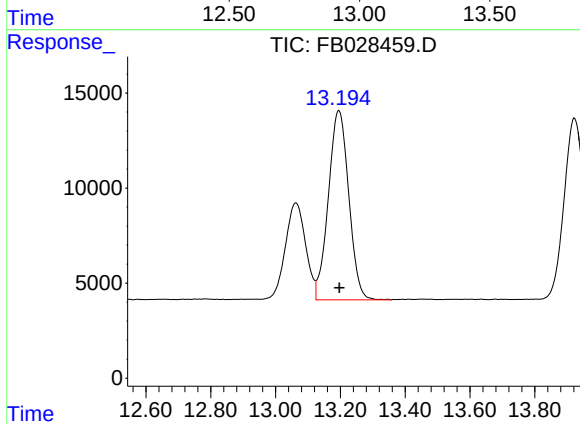

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.002 min
Response: 435682
Conc: 19.96 ng/ml

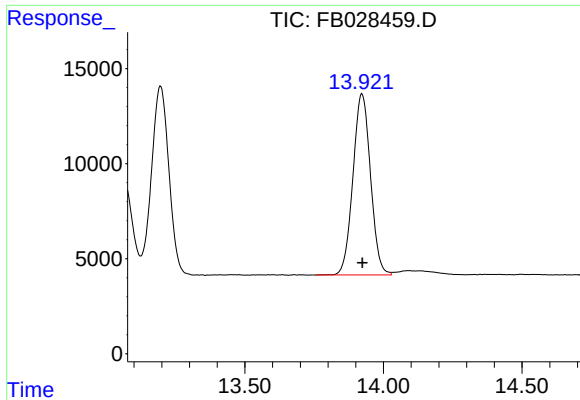

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.001 min
Response: 419310
Conc: 20.01 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(0-6)MSD

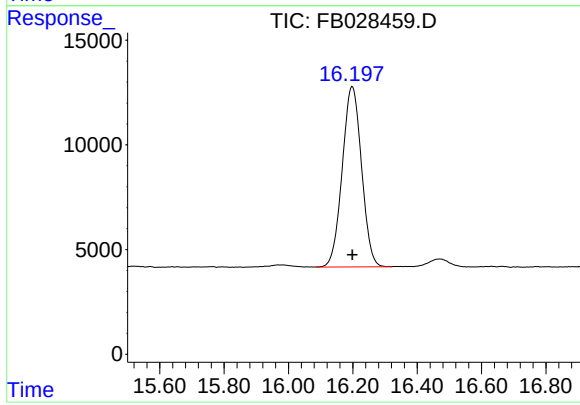

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 358314
Conc: 17.82 ng/ml