

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092818\
 Data File : FB017995.D
 Signal(s) : FID2B.CH
 Acq On : 28 Sep 2018 10:33
 Operator : MJ/SJ
 Sample : BSF0928S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 28 13:19:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
 Quant Title :
 QLast Update : Fri Sep 14 13:09:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	173575	20.520 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	404072	25.373 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	401649	25.239 ng/ml
3) t n-Heptane	8.065	128745	8.354 ng/ml
4) t Benzene	8.203	171634	9.016 ng/ml
6) t Toluene	10.957	431599	27.271 ng/ml
7) t Ethylbenzene	13.407	153064	9.367 ng/ml
8) t m-Xylene	13.539	325115	18.793 ng/ml
9) t O-Xylene	14.271	345109	18.991 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	386254	18.158 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092818\
Data File : FB017995.D
Signal(s) : FID2B.CH
Acq On : 28 Sep 2018 10:33
Operator : MJ/SJ
Sample : BSF0928S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 28 13:19:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB091418.M
Quant Title :
QLast Update : Fri Sep 14 13:09:25 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

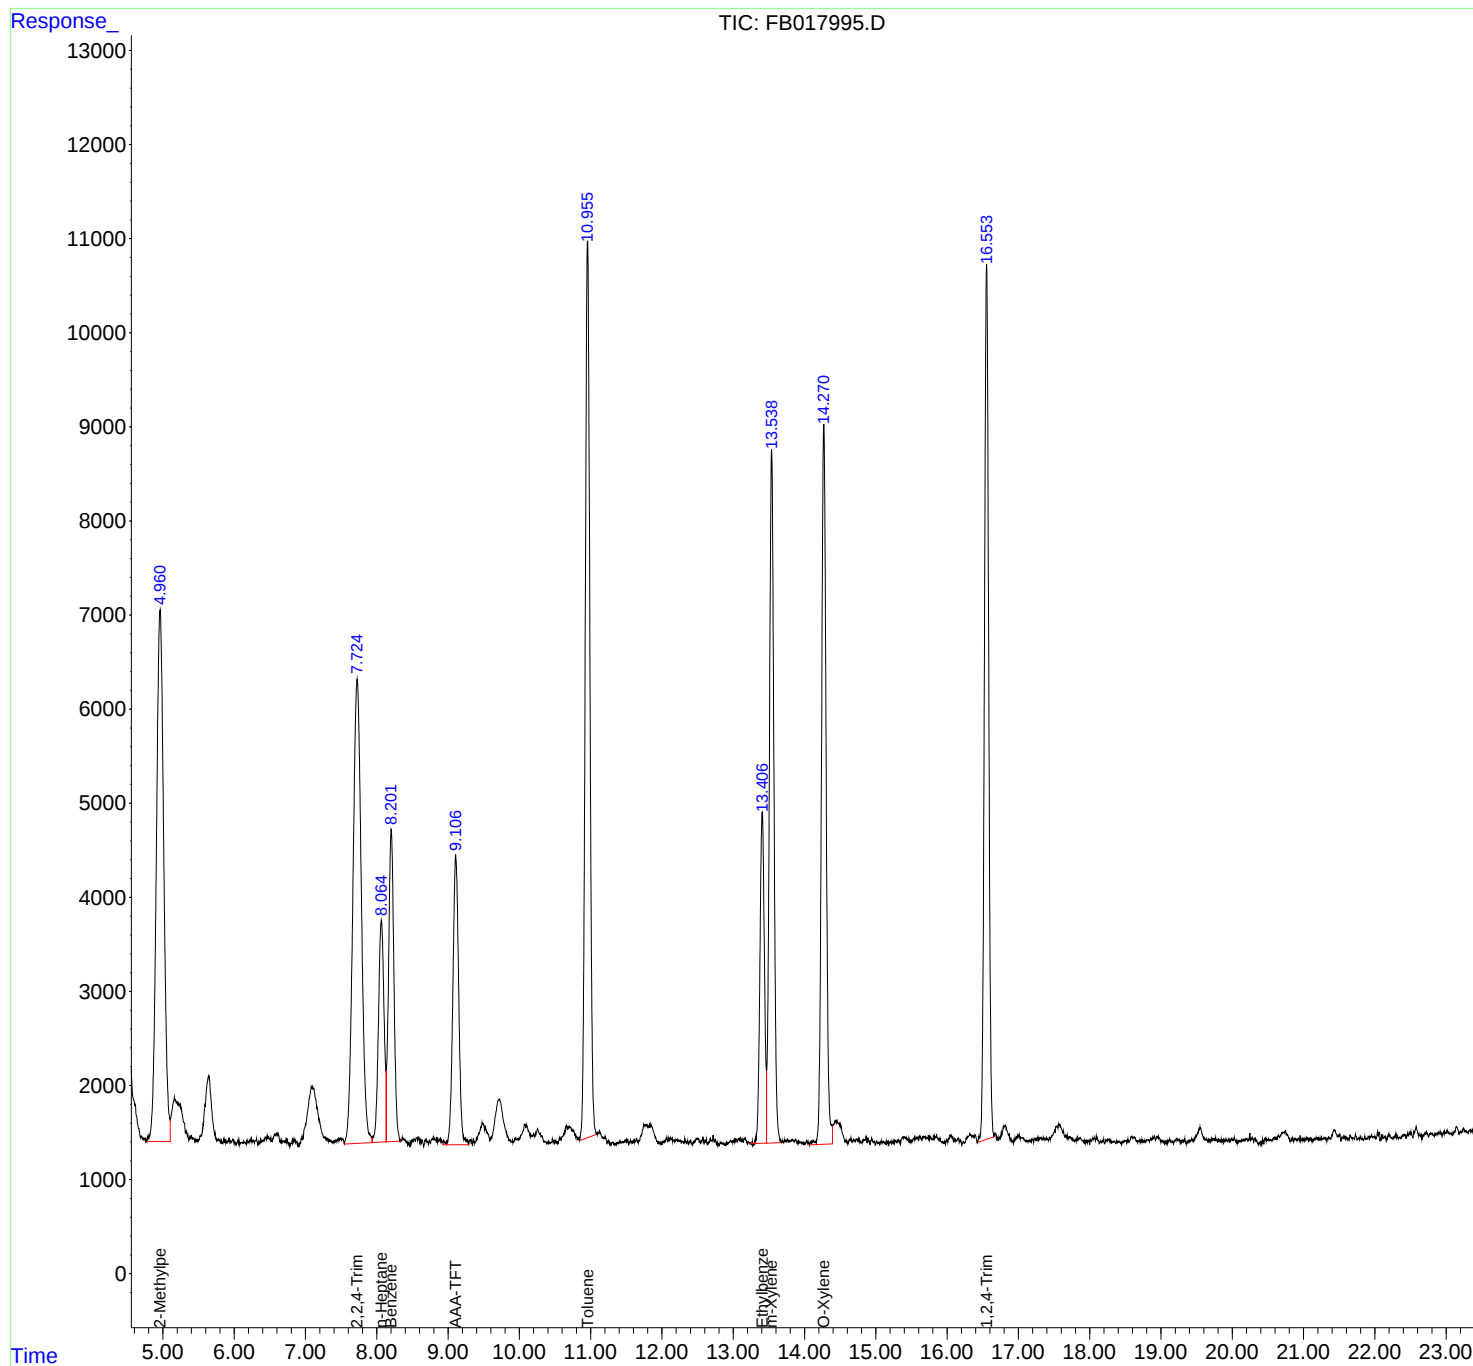

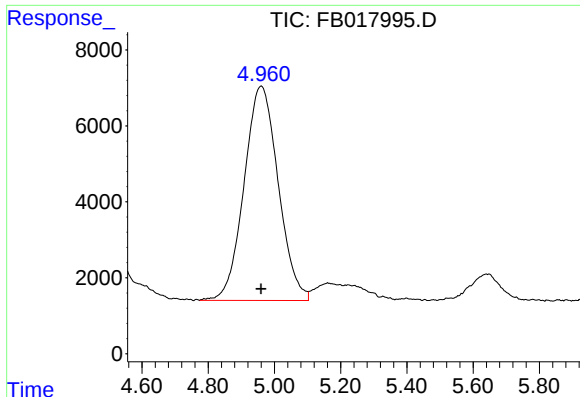


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 404072
Conc: 25.37 ng/ml

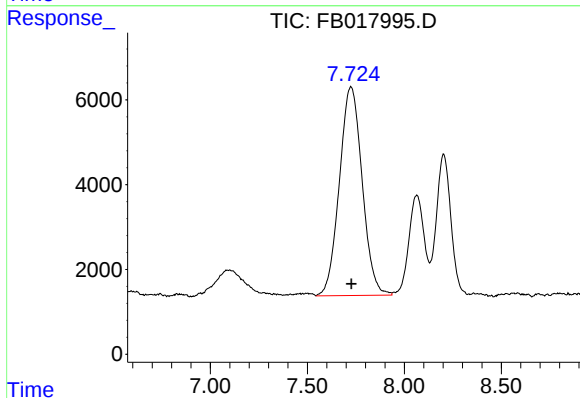


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.002 min
Response: 401649
Conc: 25.24 ng/ml

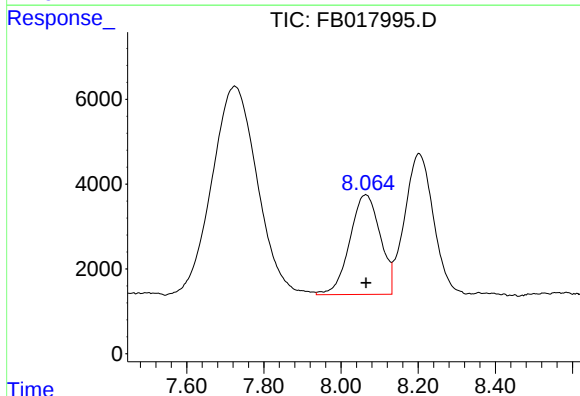


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 128745
Conc: 8.35 ng/ml

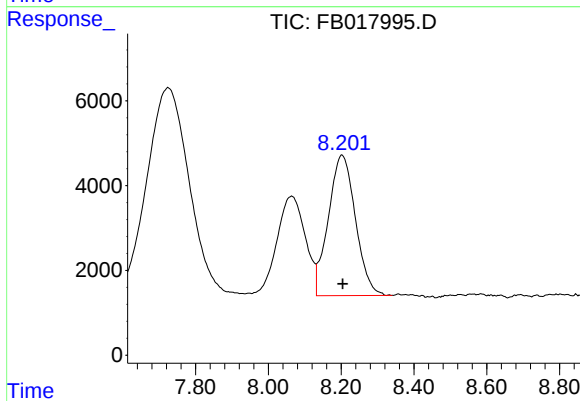


#4 Benzene

R.T.: 8.203 min
Delta R.T.: -0.001 min
Response: 171634
Conc: 9.02 ng/ml

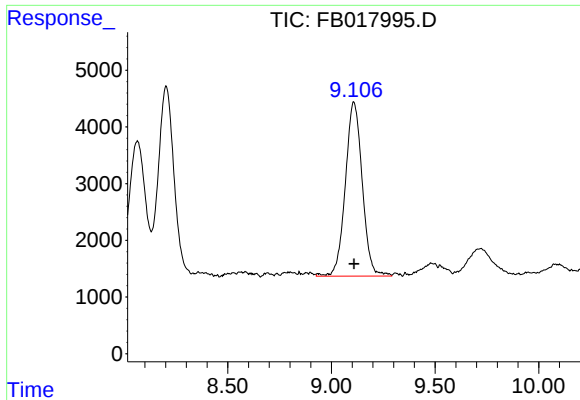


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.002 min
Response: 173575
Conc: 20.52 ng/ml

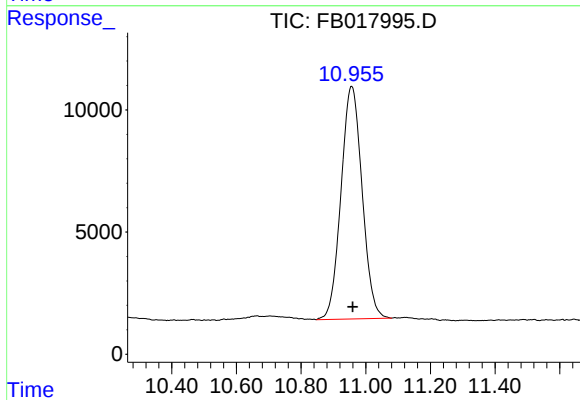


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.002 min
Response: 431599
Conc: 27.27 ng/ml

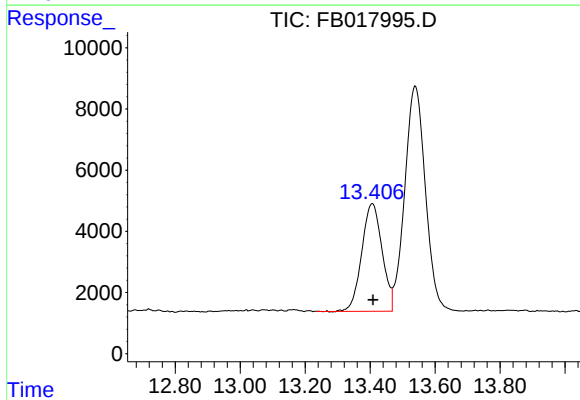


#7 Ethylbenzene

R.T.: 13.407 min
Delta R.T.: -0.002 min
Response: 153064
Conc: 9.37 ng/ml

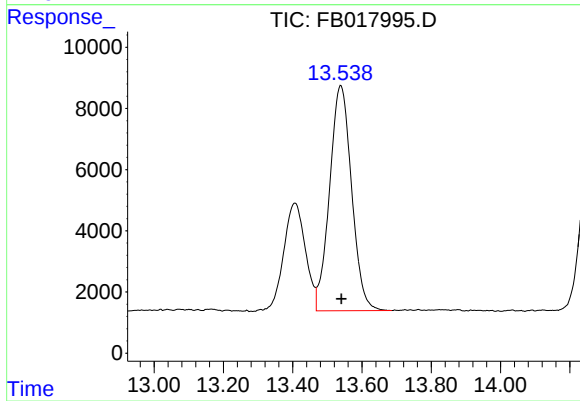


#8 m-Xylene

R.T.: 13.539 min
Delta R.T.: -0.002 min
Response: 325115
Conc: 18.79 ng/ml

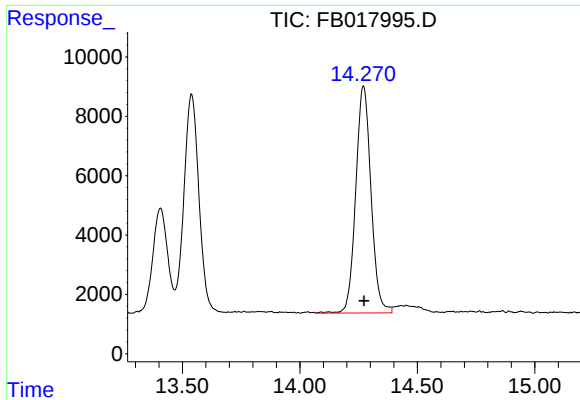

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: -0.002 min
Response: 345109
Conc: 18.99 ng/ml

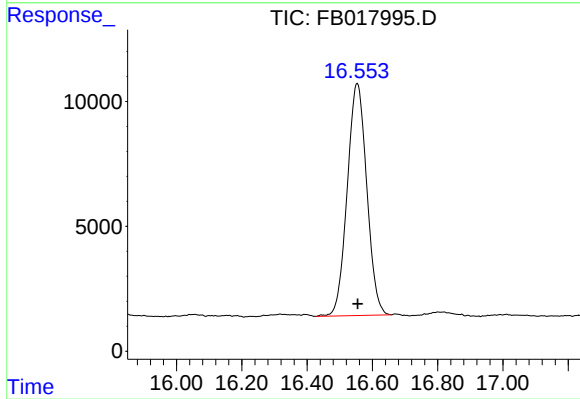

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.001 min
Response: 386254
Conc: 18.16 ng/ml