

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092920\
 Data File : FB024965.D
 Signal(s) : FID2B.CH
 Acq On : 29 Sep 2020 11:25
 Operator : DD/AJ
 Sample : BSF0929S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0929S1

Integration File: Calibration.e
 Quant Time: Sep 30 00:52:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	383442	18.264 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	841798	27.991 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	889658	29.108 ng/ml
3) t n-Heptane	7.759	294011	9.665 ng/ml
4) t Benzene	7.894	352796	9.471 ng/ml
6) t Toluene	10.632	999555	28.633 ng/ml
7) t Ethylbenzene	13.072	310480	9.578 ng/ml
8) t m-Xylene	13.205	613417	19.310 ng/ml
9) t O-Xylene	13.933	596643	19.634 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	500323	19.727 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092920\
Data File : FB024965.D
Signal(s) : FID2B.CH
Acq On : 29 Sep 2020 11:25
Operator : DD/AJ
Sample : BSF0929S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0929S1

Integration File: Calibration.e
Quant Time: Sep 30 00:52:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

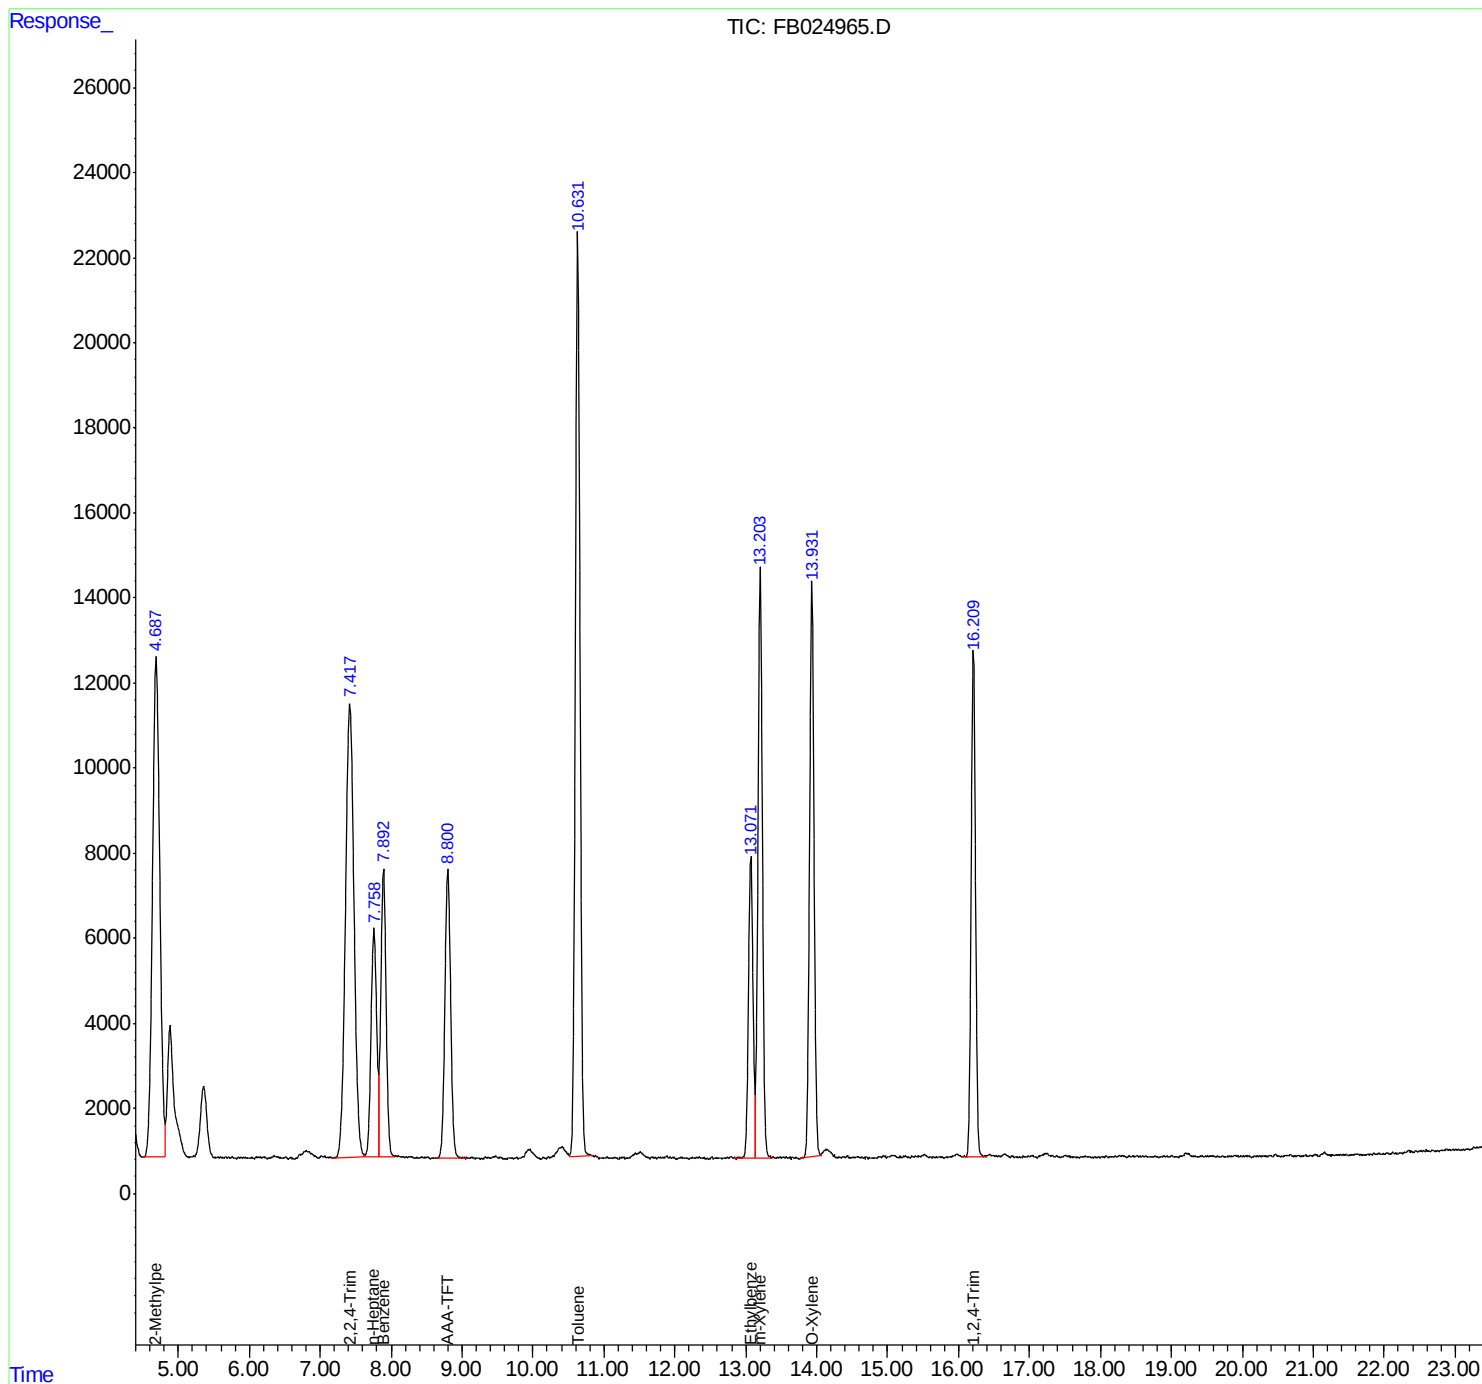


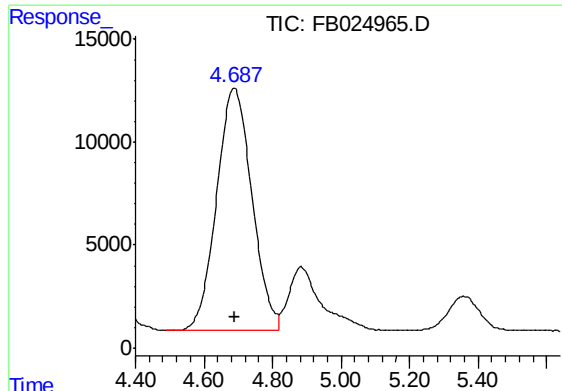

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 841798
Conc: 27.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S1

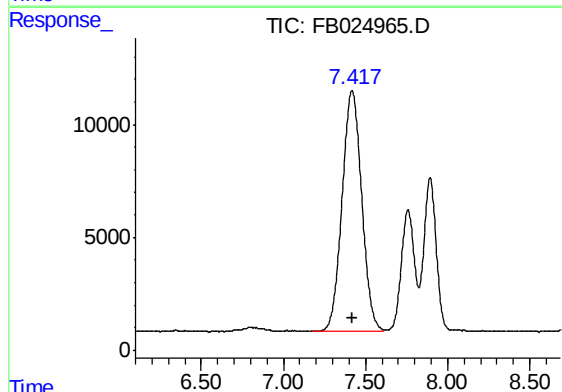


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 889658
Conc: 29.11 ng/ml

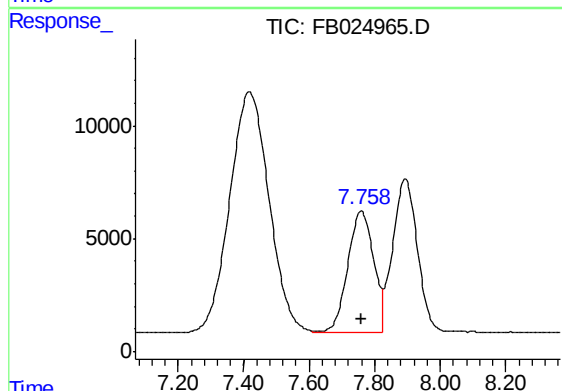


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 294011
Conc: 9.66 ng/ml

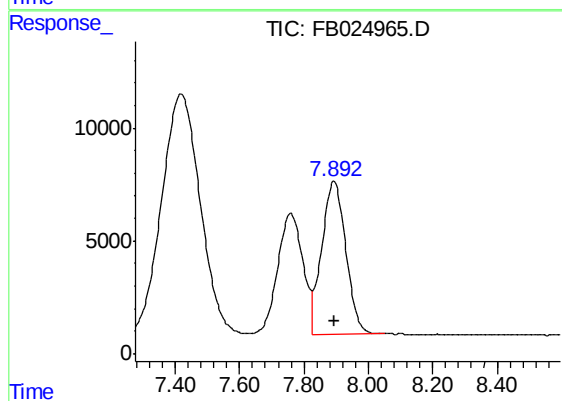

#4 Benzene


R.T.: 7.894 min
Delta R.T.: -0.001 min
Response: 352796
Conc: 9.47 ng/ml

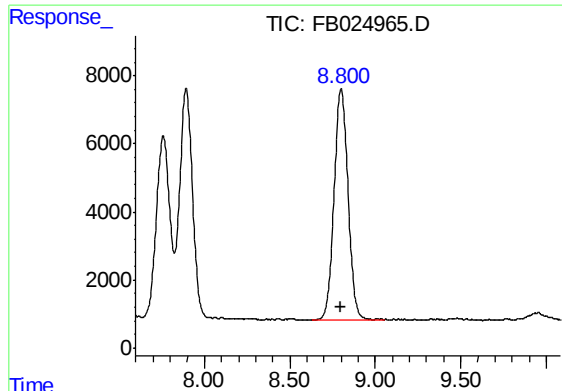

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 383442
Conc: 18.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S1

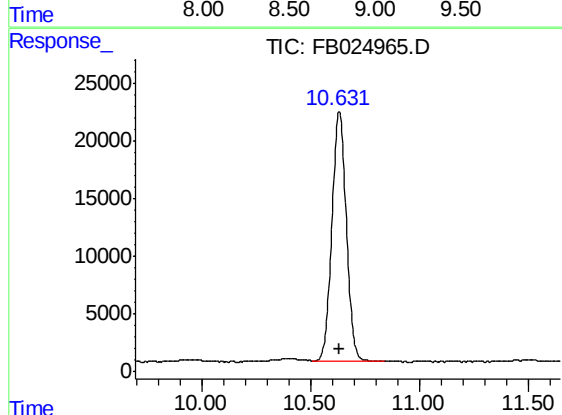


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 999555
Conc: 28.63 ng/ml

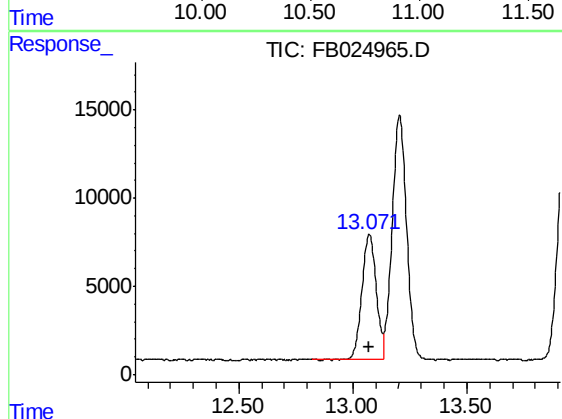


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 310480
Conc: 9.58 ng/ml

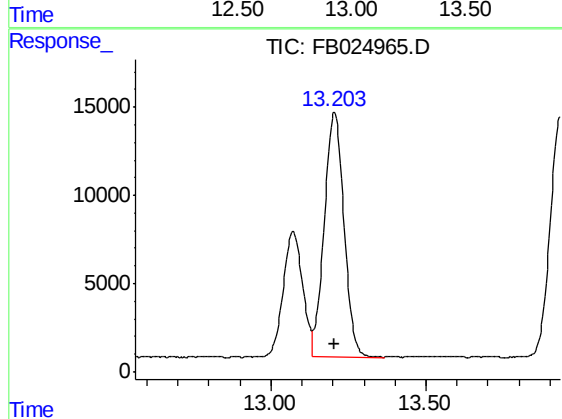

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 613417
Conc: 19.31 ng/ml

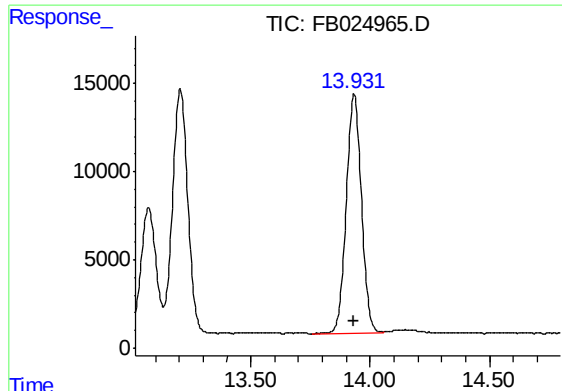

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 596643
Conc: 19.63 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S1

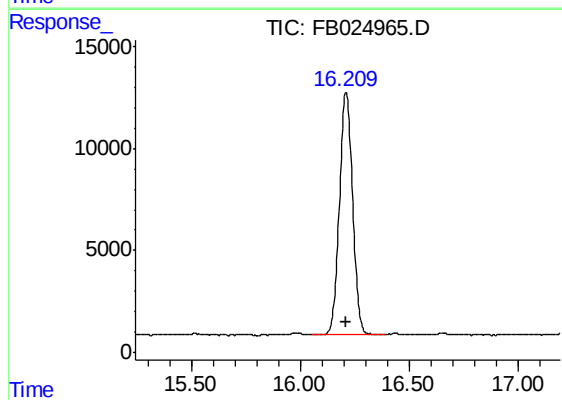

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 500323
Conc: 19.73 ng/ml