

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092920\
 Data File : FB024969.D
 Signal(s) : FID2B.CH
 Acq On : 29 Sep 2020 13:30
 Operator : DD/AJ
 Sample : L3869-12MSD
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-03-092820MSD

Integration File: Calibration.e
 Quant Time: Sep 30 00:53:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	401068	19.104 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	715947	23.807 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	619180	20.259 ng/ml
3) t n-Heptane	7.761	164410	5.404 ng/ml
4) t Benzene	7.896	350874	9.419 ng/ml
6) t Toluene	10.633	885720	25.372 ng/ml
7) t Ethylbenzene	13.073	239777	7.397 ng/ml
8) t m-Xylene	13.206	304889	9.598 ng/ml
9) t O-Xylene	13.934	404869	13.323 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	64773	2.554 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092920\
Data File : FB024969.D
Signal(s) : FID2B.CH
Acq On : 29 Sep 2020 13:30
Operator : DD/AJ
Sample : L3869-12MSD
Misc : 5.05/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-03-092820MSD

Integration File: Calibration.e
Quant Time: Sep 30 00:53:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

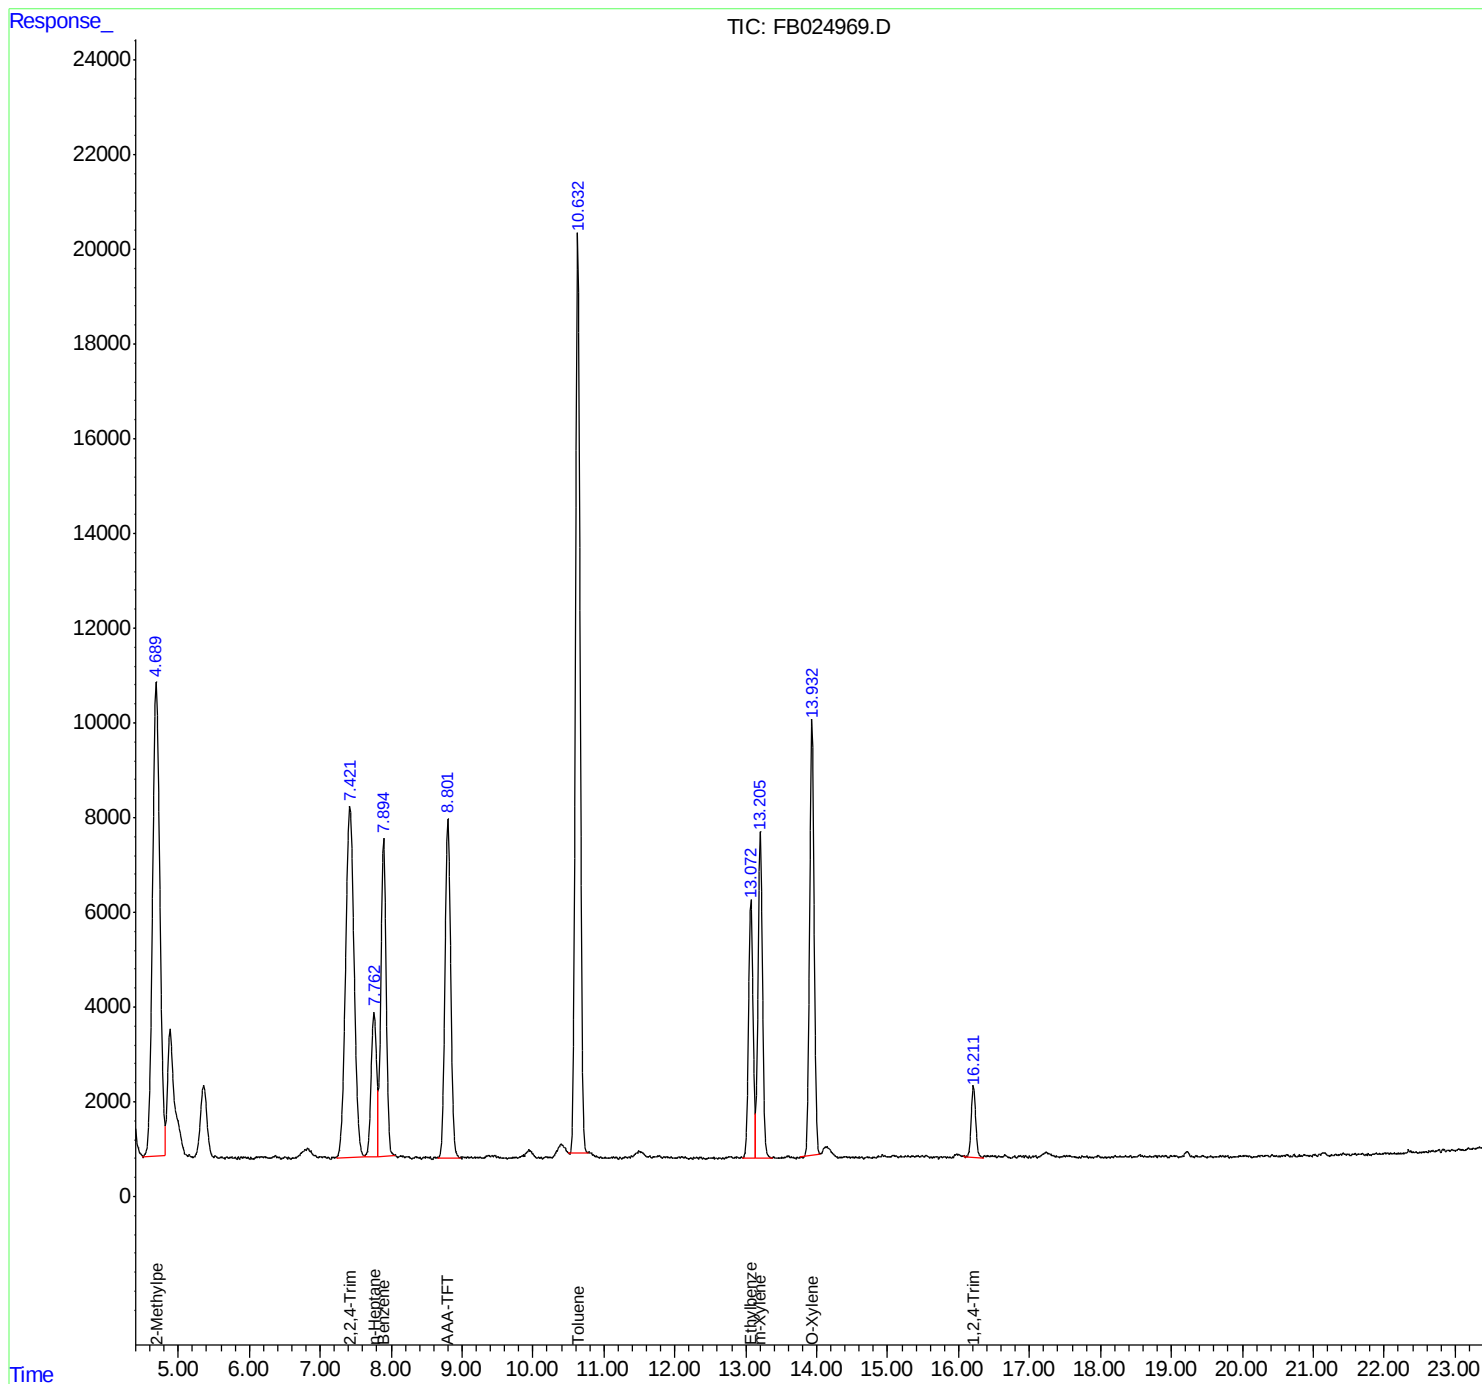


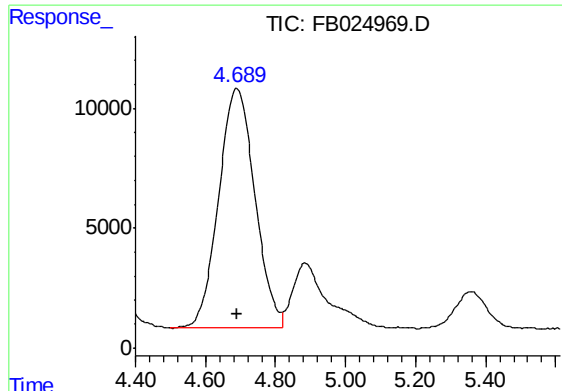

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 715947
Conc: 23.81 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-03-092820MSD

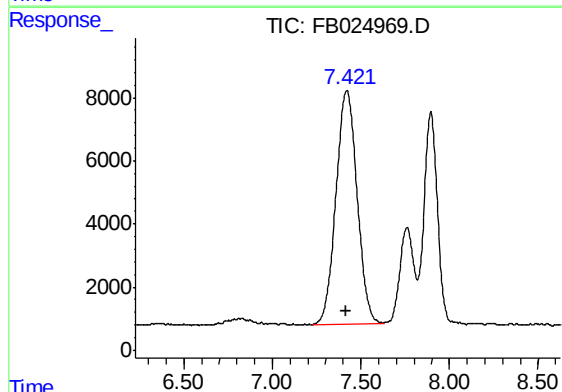


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.004 min
Response: 619180
Conc: 20.26 ng/ml

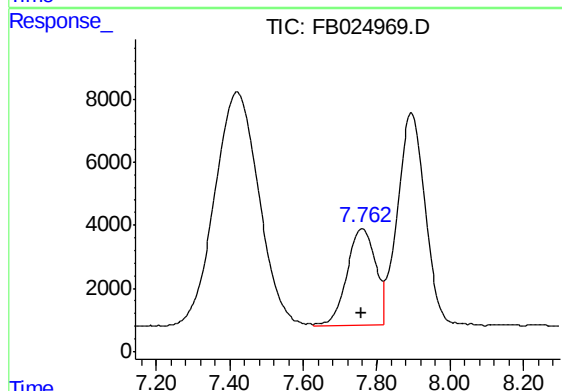


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.002 min
Response: 164410
Conc: 5.40 ng/ml

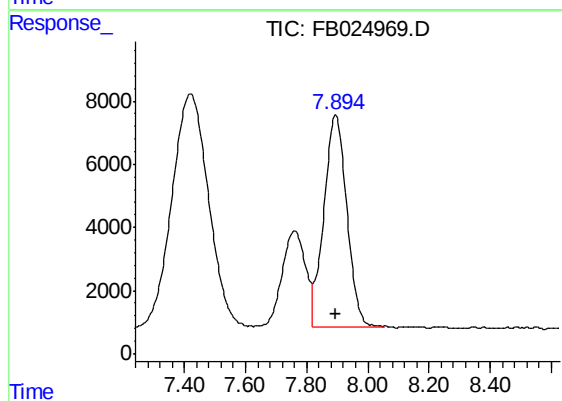

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 350874
Conc: 9.42 ng/ml

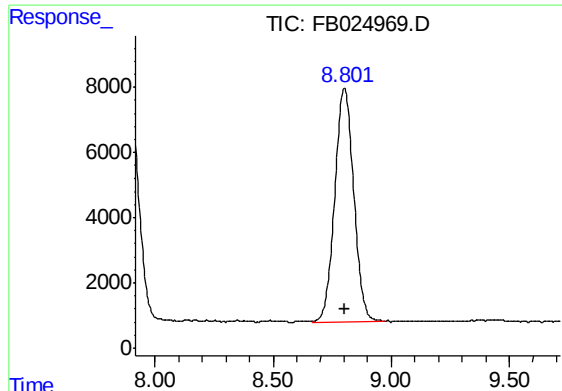

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 401068
Conc: 19.10 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-03-092820MSD

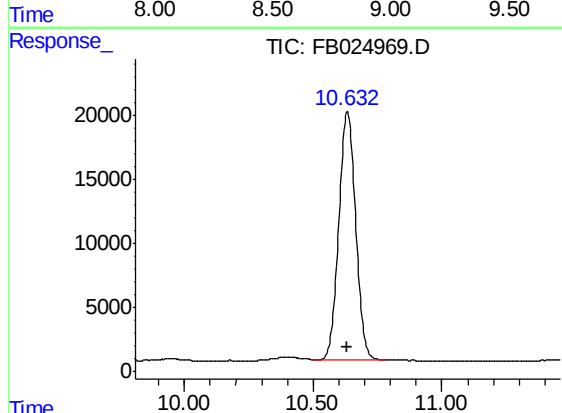


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.002 min
Response: 885720
Conc: 25.37 ng/ml

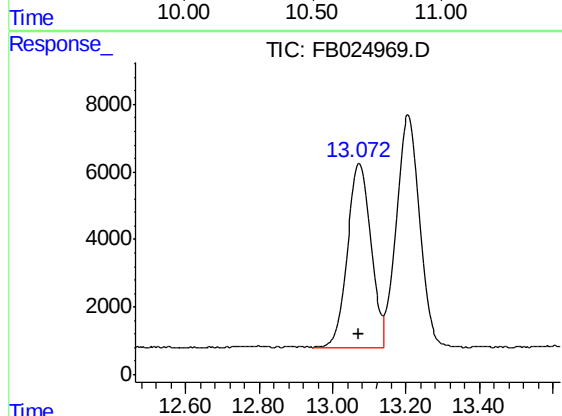


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.002 min
Response: 239777
Conc: 7.40 ng/ml

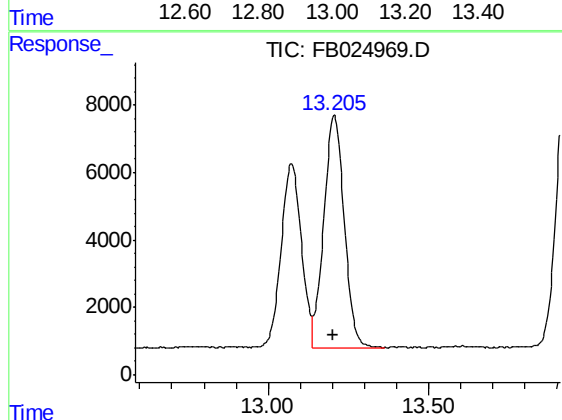

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.002 min
Response: 304889
Conc: 9.60 ng/ml

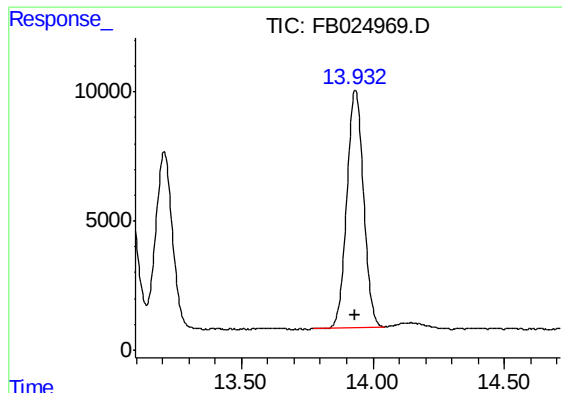

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.002 min
Response: 404869
Conc: 13.32 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-03-092820MSD

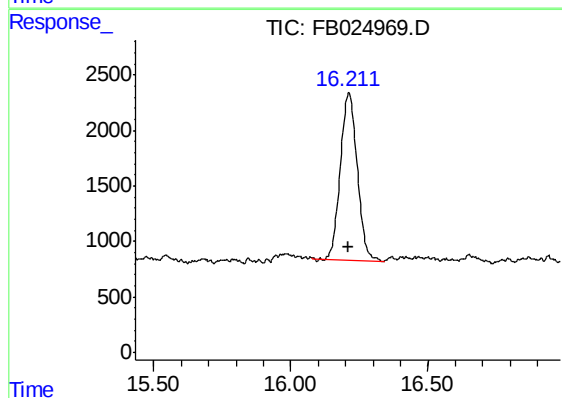

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.002 min
Response: 64773
Conc: 2.55 ng/ml