

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092920\
Data File : FB024966.D
Signal(s) : FID2B.CH
Acq On : 29 Sep 2020 11:56
Operator : DD/AJ
Sample : L3867-08
Misc : 5.04/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
EO-01-092820

Integration File: Calibration.e
Quant Time: Sep 30 00:52:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	439498	20.934 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092920\
Data File : FB024966.D
Signal(s) : FID2B.CH
Acq On : 29 Sep 2020 11:56
Operator : DD/AJ
Sample : L3867-08
Misc : 5.04/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
EO-01-092820

Integration File: Calibration.e
Quant Time: Sep 30 00:52:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

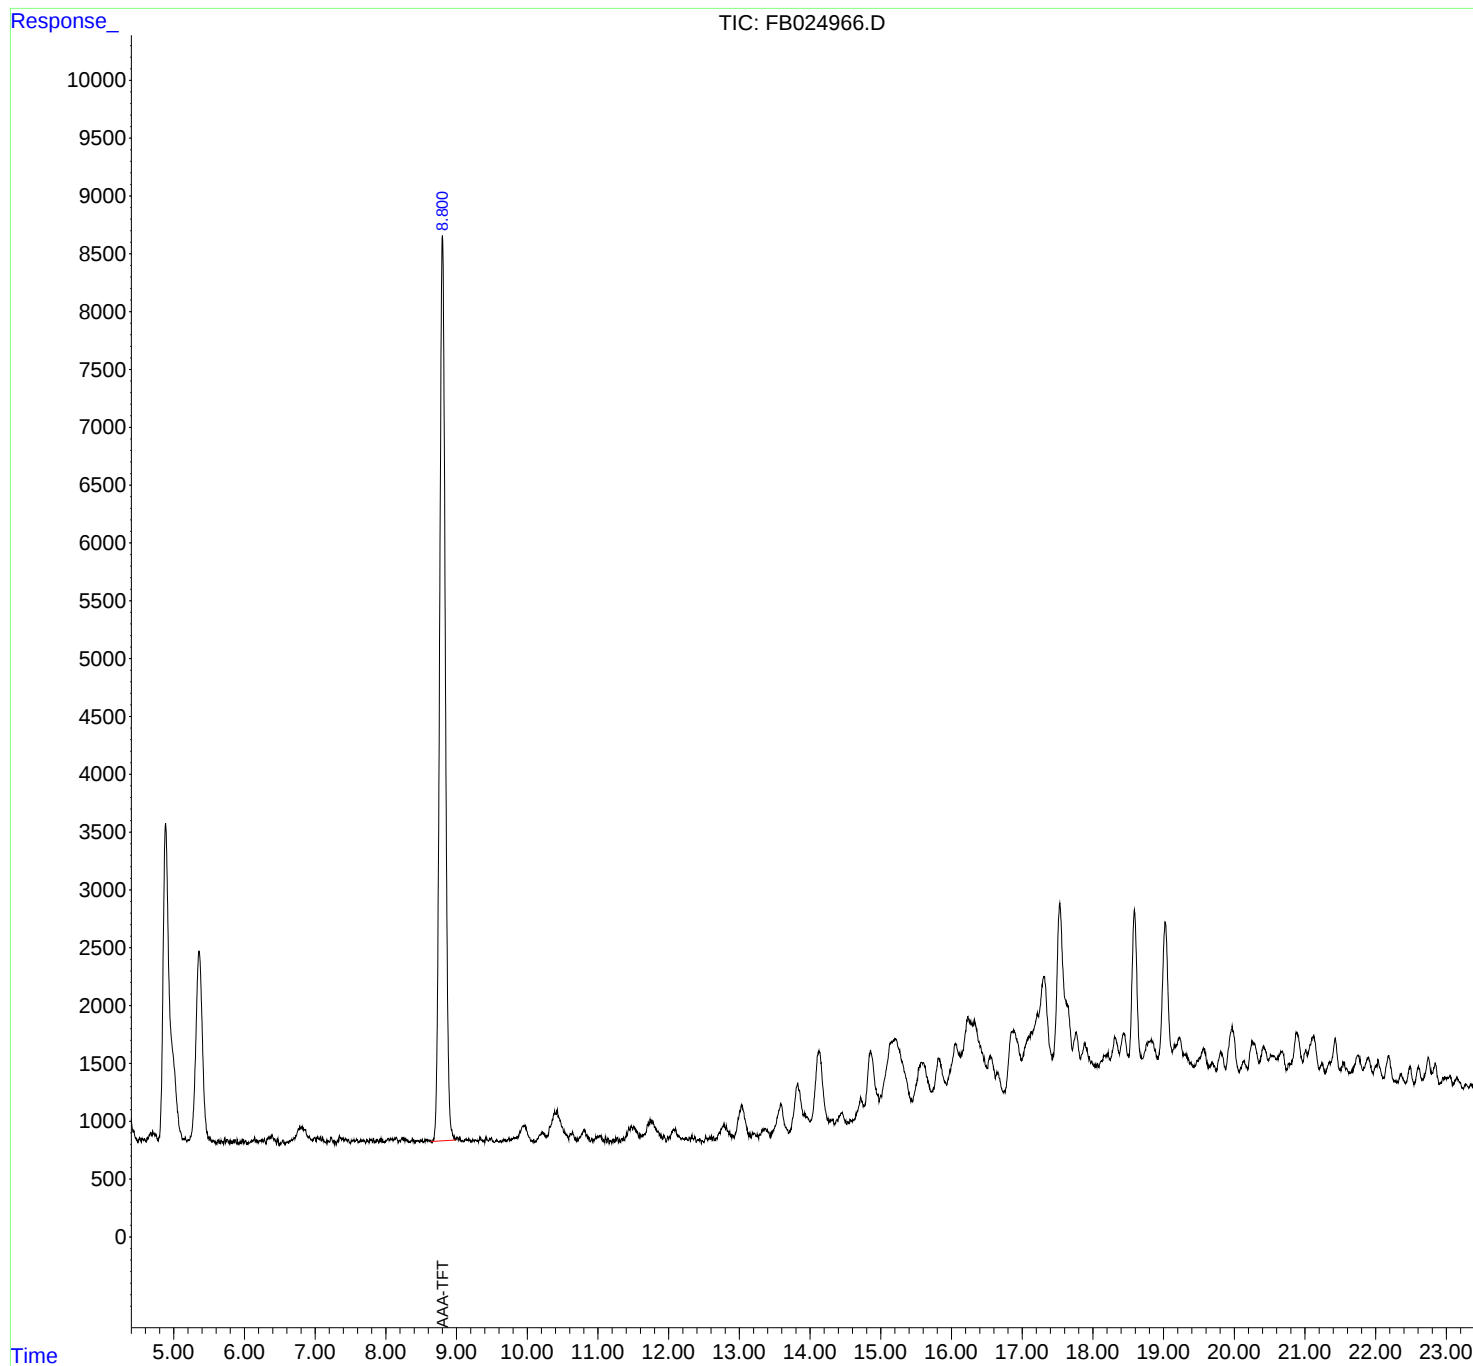

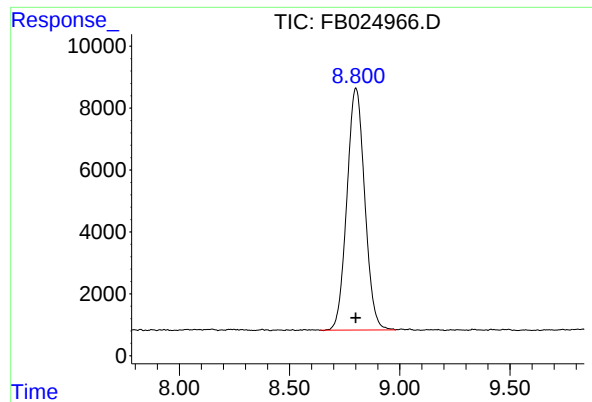

#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 439498
Conc: 20.93 ng/ml

Instrument :
FID_B
ClientSampleId :
EO-01-092820