

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092922\
 Data File : FB028481.D
 Signal(s) : FID2B.CH
 Acq On : 29 Sep 2022 11:49
 Operator : AJ/MA
 Sample : BSF0929S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0929S1

Integration File: SAMPLE.e
 Quant Time: Sep 29 18:49:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	213486	17.837 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	626002	30.918 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	662566	31.497 ng/ml
3) t n-Heptane	7.750	218535	10.166 ng/ml
4) t Benzene	7.887	266710	10.841 ng/ml
6) t Toluene	10.619	764609	32.842 ng/ml
7) t Ethylbenzene	13.056	233390	10.495 ng/ml
8) t m-Xylene	13.188	463130	21.223 ng/ml
9) t O-Xylene	13.915	450704	21.511 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	431768	21.473 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092922\
Data File : FB028481.D
Signal(s) : FID2B.CH
Acq On : 29 Sep 2022 11:49
Operator : AJ/MA
Sample : BSF0929S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0929S1

Integration File: SAMPLE.e
Quant Time: Sep 29 18:49:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

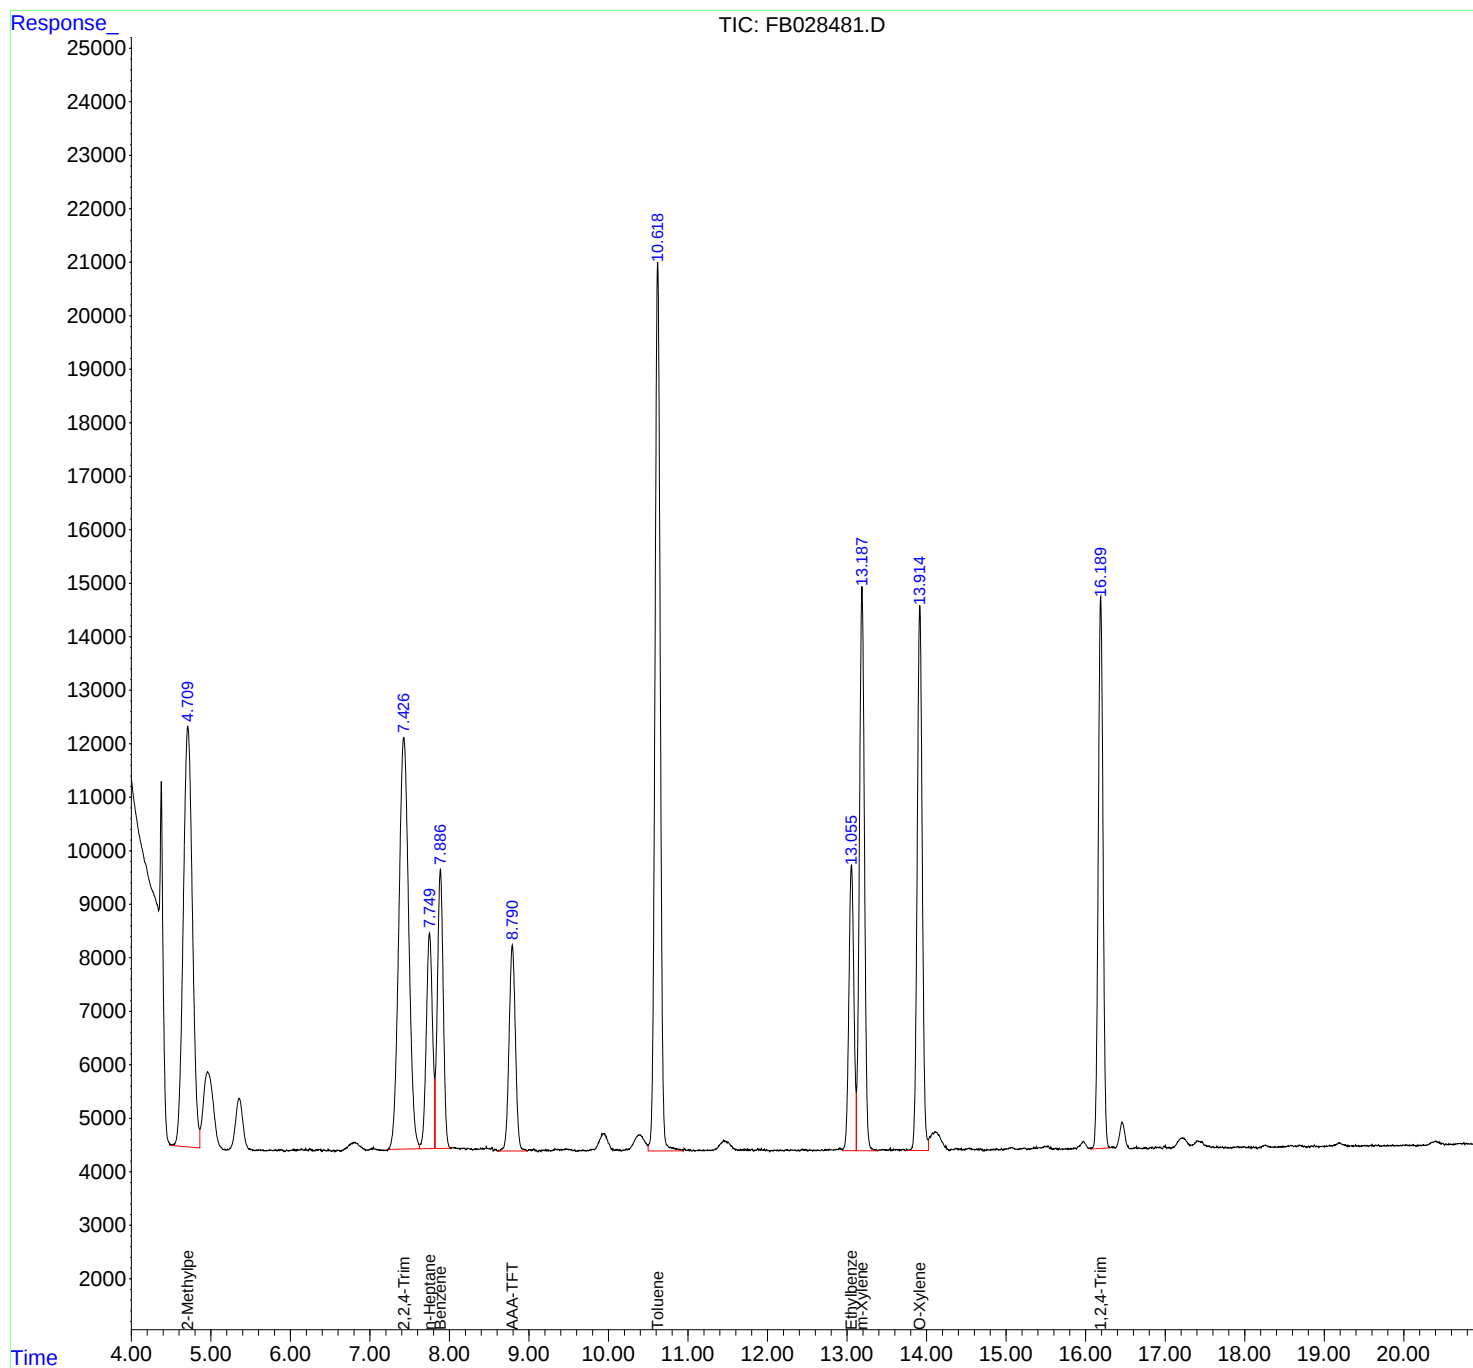


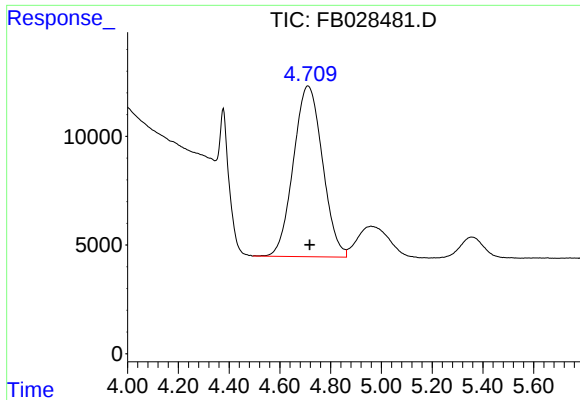

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: -0.007 min
Response: 626002
Conc: 30.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S1

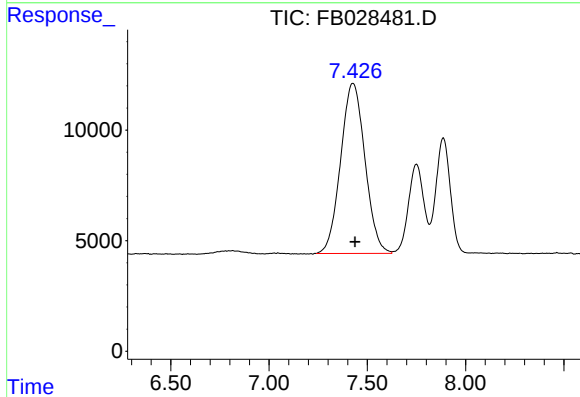


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.010 min
Response: 662566
Conc: 31.50 ng/ml

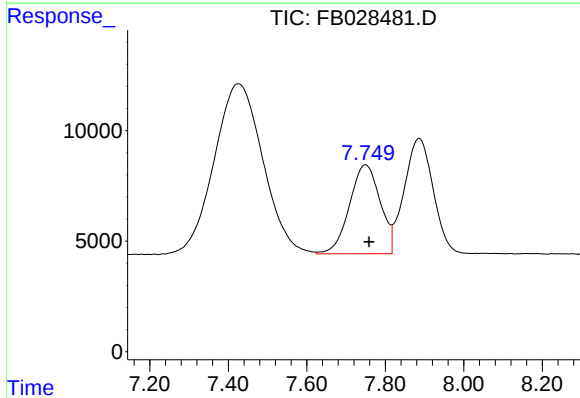


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.008 min
Response: 218535
Conc: 10.17 ng/ml

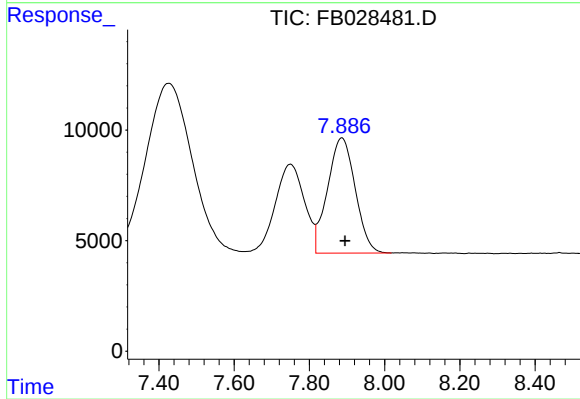

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.008 min
Response: 266710
Conc: 10.84 ng/ml

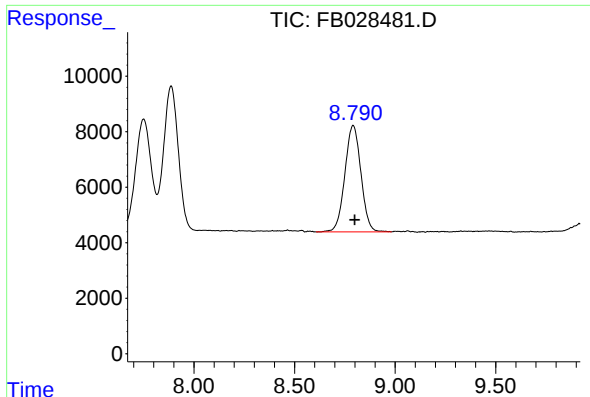

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.008 min
Response: 213486
Conc: 17.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S1

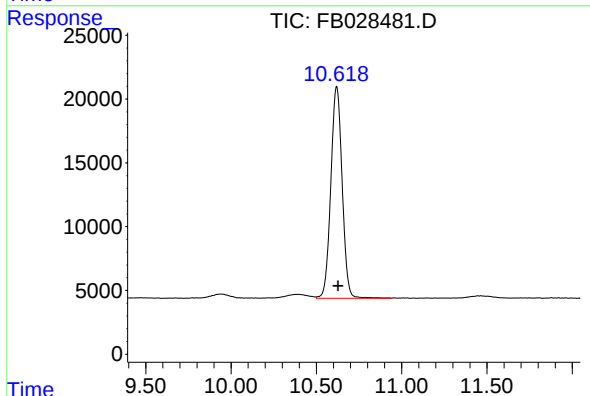


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.009 min
Response: 764609
Conc: 32.84 ng/ml

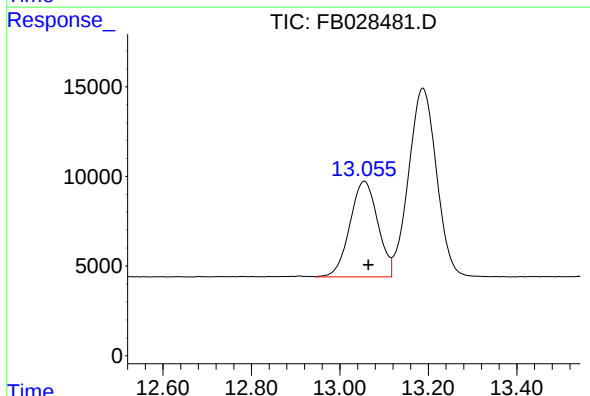


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.009 min
Response: 233390
Conc: 10.49 ng/ml

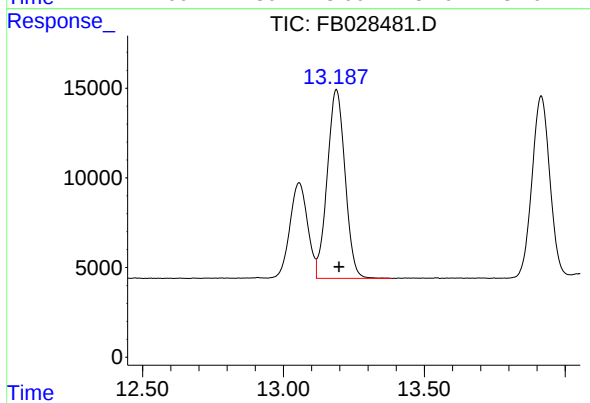

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.009 min
Response: 463130
Conc: 21.22 ng/ml

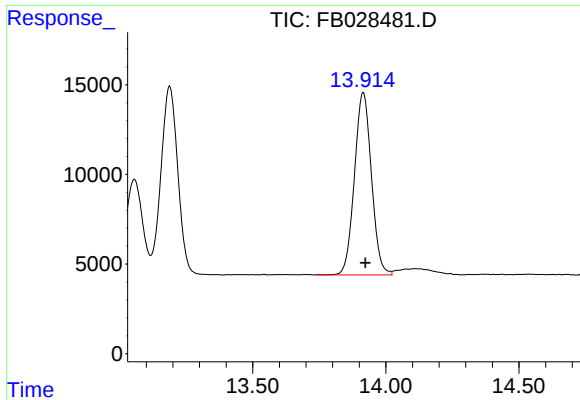

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.009 min
Response: 450704
Conc: 21.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S1

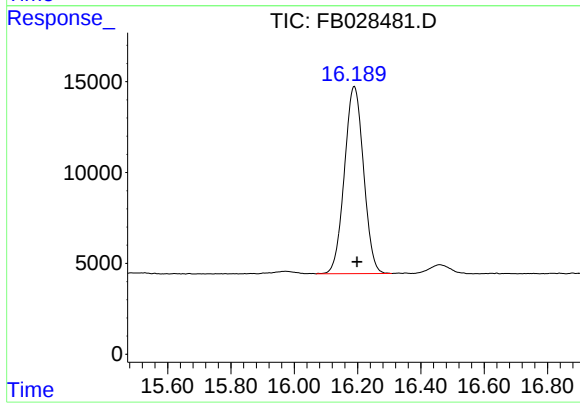

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.009 min
Response: 431768
Conc: 21.47 ng/ml