

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092922\
 Data File : FB028490.D
 Signal(s) : FID2B.CH
 Acq On : 29 Sep 2022 17:49
 Operator : AJ/MA
 Sample : N4803-02MSD 50X
 Misc : 5.05G/5.00 ML MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-T-1-(17-23)MSD

Integration File: SAMPLE.e
 Quant Time: Sep 29 18:58:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	211576	17.677 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	493196	24.359 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	621233	29.532 ng/ml
3) t n-Heptane	7.750	216443	10.069 ng/ml
4) t Benzene	7.889	277859	11.295 ng/ml
6) t Toluene	10.624	756591	32.498 ng/ml
7) t Ethylbenzene	13.061	235194	10.576 ng/ml
8) t m-Xylene	13.194	458045	20.990 ng/ml
9) t O-Xylene	13.921	435098	20.766 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	383435	19.070 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092922\
Data File : FB028490.D
Signal(s) : FID2B.CH
Acq On : 29 Sep 2022 17:49
Operator : AJ/MA
Sample : N4803-02MSD 50X
Misc : 5.05G/5.00 ML MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(17-23)MSD

Integration File: SAMPLE.e
Quant Time: Sep 29 18:58:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

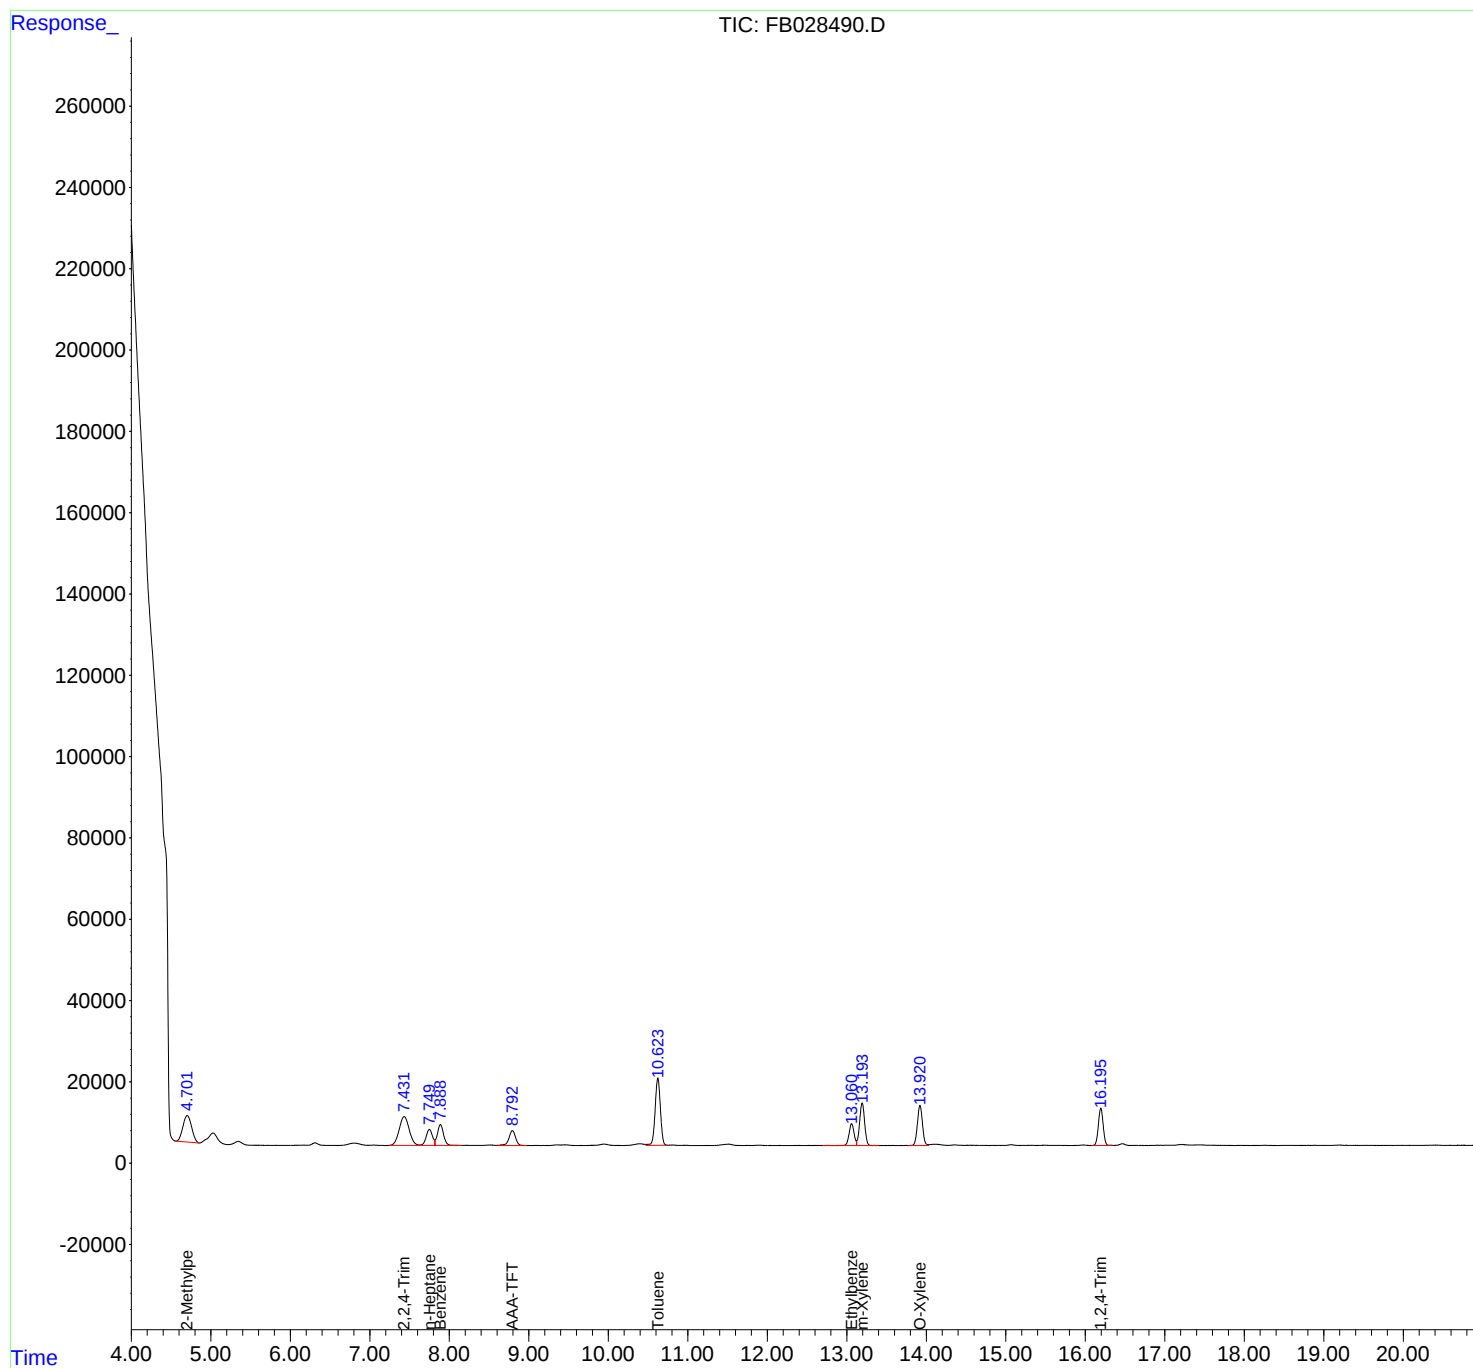


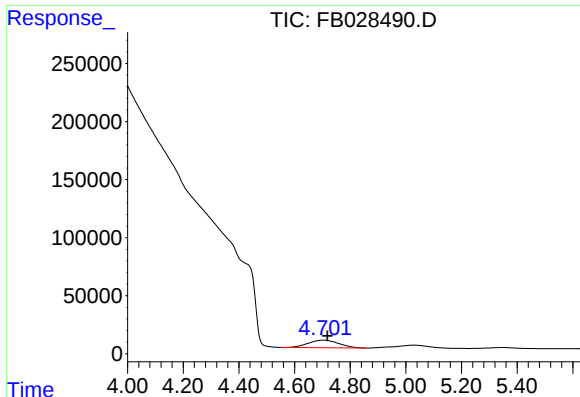

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.016 min
Response: 493196
Conc: 24.36 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(17-23)MSD

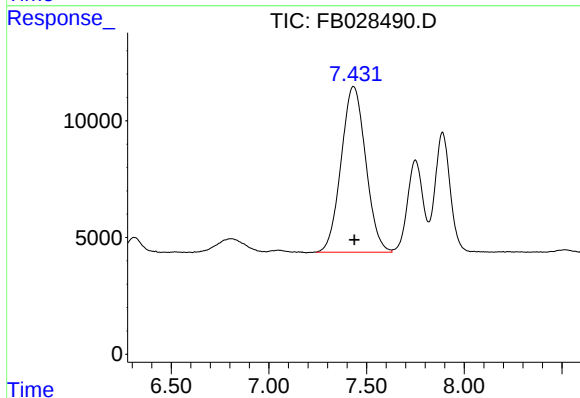


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: -0.005 min
Response: 621233
Conc: 29.53 ng/ml

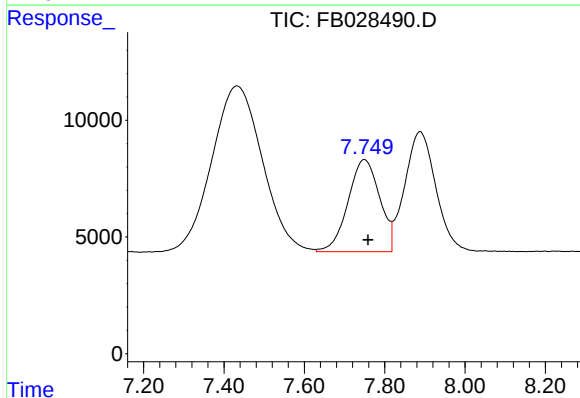


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.009 min
Response: 216443
Conc: 10.07 ng/ml

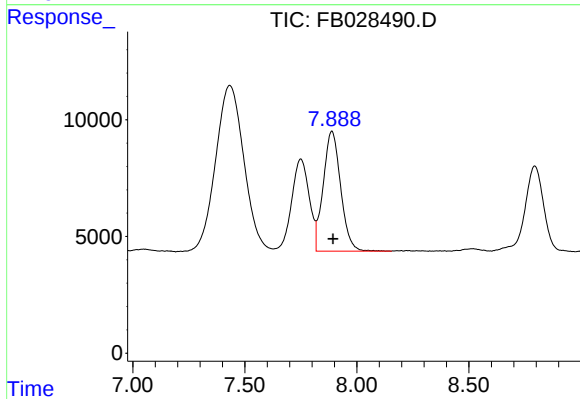

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.006 min
Response: 277859
Conc: 11.29 ng/ml

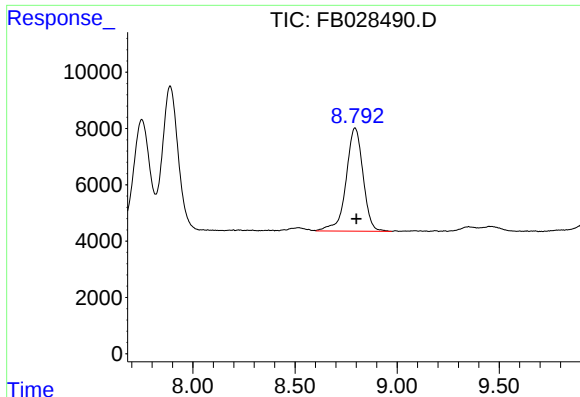

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.006 min
Response: 211576
Conc: 17.68 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(17-23)MSD

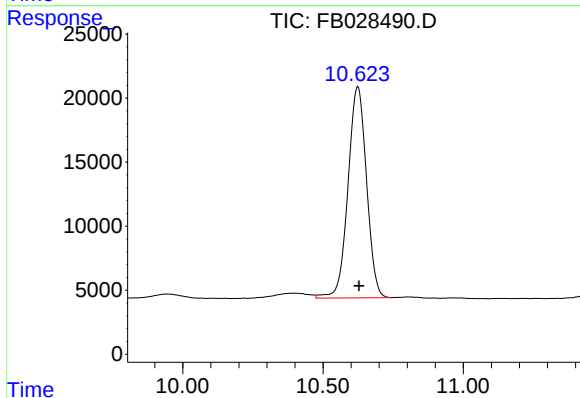


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.004 min
Response: 756591
Conc: 32.50 ng/ml

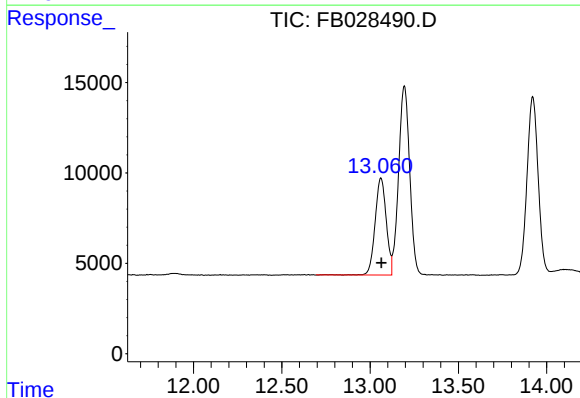


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.003 min
Response: 235194
Conc: 10.58 ng/ml

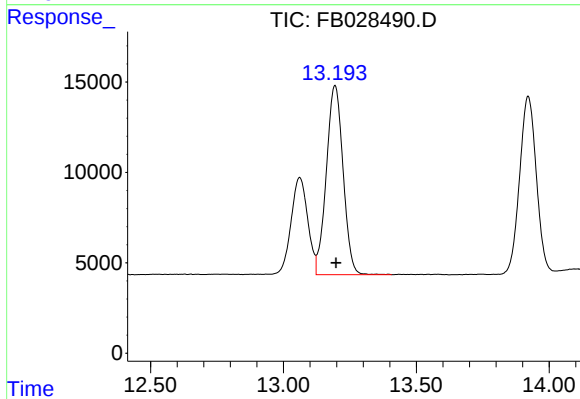

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.003 min
Response: 458045
Conc: 20.99 ng/ml

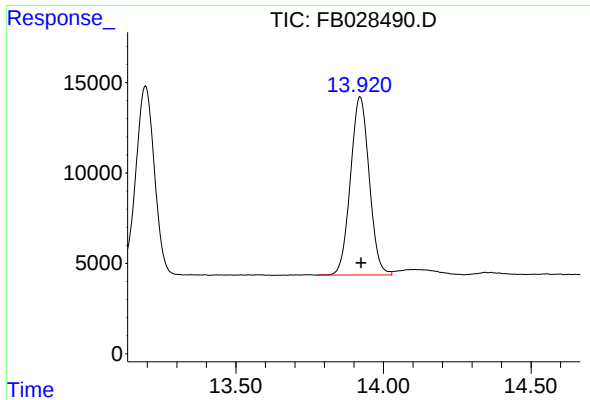

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.003 min
Response: 435098
Conc: 20.77 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-1-(17-23)MSD

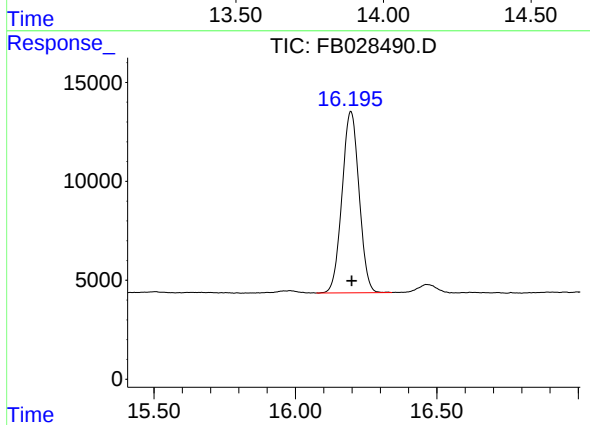

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.003 min
Response: 383435
Conc: 19.07 ng/ml