

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092922\
 Data File : FB028491.D
 Signal(s) : FID2B.CH
 Acq On : 29 Sep 2022 18:29
 Operator : AJ/MA
 Sample : BSF0929S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0929S2

Integration File: SAMPLE.e
 Quant Time: Sep 29 18:58:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
 Quant Title :
 QLast Update : Thu Sep 08 15:28:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	236737	19.779 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	612643	30.258 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	677005	32.183 ng/ml
3) t n-Heptane	7.756	222033	10.329 ng/ml
4) t Benzene	7.893	261103	10.613 ng/ml
6) t Toluene	10.626	759817	32.636 ng/ml
7) t Ethylbenzene	13.063	239123	10.753 ng/ml
8) t m-Xylene	13.195	469725	21.525 ng/ml
9) t O-Xylene	13.922	452505	21.597 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	422372	21.006 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092922\
Data File : FB028491.D
Signal(s) : FID2B.CH
Acq On : 29 Sep 2022 18:29
Operator : AJ/MA
Sample : BSF0929S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0929S2

Integration File: SAMPLE.e
Quant Time: Sep 29 18:58:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

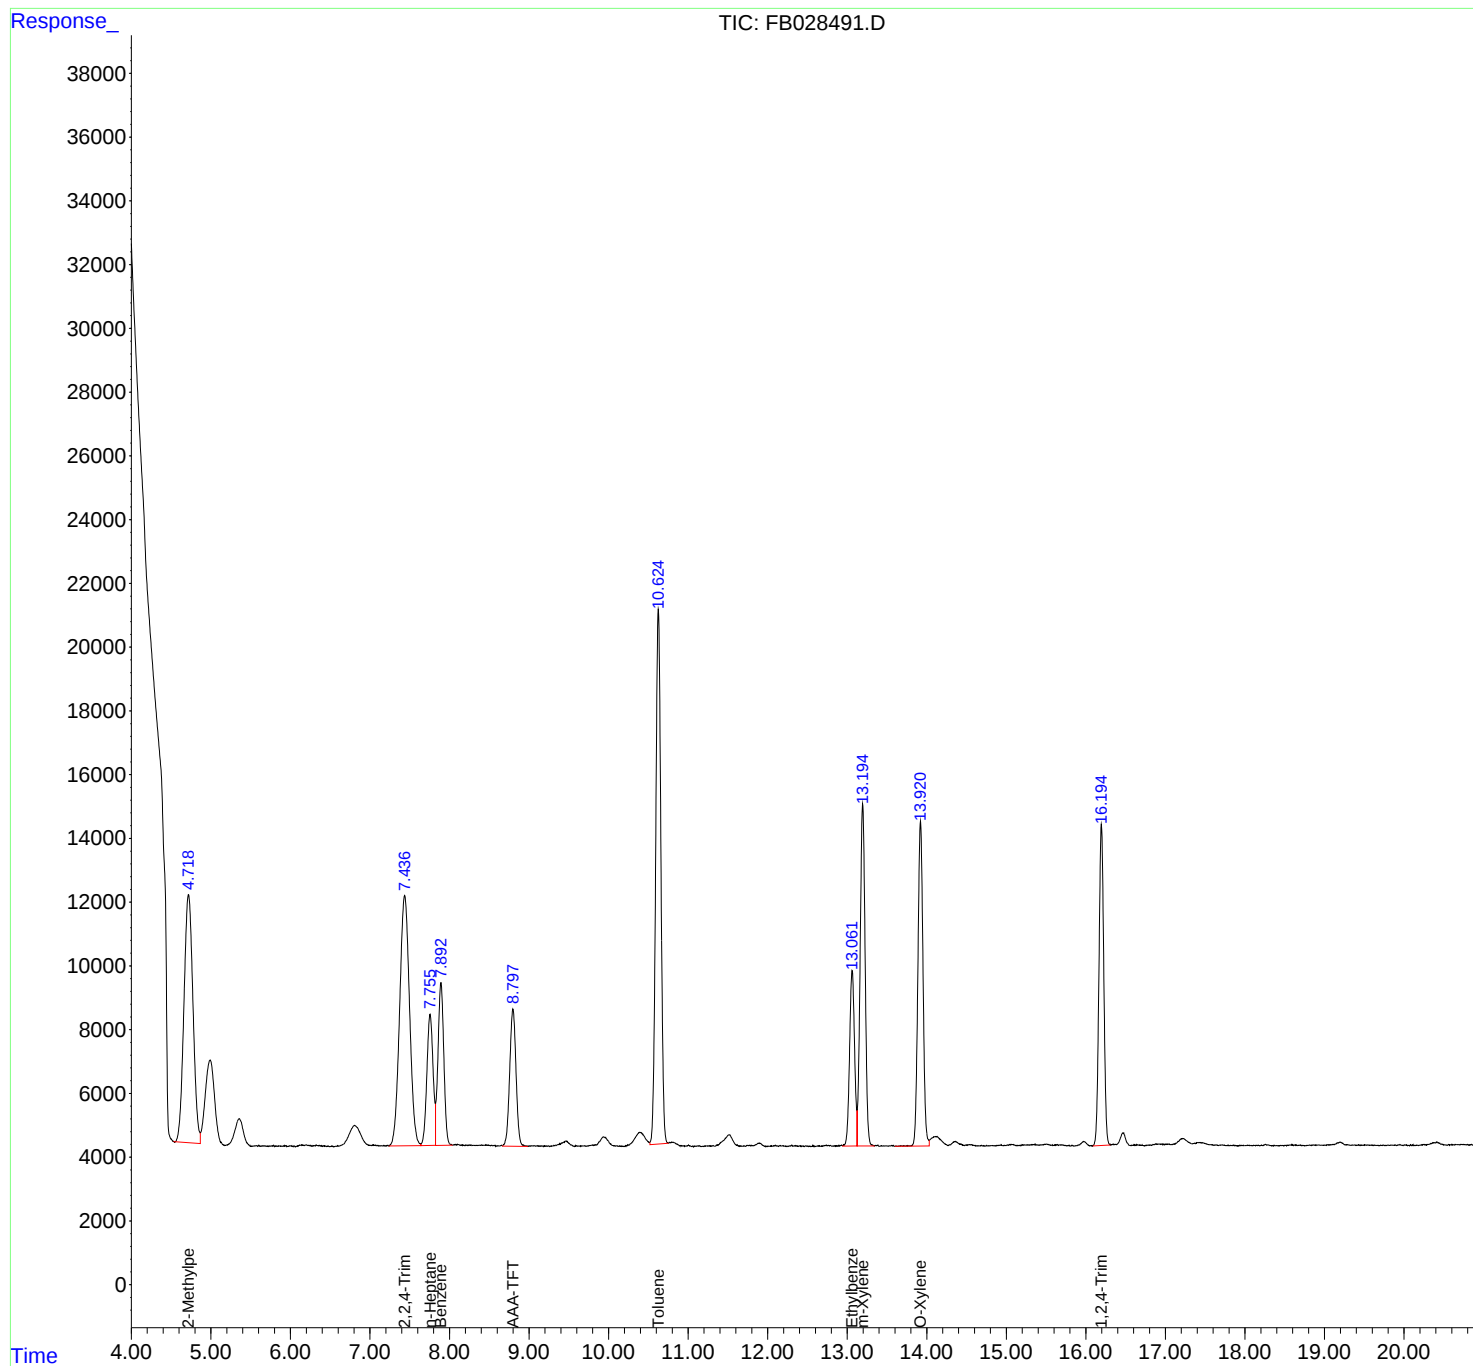


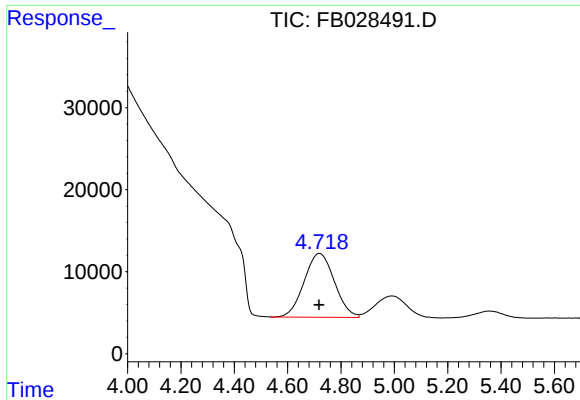

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 612643
Conc: 30.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S2

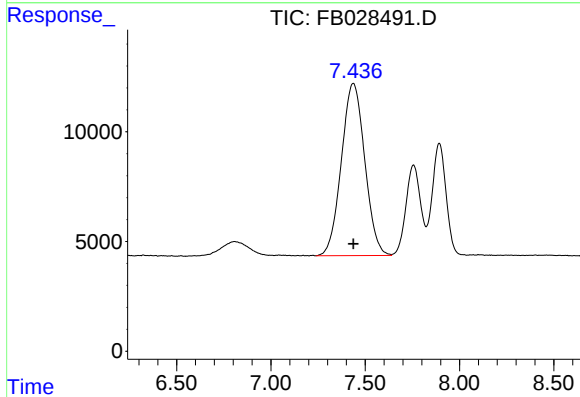


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.000 min
Response: 677005
Conc: 32.18 ng/ml

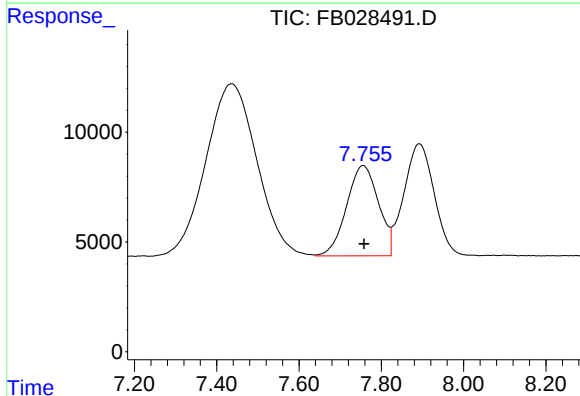


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 222033
Conc: 10.33 ng/ml

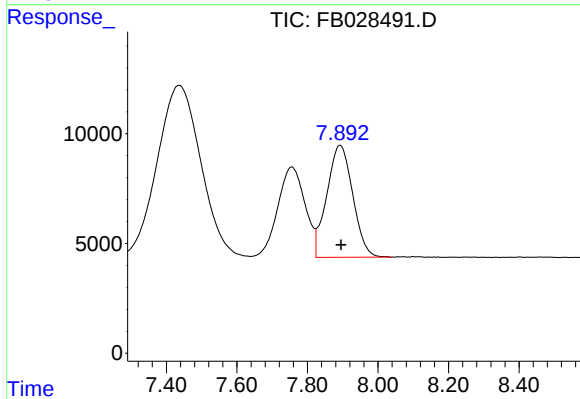

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 261103
Conc: 10.61 ng/ml

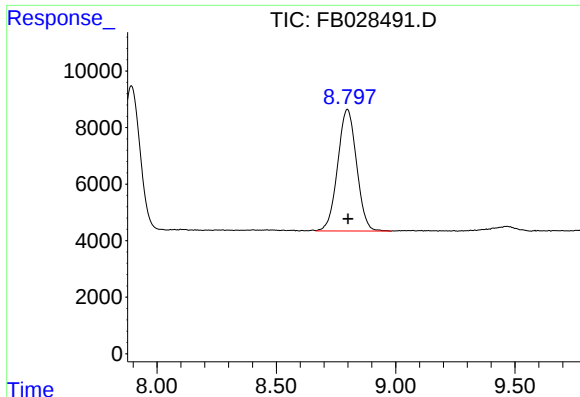

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 236737
Conc: 19.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S2

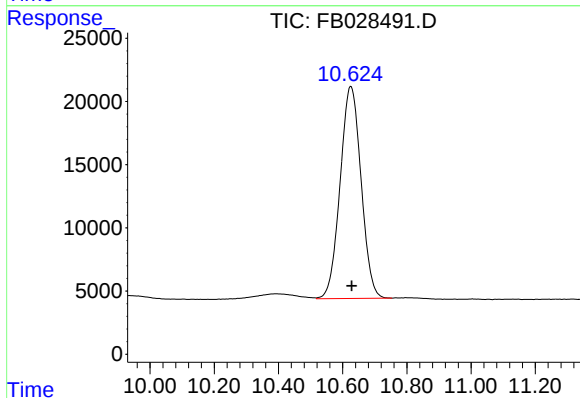


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.002 min
Response: 759817
Conc: 32.64 ng/ml

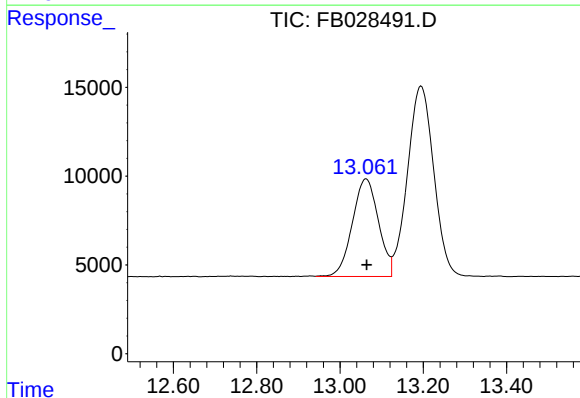


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.002 min
Response: 239123
Conc: 10.75 ng/ml

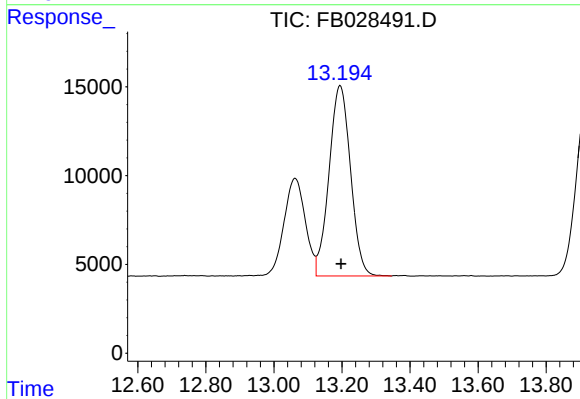

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 469725
Conc: 21.52 ng/ml

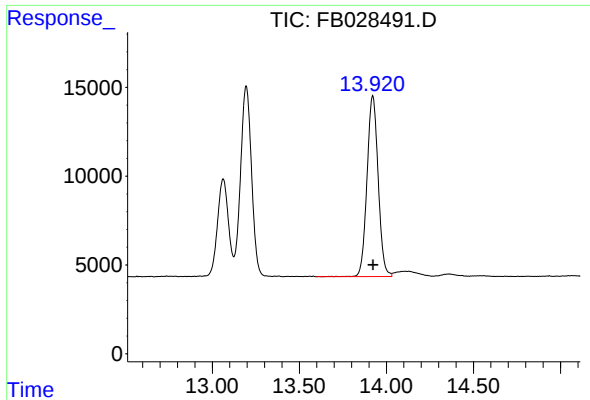

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 452505
Conc: 21.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0929S2

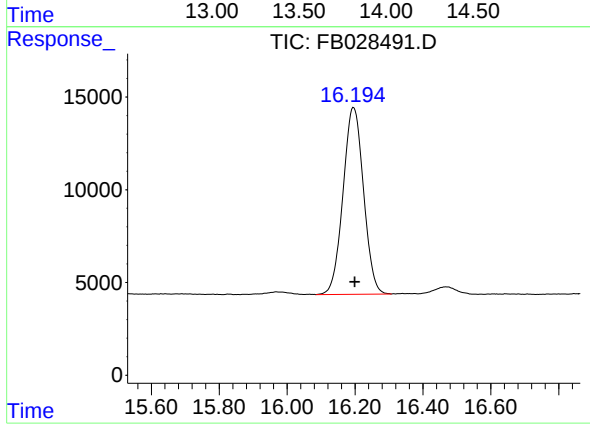

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.003 min
Response: 422372
Conc: 21.01 ng/ml