

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093019\
 Data File : FB022645.D
 Signal(s) : FID2B.CH
 Acq On : 30 Sep 2019 19:48
 Operator : DD/AJ
 Sample : K5079-02MS
 Misc : 5.02g/5.00ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-1-1MS

Integration File: Calibration.e
 Quant Time: Oct 01 01:25:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.966	549515	18.892 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.831	1010999	20.577 ng/ml
2) t 2,2,4-Trimethylpentane	7.583	1156755	22.401 ng/ml
3) t n-Heptane	7.923	368288	7.317 ng/ml
4) t Benzene	8.058	472817	7.967 ng/ml
6) t Toluene	10.807	1389252	29.202 ng/ml
7) t Ethylbenzene	13.253	443373	14.789 ng/ml
8) t m-Xylene	13.386	882650	33.224 ng/ml
9) t O-Xylene	14.116	843626	34.774 ng/ml
10) t 1,2,4-Trimethylbenzene	16.397	592018	22.708 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093019\
Data File : FB022645.D
Signal(s) : FID2B.CH
Acq On : 30 Sep 2019 19:48
Operator : DD/AJ
Sample : K5079-02MS
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-1-1MS

Integration File: Calibration.e
Quant Time: Oct 01 01:25:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

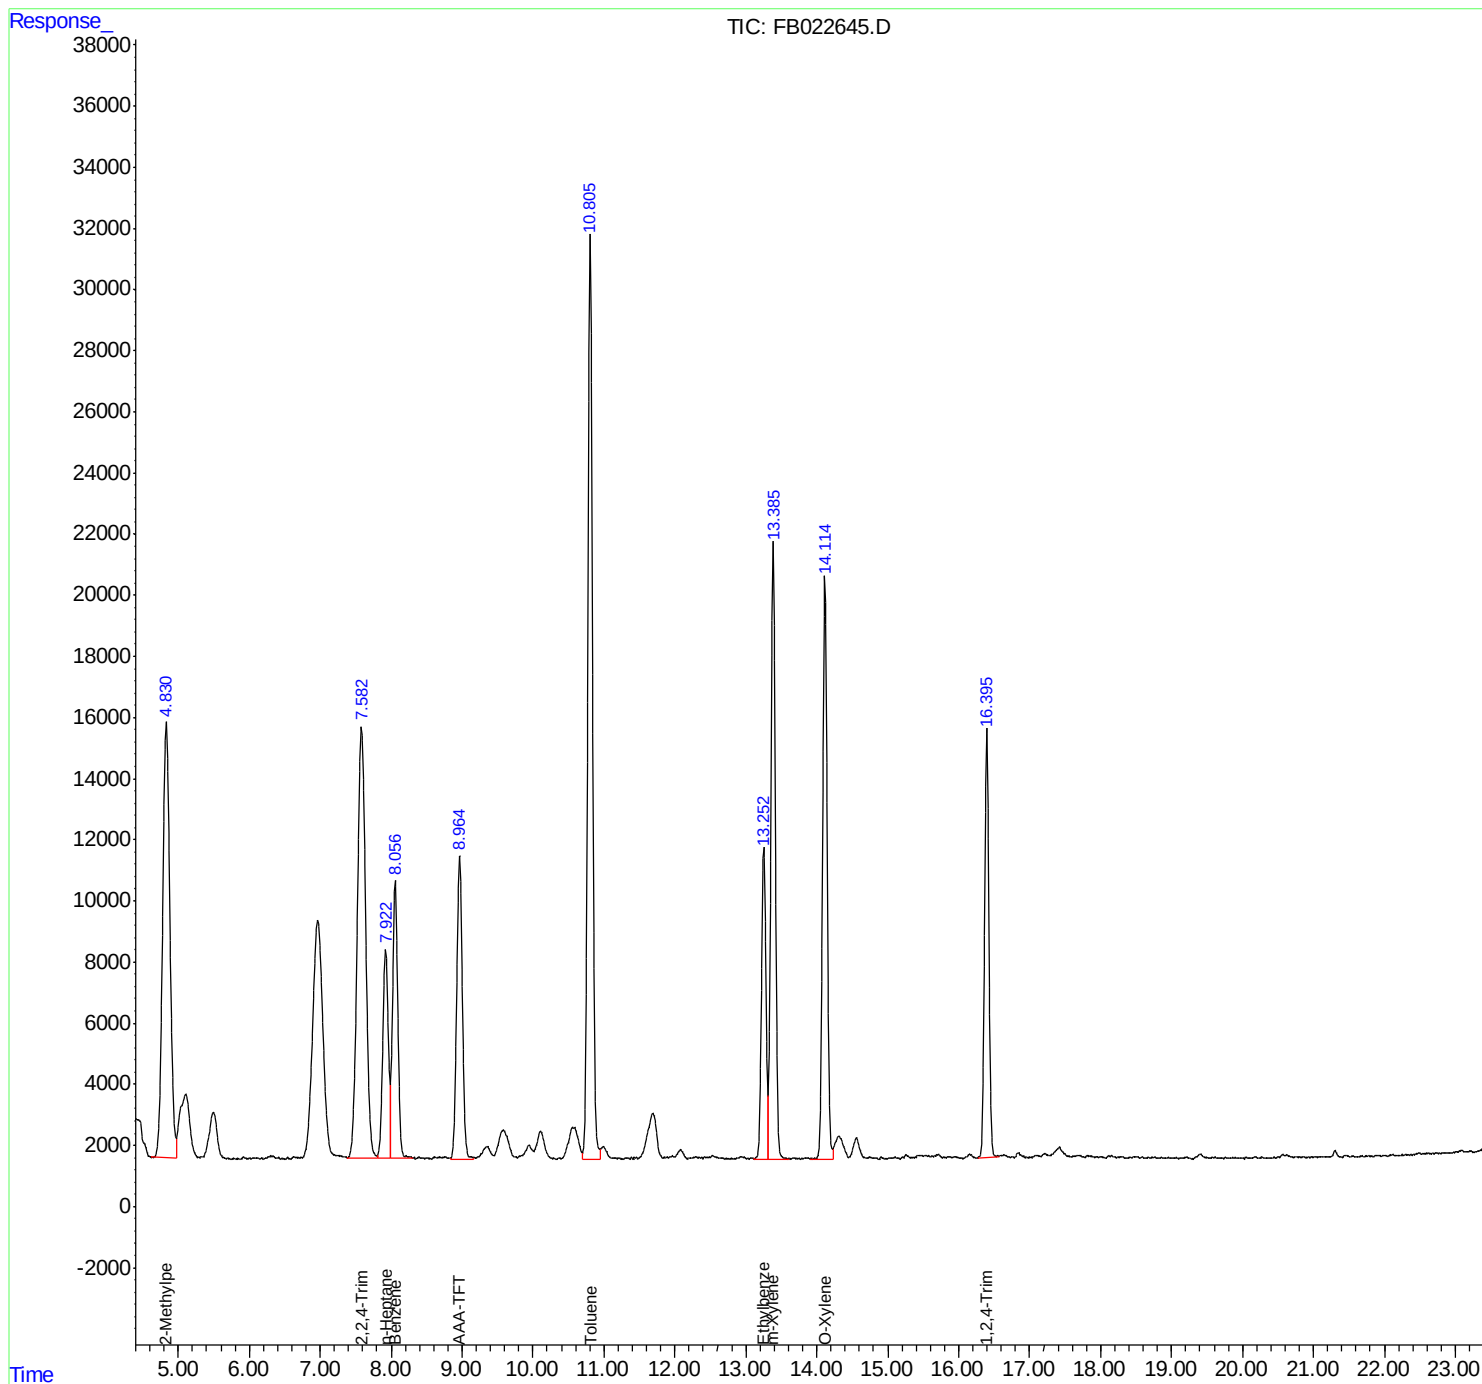


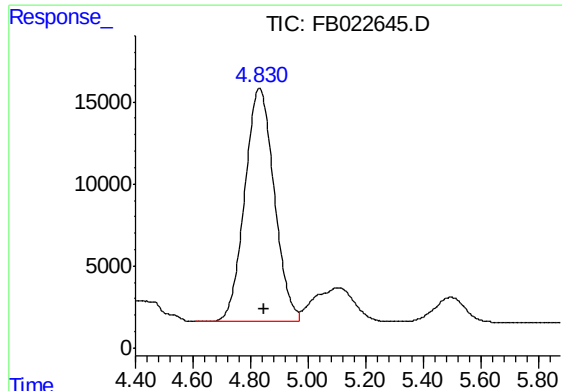

#1 2-Methylpentane


R.T.: 4.831 min
Delta R.T.: -0.016 min
Response: 1010999
Conc: 20.58 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1-1MS

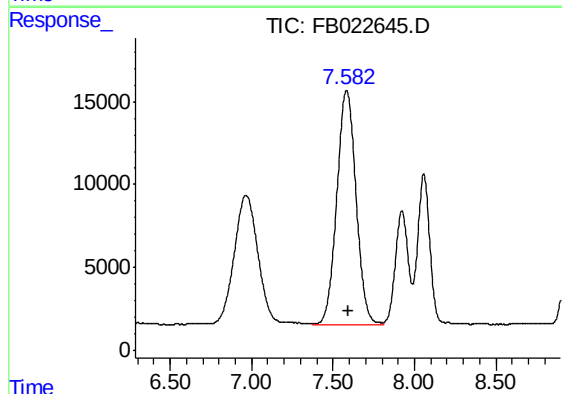


#2 2,2,4-Trimethylpentane

R.T.: 7.583 min
Delta R.T.: -0.014 min
Response: 1156755
Conc: 22.40 ng/ml

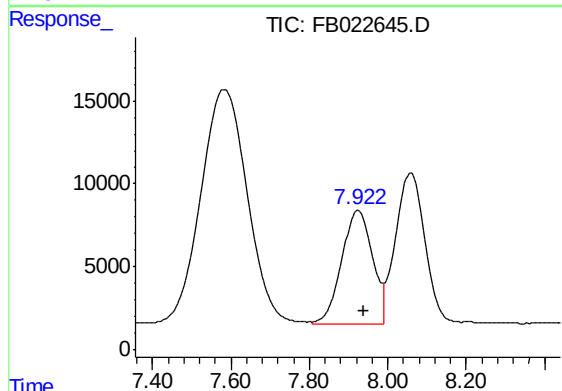


#3 n-Heptane

R.T.: 7.923 min
Delta R.T.: -0.014 min
Response: 368288
Conc: 7.32 ng/ml

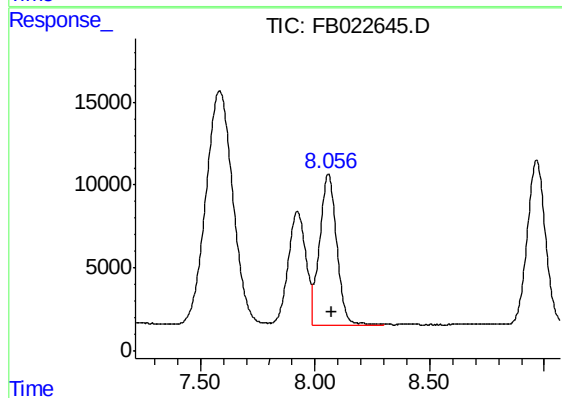

#4 Benzene


R.T.: 8.058 min
Delta R.T.: -0.014 min
Response: 472817
Conc: 7.97 ng/ml

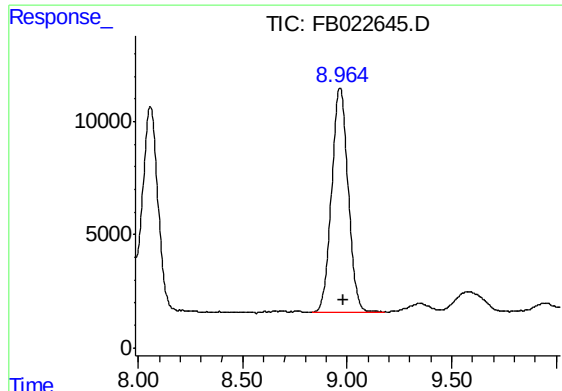

#5 AAA-TFT


R.T.: 8.966 min
Delta R.T.: -0.014 min
Response: 549515
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1-1MS

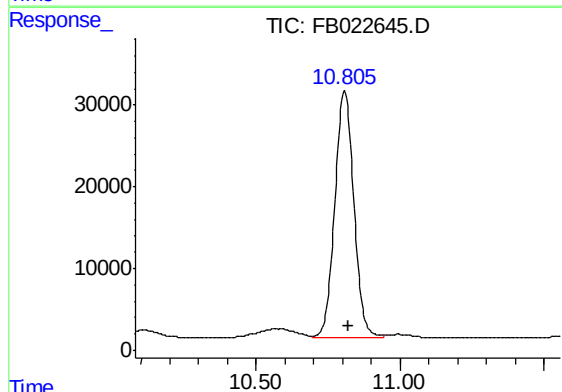


#6 Toluene

R.T.: 10.807 min
Delta R.T.: -0.013 min
Response: 1389252
Conc: 29.20 ng/ml

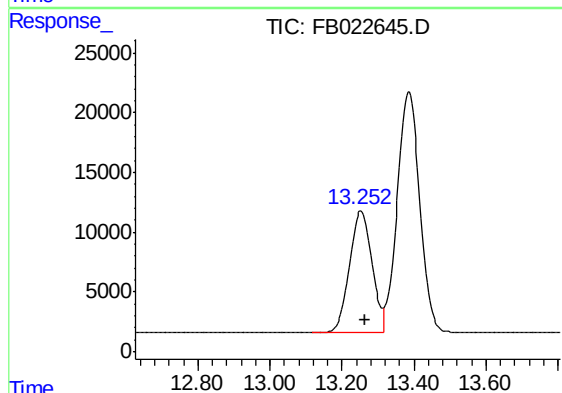


#7 Ethylbenzene

R.T.: 13.253 min
Delta R.T.: -0.012 min
Response: 443373
Conc: 14.79 ng/ml

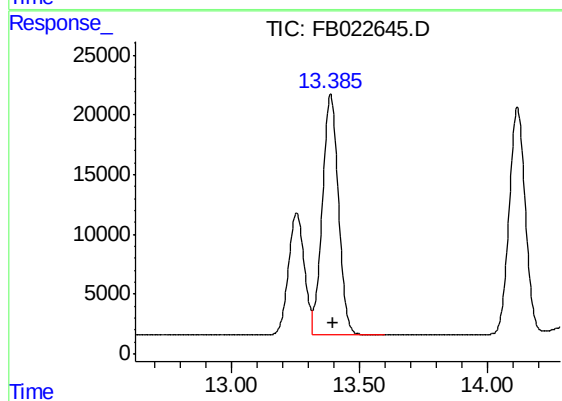

#8 m-Xylene


R.T.: 13.386 min
Delta R.T.: -0.012 min
Response: 882650
Conc: 33.22 ng/ml

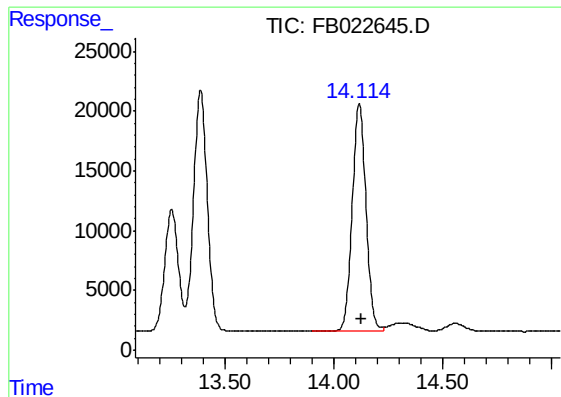

#9 O-Xylene

R.T.: 14.116 min
Delta R.T.: -0.012 min
Response: 843626
Conc: 34.77 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1-1MS

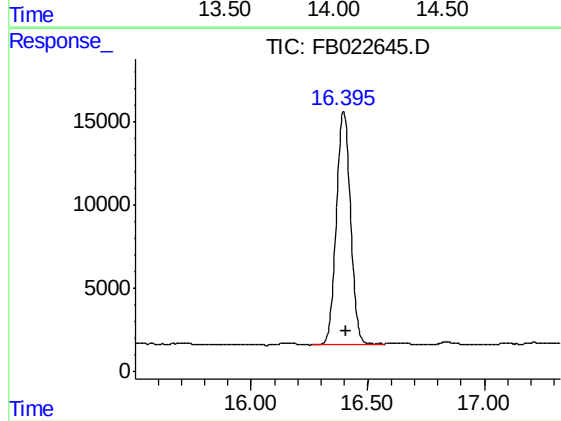

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min
Delta R.T.: -0.011 min
Response: 592018
Conc: 22.71 ng/ml