

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093019\
 Data File : FB022646.D
 Signal(s) : FID2B.CH
 Acq On : 30 Sep 2019 20:17
 Operator : DD/AJ
 Sample : K5079-02MSD
 Misc : 5.04g/5.00ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-1-1MSD

Integration File: Calibration.e
 Quant Time: Oct 01 01:25:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.966	559954	19.251 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.832	977287	19.891 ng/ml
2) t 2,2,4-Trimethylpentane	7.583	1141615	22.108 ng/ml
3) t n-Heptane	7.923	364564	7.243 ng/ml
4) t Benzene	8.058	469803	7.916 ng/ml
6) t Toluene	10.806	1378268	28.972 ng/ml
7) t Ethylbenzene	13.253	439020	14.644 ng/ml
8) t m-Xylene	13.386	870403	32.763 ng/ml
9) t O-Xylene	14.115	829578	34.195 ng/ml
10) t 1,2,4-Trimethylbenzene	16.396	580781	22.277 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093019\
Data File : FB022646.D
Signal(s) : FID2B.CH
Acq On : 30 Sep 2019 20:17
Operator : DD/AJ
Sample : K5079-02MSD
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-1-1MSD

Integration File: Calibration.e
Quant Time: Oct 01 01:25:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

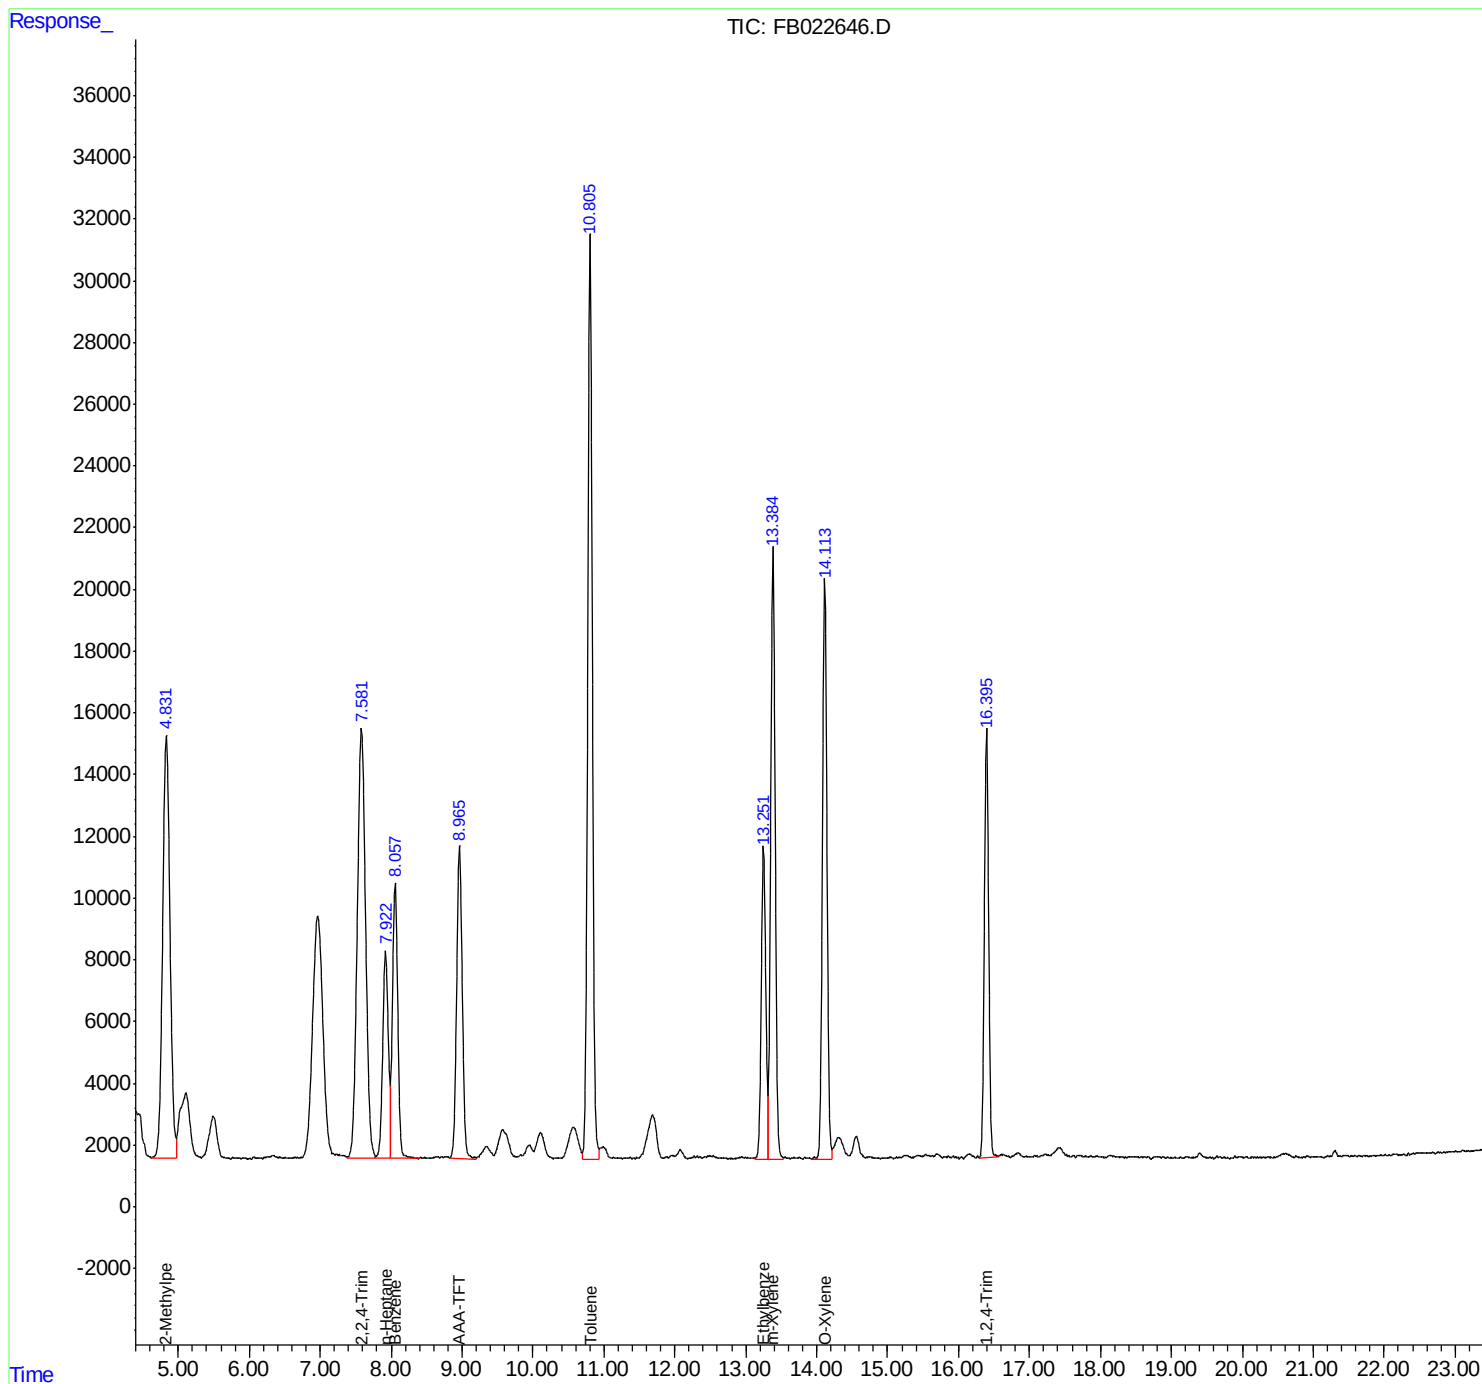


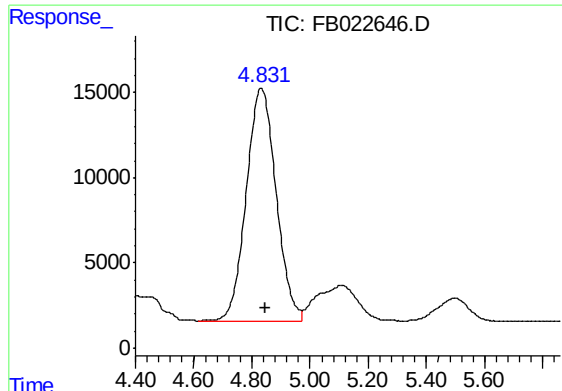

#1 2-Methylpentane


R.T.: 4.832 min
Delta R.T.: -0.015 min
Response: 977287
Conc: 19.89 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1-1MSD

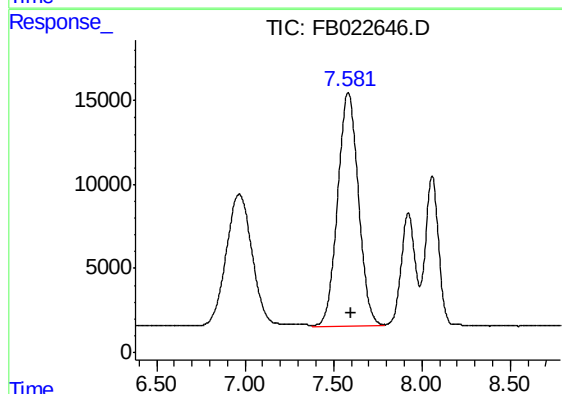


#2 2,2,4-Trimethylpentane

R.T.: 7.583 min
Delta R.T.: -0.015 min
Response: 1141615
Conc: 22.11 ng/ml

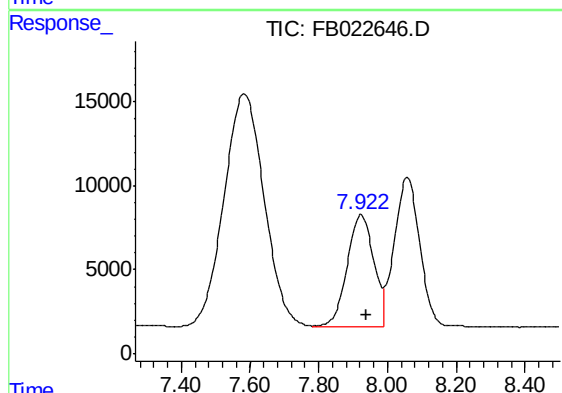


#3 n-Heptane

R.T.: 7.923 min
Delta R.T.: -0.014 min
Response: 364564
Conc: 7.24 ng/ml

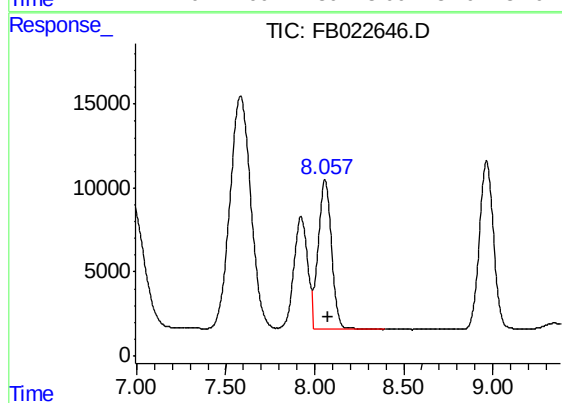

#4 Benzene


R.T.: 8.058 min
Delta R.T.: -0.014 min
Response: 469803
Conc: 7.92 ng/ml

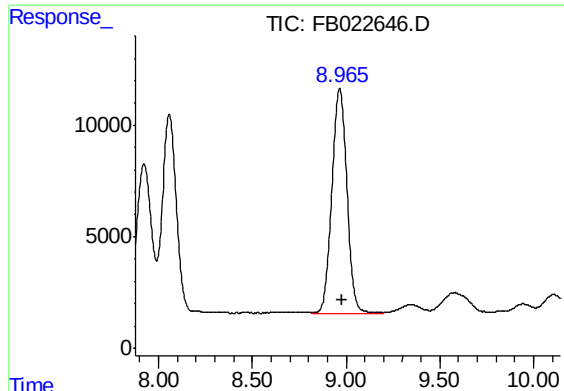

#5 AAA-TFT


R.T.: 8.966 min
Delta R.T.: -0.013 min
Response: 559954
Conc: 19.25 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1-1MSD

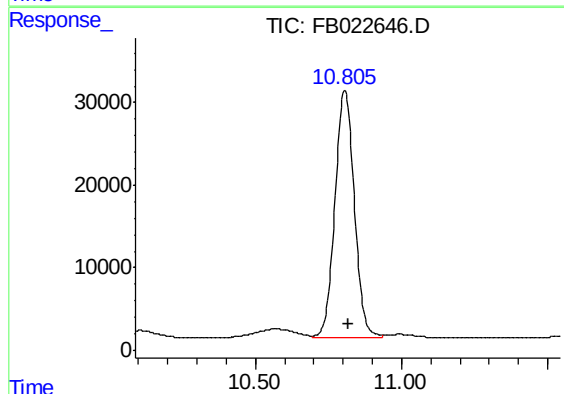


#6 Toluene

R.T.: 10.806 min
Delta R.T.: -0.013 min
Response: 1378268
Conc: 28.97 ng/ml

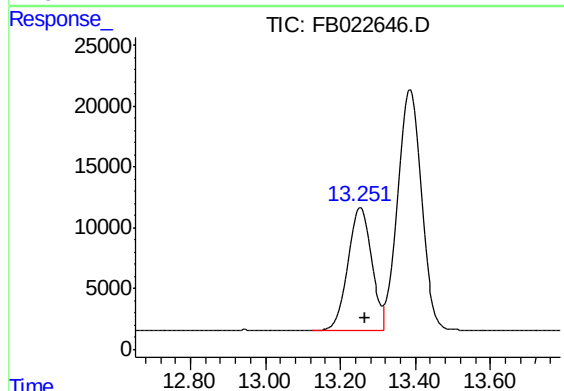


#7 Ethylbenzene

R.T.: 13.253 min
Delta R.T.: -0.013 min
Response: 439020
Conc: 14.64 ng/ml

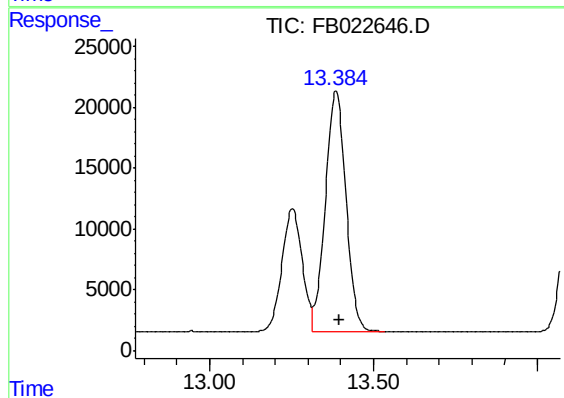

#8 m-Xylene


R.T.: 13.386 min
Delta R.T.: -0.012 min
Response: 870403
Conc: 32.76 ng/ml

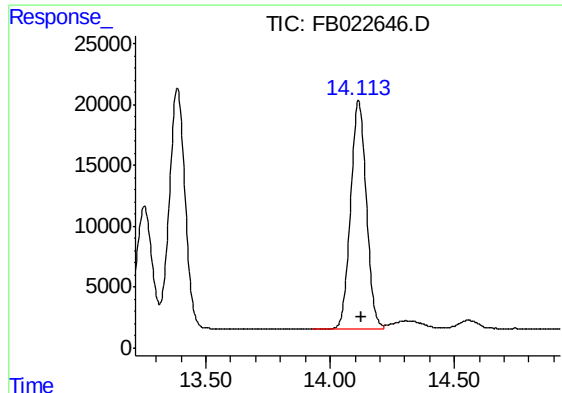

#9 O-Xylene

R.T.: 14.115 min
Delta R.T.: -0.013 min
Response: 829578
Conc: 34.20 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1-1MSD

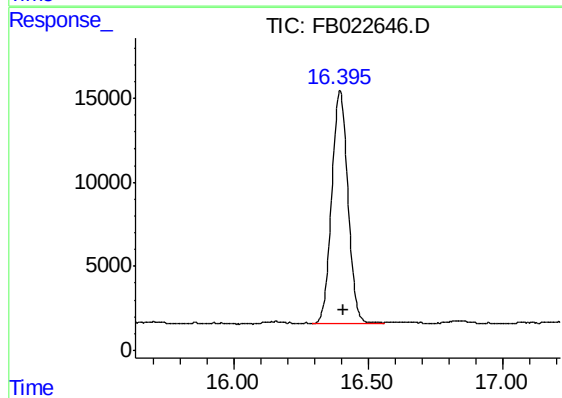

#10 1,2,4-Trimethylbenzene

R.T.: 16.396 min
Delta R.T.: -0.011 min
Response: 580781
Conc: 22.28 ng/ml