

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093020\
 Data File : FB024976.D
 Signal(s) : FID2B.CH
 Acq On : 30 Sep 2020 12:02
 Operator : DD/AJ
 Sample : BSF0930S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 01 01:00:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
 Quant Title :
 QLast Update : Wed Sep 23 11:20:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	379673	18.085 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	803767	26.727 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	853433	27.923 ng/ml
3) t n-Heptane	7.757	282183	9.276 ng/ml
4) t Benzene	7.892	341067	9.156 ng/ml
6) t Toluene	10.631	964448	27.627 ng/ml
7) t Ethylbenzene	13.071	300565	9.272 ng/ml
8) t m-Xylene	13.204	591919	18.634 ng/ml
9) t O-Xylene	13.931	572610	18.844 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	477830	18.840 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB093020\
Data File : FB024976.D
Signal(s) : FID2B.CH
Acq On : 30 Sep 2020 12:02
Operator : DD/AJ
Sample : BSF0930S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 01 01:00:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092320.M
Quant Title :
QLast Update : Wed Sep 23 11:20:20 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

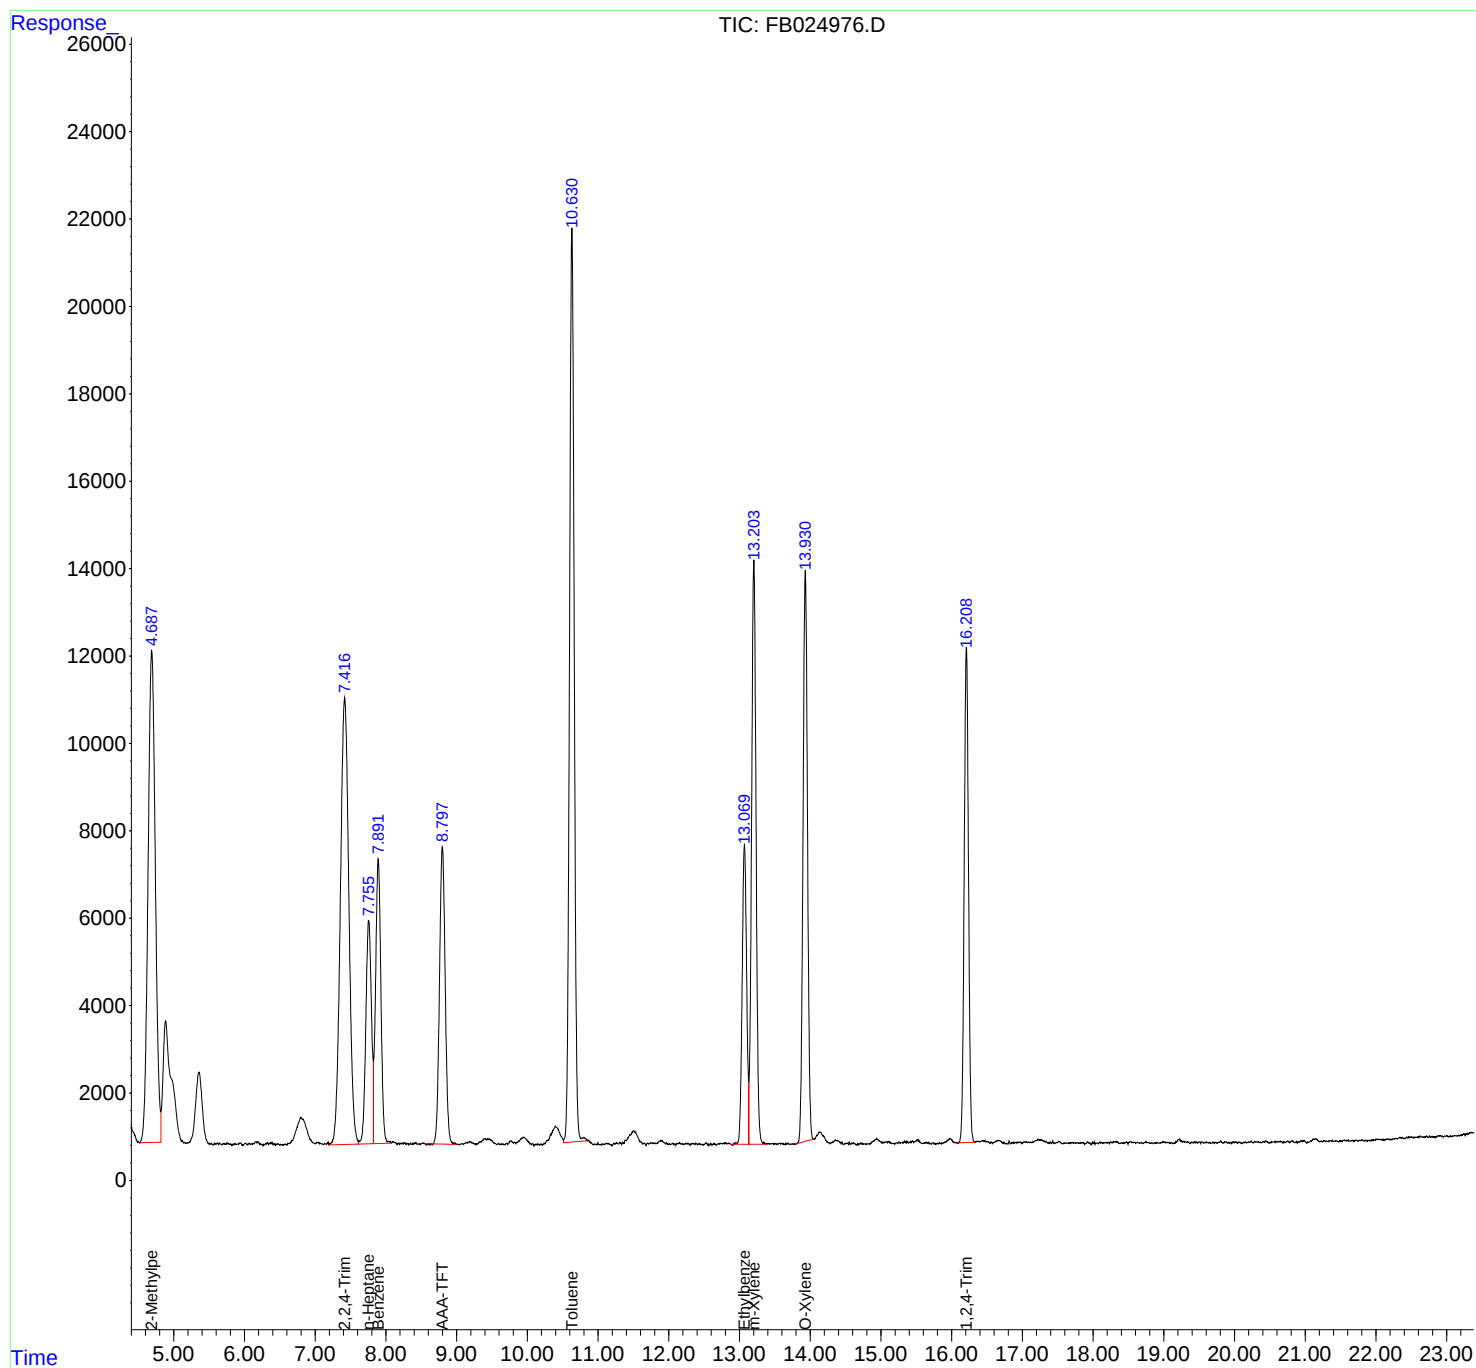

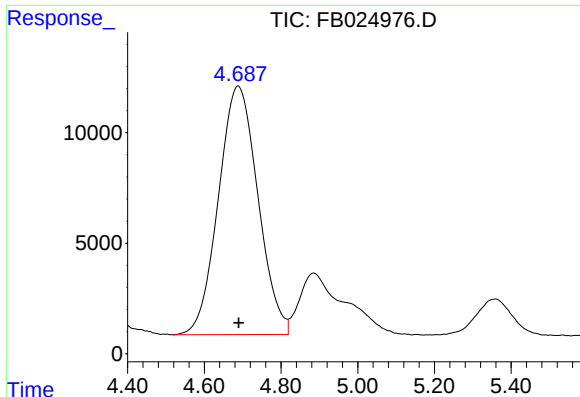


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.001 min
Response: 803767
Conc: 26.73 ng/ml

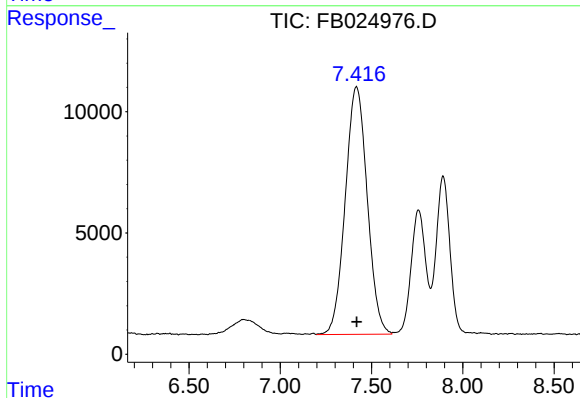


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 853433
Conc: 27.92 ng/ml

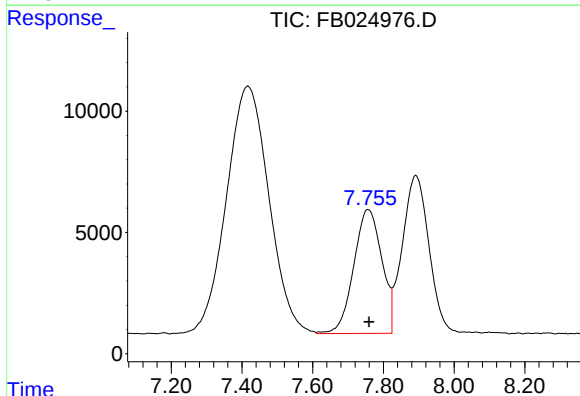


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 282183
Conc: 9.28 ng/ml

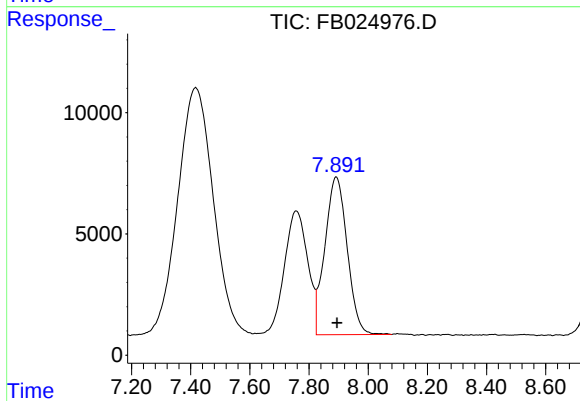


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 341067
Conc: 9.16 ng/ml

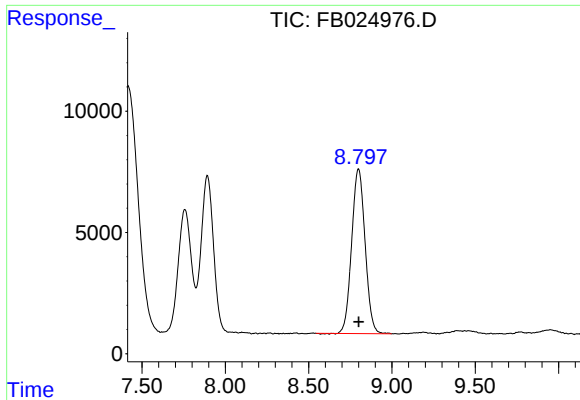


#5 AAA-TFT

R.T.: 8.799 min
 Delta R.T.: -0.002 min
 Response: 379673
 Conc: 18.08 ng/ml

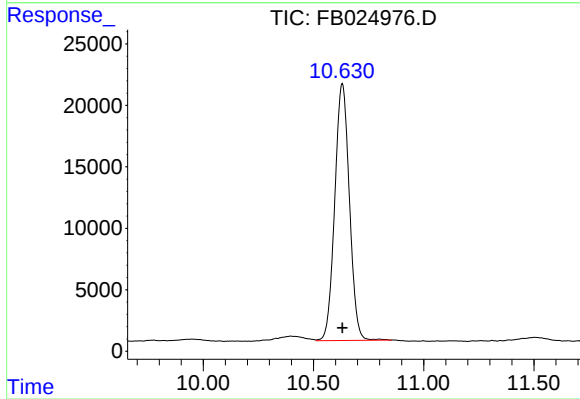


#6 Toluene

R.T.: 10.631 min
 Delta R.T.: 0.000 min
 Response: 964448
 Conc: 27.63 ng/ml

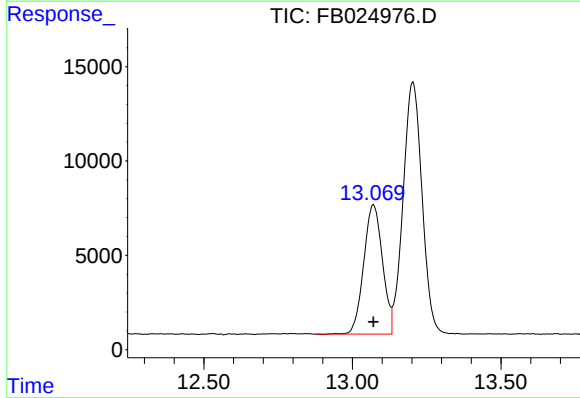


#7 Ethylbenzene

R.T.: 13.071 min
 Delta R.T.: 0.000 min
 Response: 300565
 Conc: 9.27 ng/ml

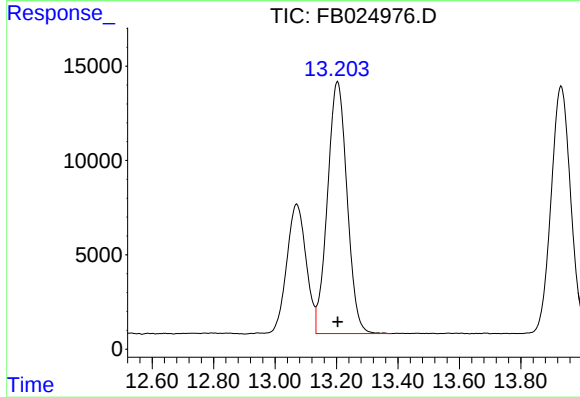


#8 m-Xylene

R.T.: 13.204 min
 Delta R.T.: 0.000 min
 Response: 591919
 Conc: 18.63 ng/ml

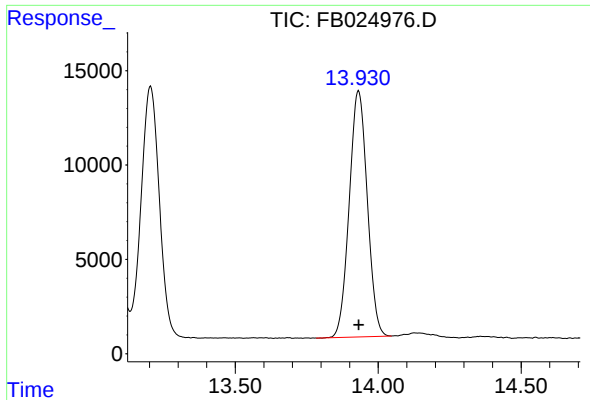

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 572610
Conc: 18.84 ng/ml

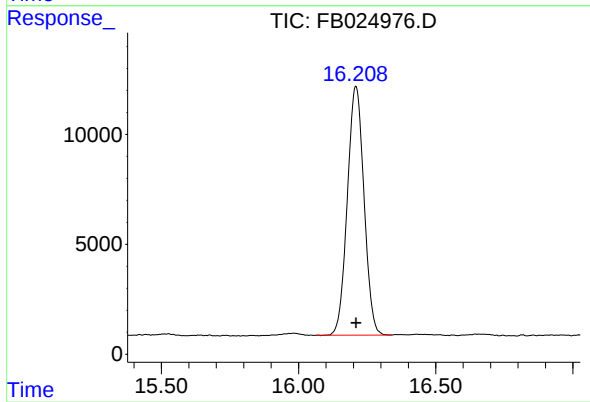

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 477830
Conc: 18.84 ng/ml